
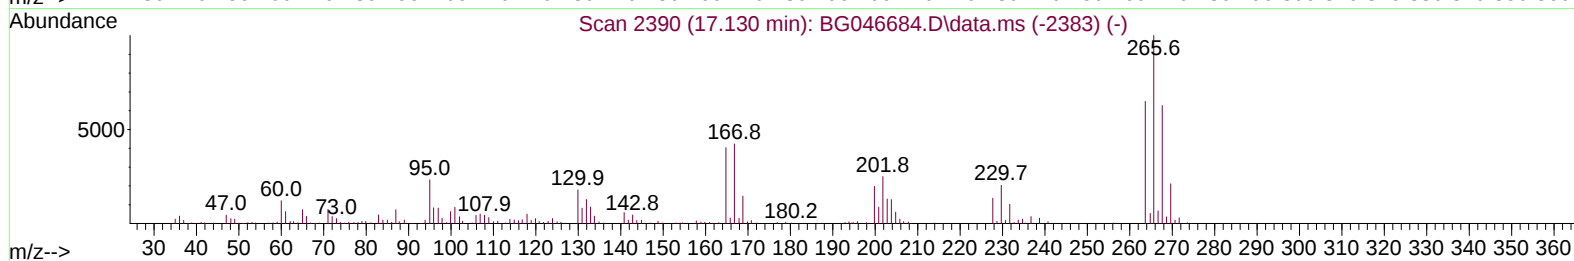
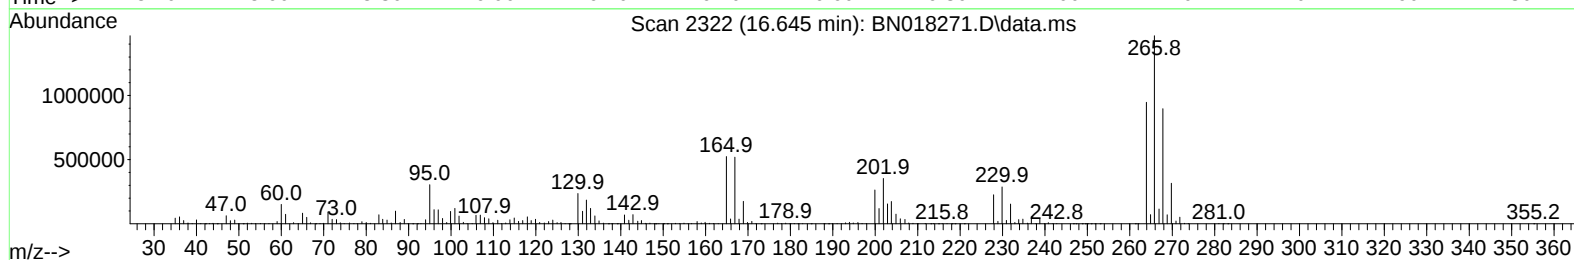


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122921\
Data File : BN018271.D
Acq On : 29 Dec 2021 21:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 05:14:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 05:13:58 2021
Response via : Initial Calibration

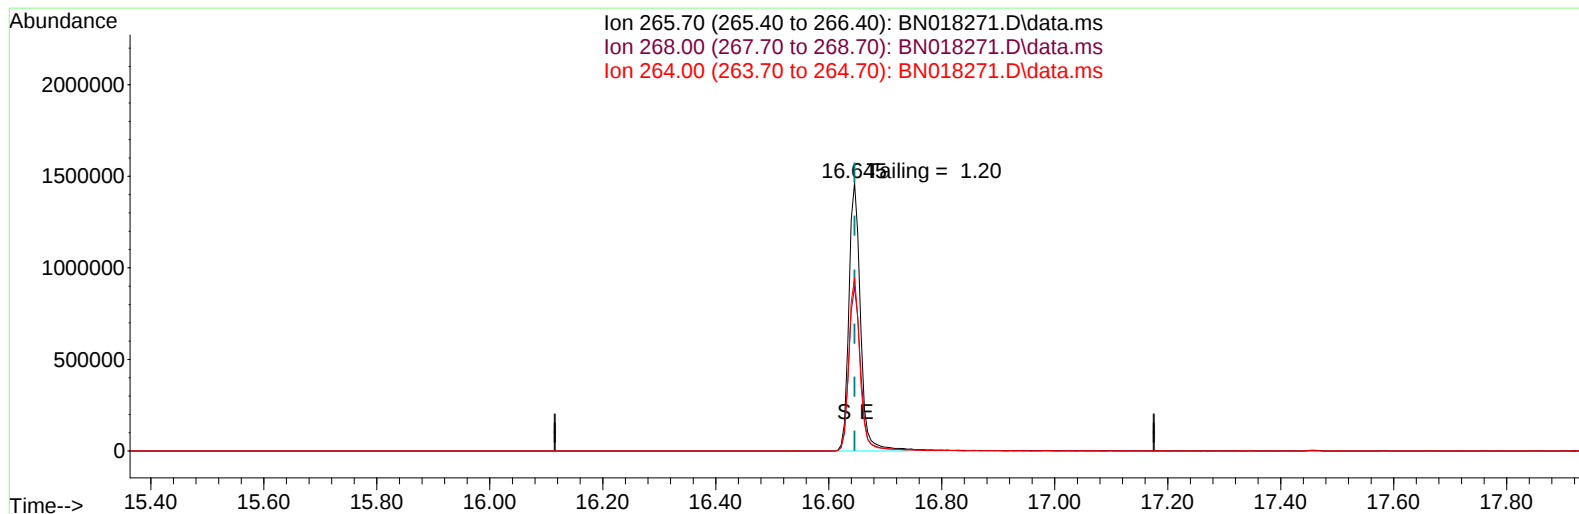

TIC: BN018271.D\data.ms

(70) Pentachlorophenol (C)




16.645min (0.000) 661830.60 ng

response 2119103

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.24
264.00	61.60	64.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122921\
Data File : BN018271.D
Acq On : 29 Dec 2021 21:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 30 05:14:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 05:13:58 2021
Response via : Initial Calibration

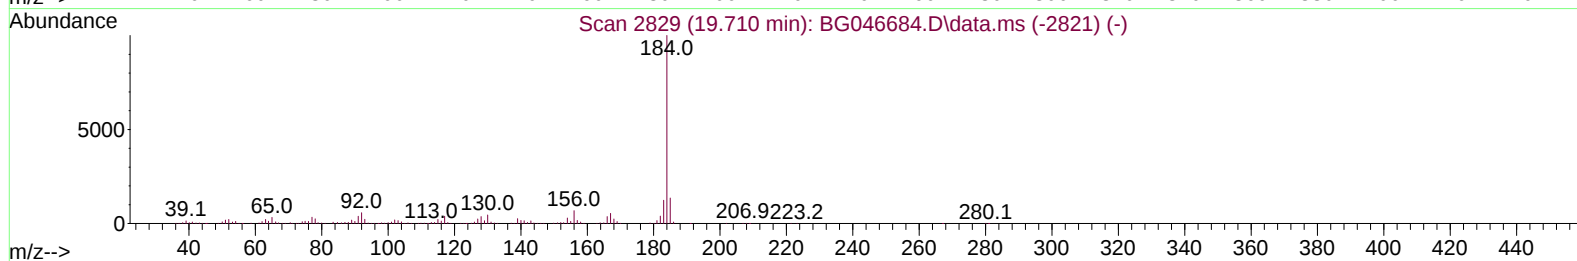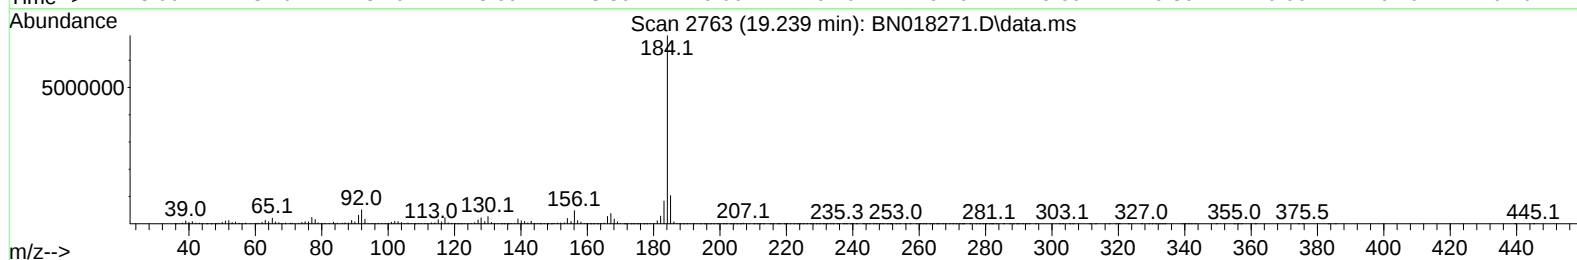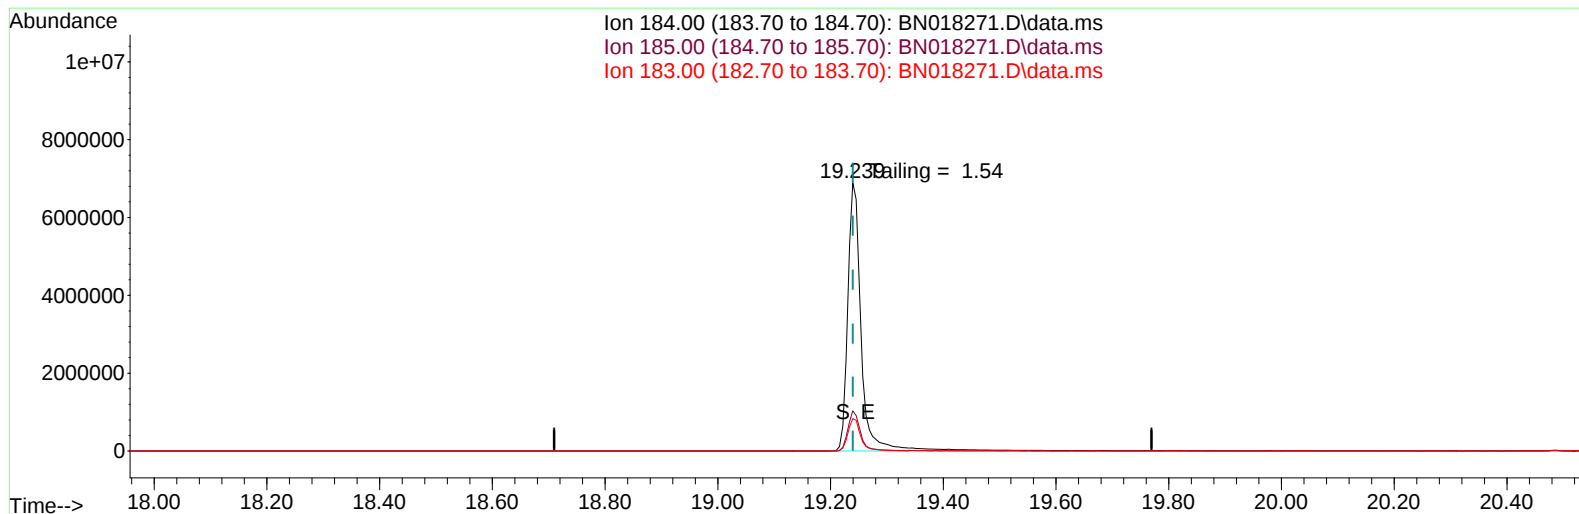

TIC: BN018271.D\data.ms

(77) Benzidine**19.239min (0.000) 910708.05 ng****response 11453749**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.97
183.00	13.20	12.07
0.00	0.00	0.00