


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122921\
 Data File : BN018253.D
 Acq On : 29 Dec 2021 09:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN122921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 29 16:08:47 2021

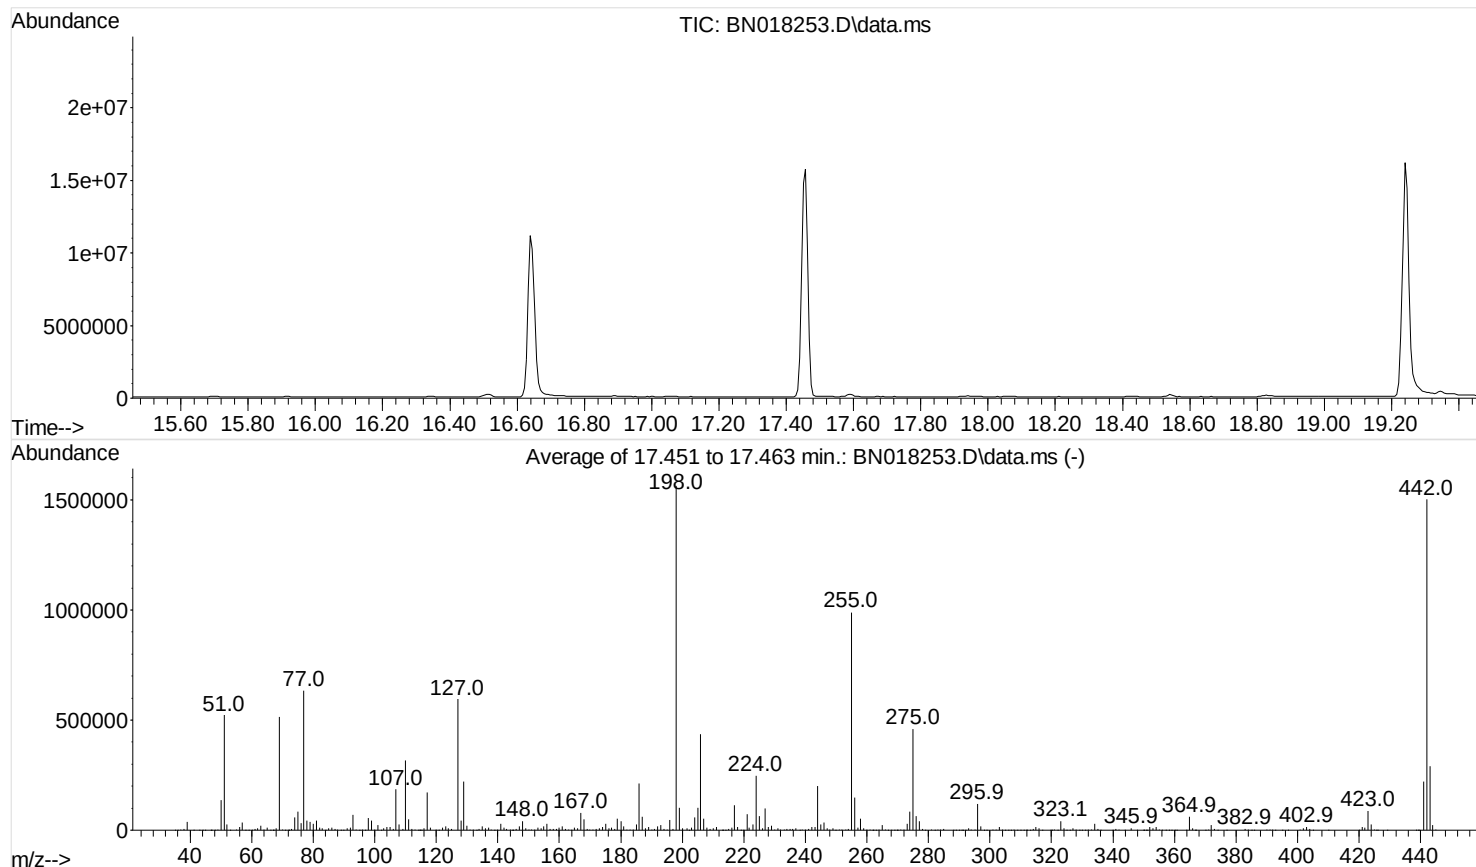




AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2451

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	33.4	521930	PASS
68	69	0.00	2	1.9	9694	PASS
69	198	0.00	100	33.0	515349	PASS
70	69	0.00	2	0.5	2812	PASS
127	198	10	80	38.0	594688	PASS
197	198	0.00	2	0.5	7152	PASS
198	198	100	100	100.0	1563819	PASS
199	198	5	9	6.6	102475	PASS
275	198	10	60	29.4	459648	PASS
365	198	1	100	3.8	59947	PASS
441	198	0.01	100	14.1	220245	PASS
442	442	50	100	100.0	1502208	PASS
443	442	15	24	19.3	289600	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122921\
 Data File : BN018253.D
 Acq On : 29 Dec 2021 09:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 31 04:57:15 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 30 05:13:58 2021
 Response via : Initial Calibration

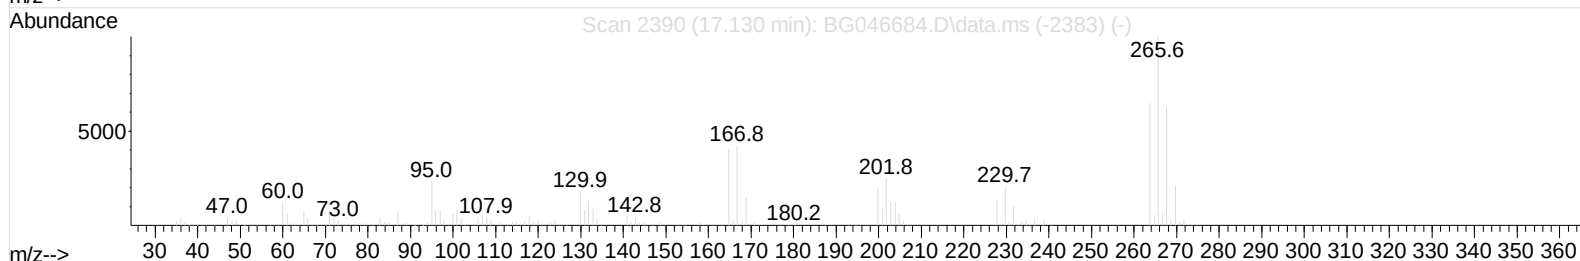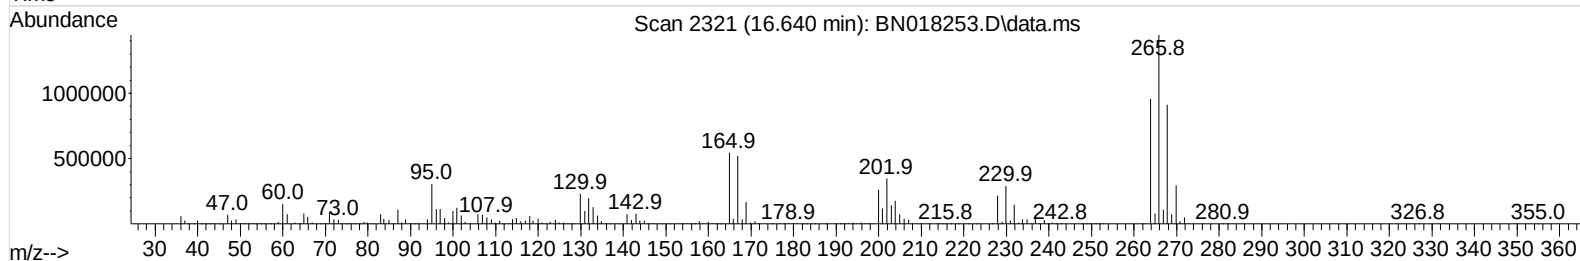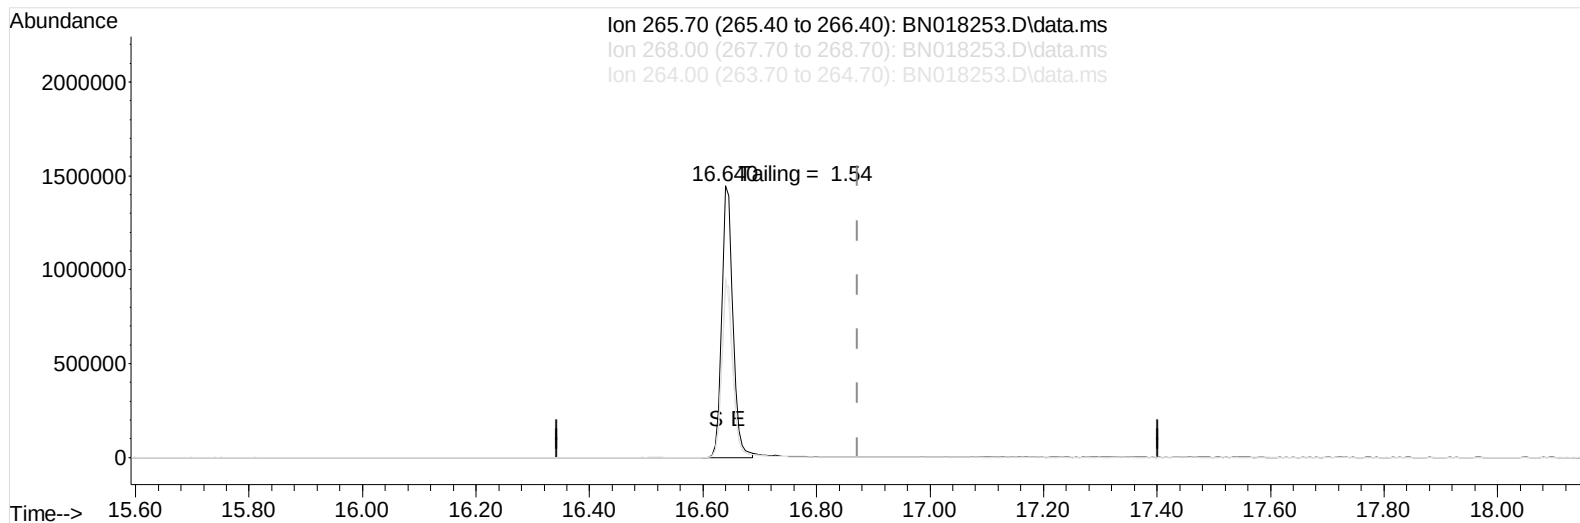

TIC: BN018253.D\data.ms

(70) Pentachlorophenol (C)

16.640min (-0.232) 23150.66 ng

response 2020106

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.12
264.00	61.60	66.07
0.00	0.00	0.00

Instrument :
BNA_N
ClientSampleId :
DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/29/2021	BNA_N	<u>BN018253.D</u>
Compound Name	Response	Retention Time
DDT	6044514	20.48
DDD	166462	20.04
DDE	15317	19.53
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
181779	6226293	2.92

Instrument :
BNA_N
ClientSampleId :
DFTPP