
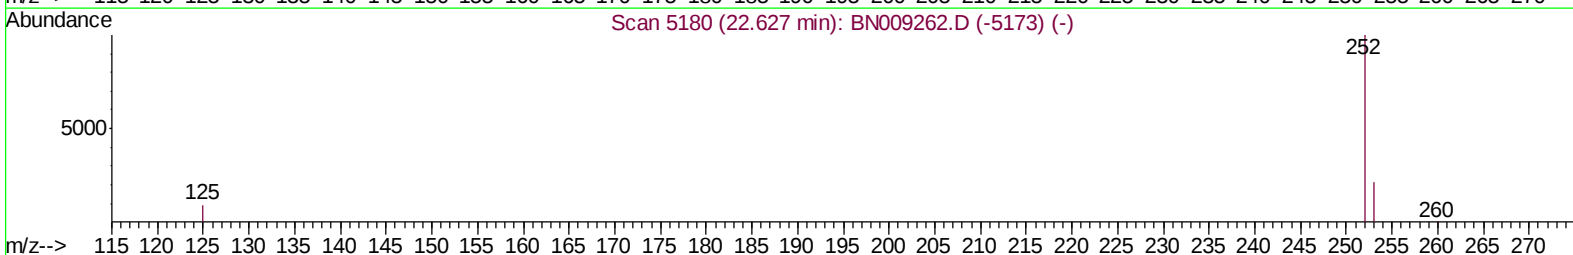
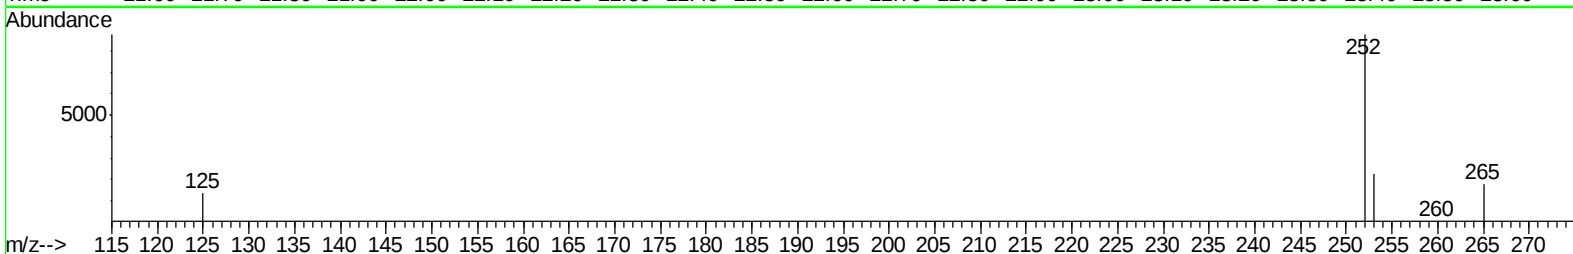


Data File : BN009264.D
Acq On : 30 Dec 2019 17:43
Operator : JU
Sample : K6322-03DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Dec 31 01:03:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 00:59:26 2019
Response via : Initial Calibration

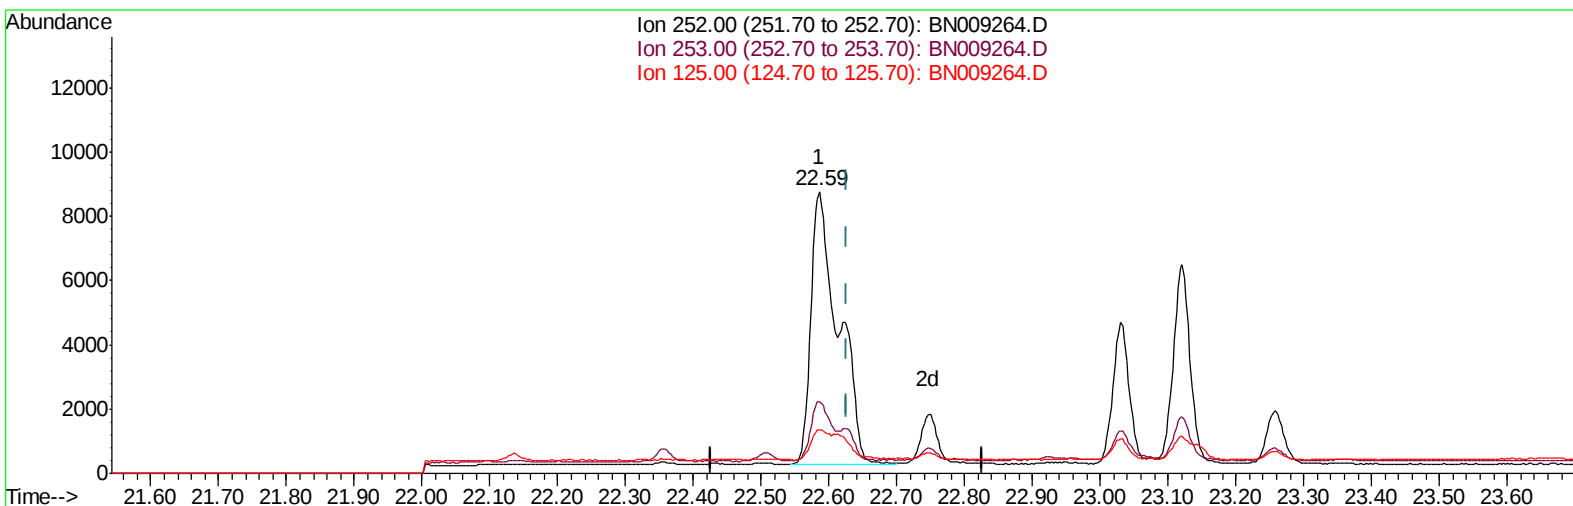

TIC: BN009264.D

(22) Benzo(k)fluoranthene
22.586min (-0.041) 0.76ng/ul
response 23877

Ion	Exp%	Act%
252.00	100	100
253.00	24.20	25.60
125.00	15.50	15.42
0.00	0.00	0.00