
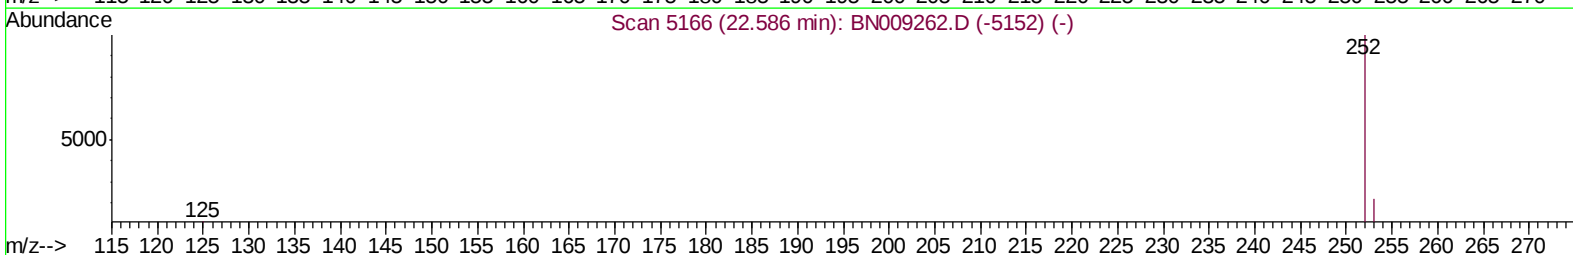
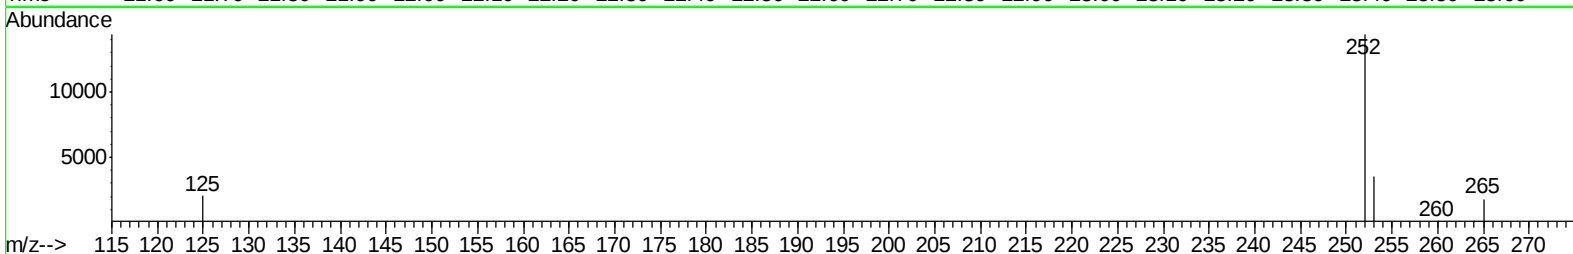


Data File : BN009266.D  
Acq On : 30 Dec 2019 18:55  
Operator : JU  
Sample : K6322-05DL 2X  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Dec 31 01:03:52 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN121619.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Dec 31 00:59:26 2019  
Response via : Initial Calibration

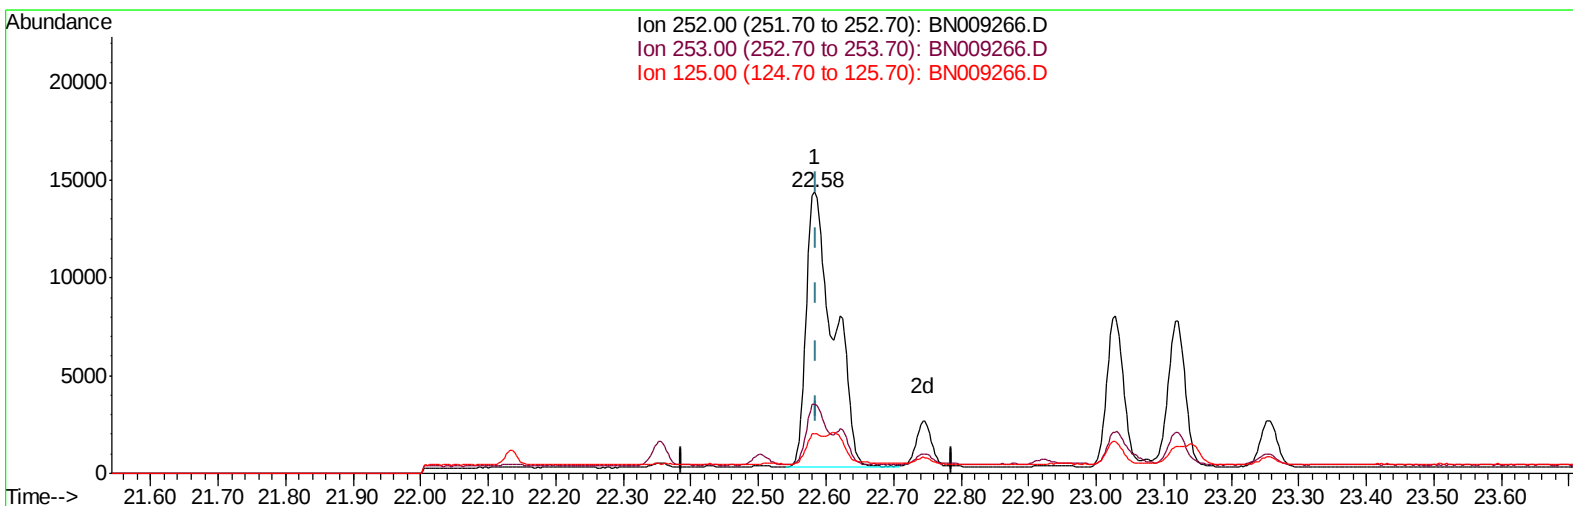

TIC: BN009266.D

(21) Benzo(b)fluoranthene  
22.583min (-0.003) 1.22ng/ul  
response 39648

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 252.00 | 100   | 100   |
| 253.00 | 24.10 | 24.60 |
| 125.00 | 15.00 | 13.99 |
| 0.00   | 0.00  | 0.00  |