
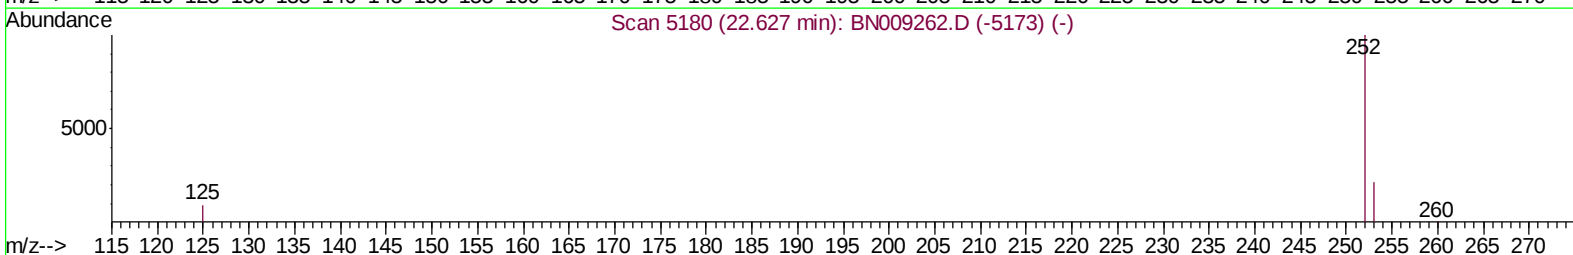
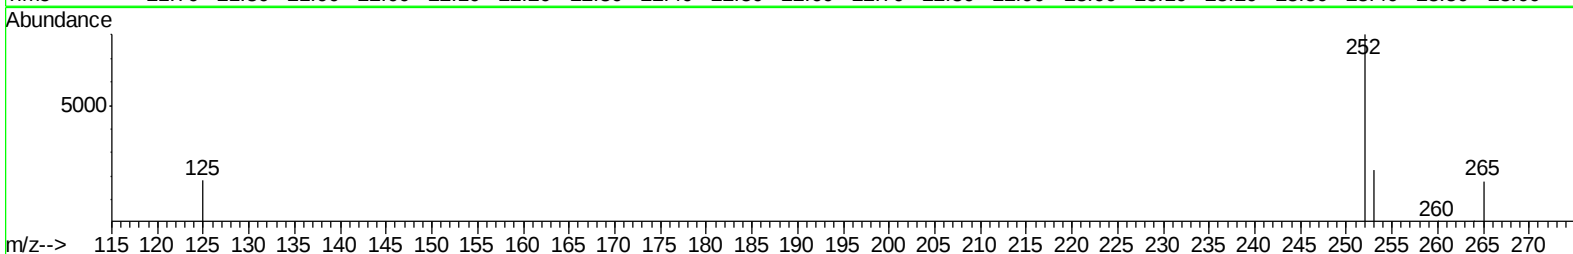


Data File : BN009266.D
Acq On : 30 Dec 2019 18:55
Operator : JU
Sample : K6322-05DL 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Dec 31 01:03:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 00:59:26 2019
Response via : Initial Calibration

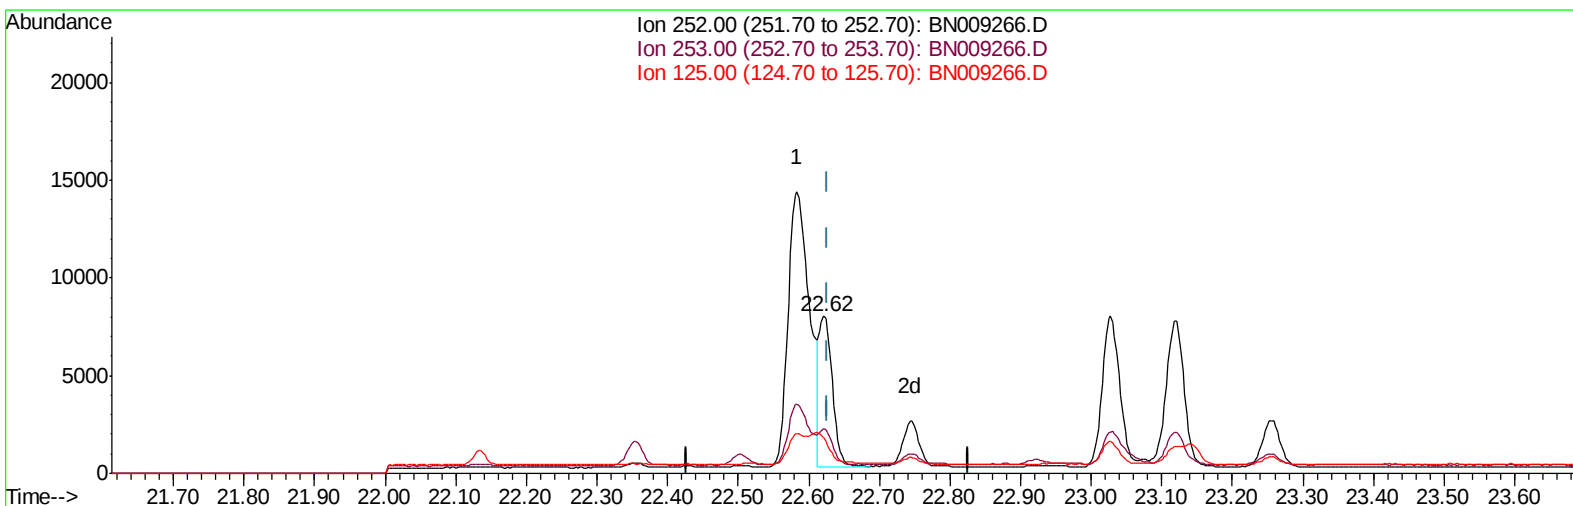

TIC: BN009266.D

(22) Benzo(k)fluoranthene

22.621min (-0.006) 0.30ng/ul m

response 9881

Ion	Exp%	Act%
252.00	100	100
253.00	24.20	28.28
125.00	15.50	22.50#
0.00	0.00	0.00