
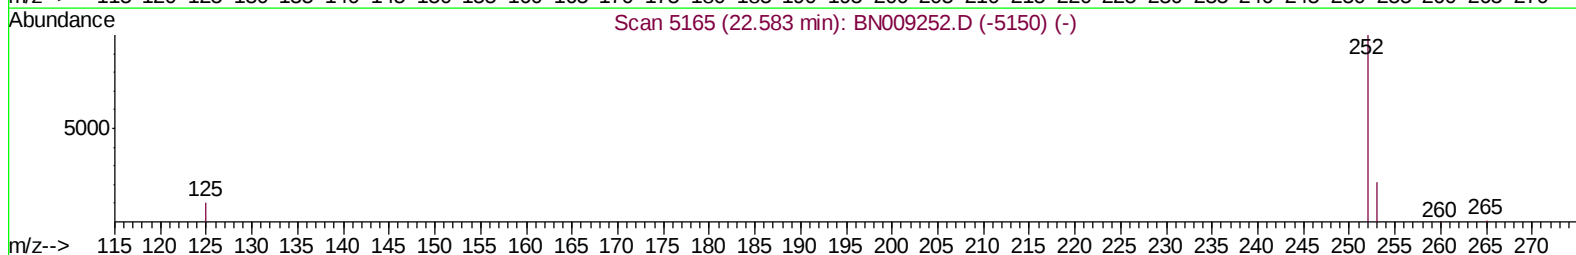
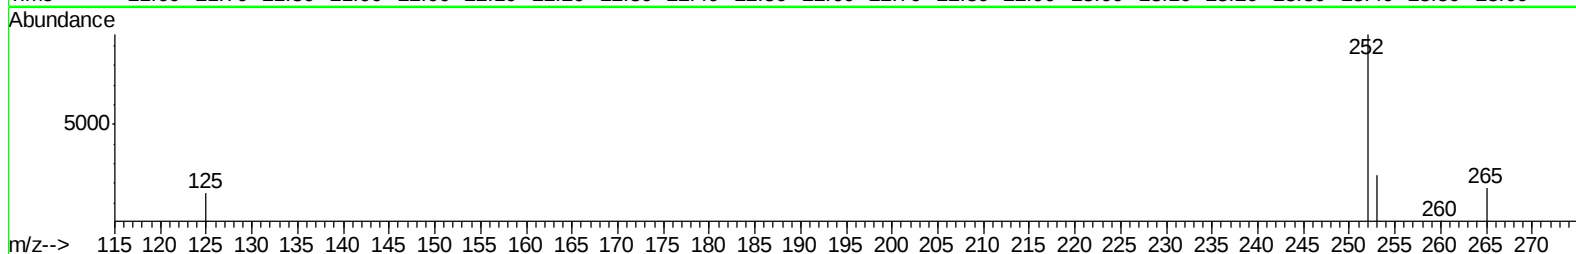


Data File : BN009268.D  
Acq On : 30 Dec 2019 20:07  
Operator : JU  
Sample : K6322-07DL 2X  
Misc :  
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Dec 31 01:04:10 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN121619.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Dec 31 00:59:26 2019  
Response via : Initial Calibration

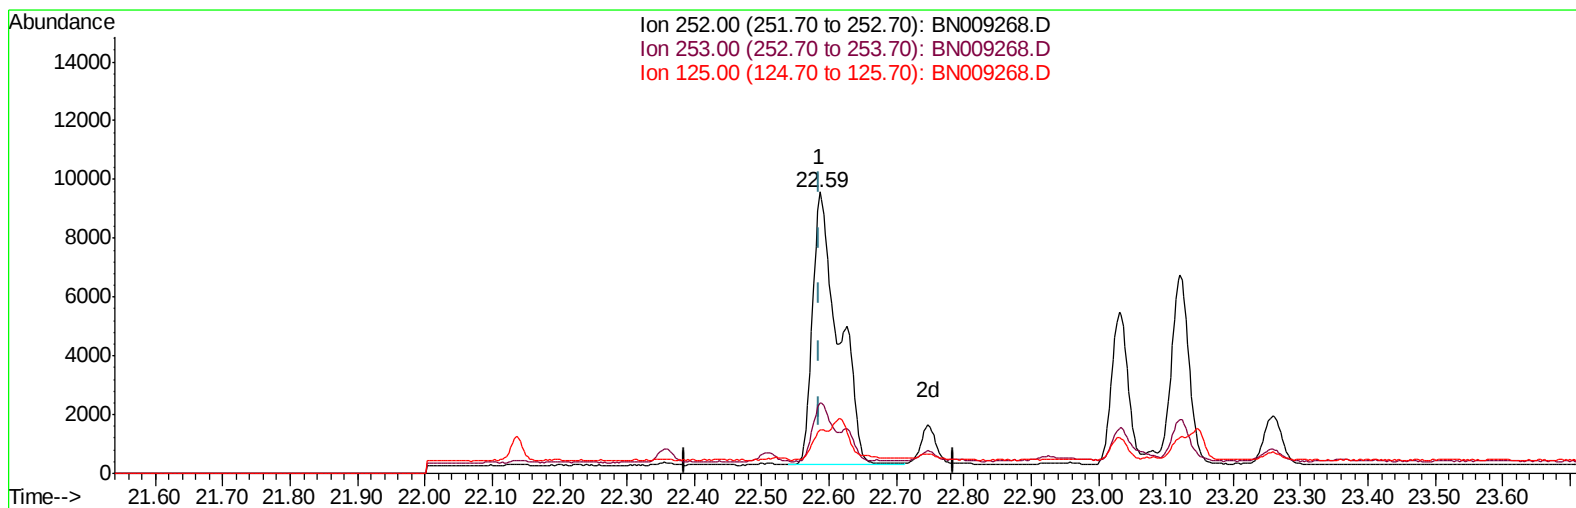

TIC: BN009268.D

(21) Benzo(b)fluoranthene

22.586min (0.000) 0.68ng/ul

response 24885

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 252.00 | 100   | 100   |
| 253.00 | 24.10 | 25.20 |
| 125.00 | 15.00 | 15.38 |
| 0.00   | 0.00  | 0.00  |