
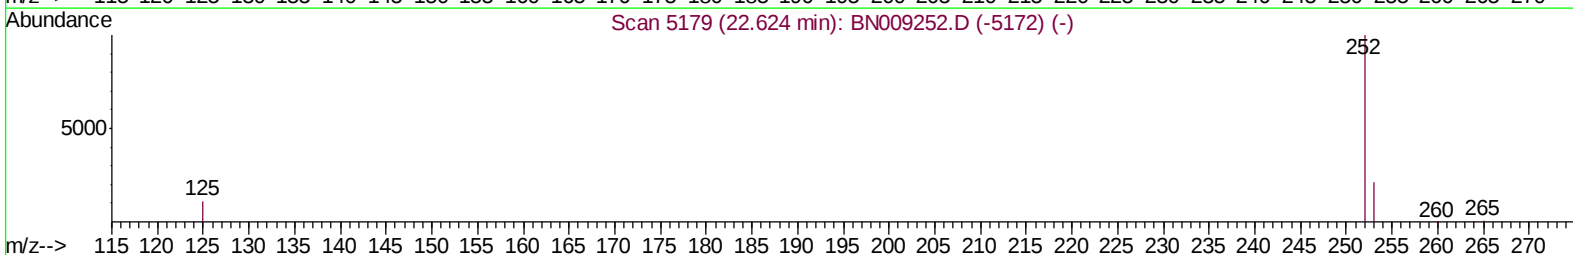
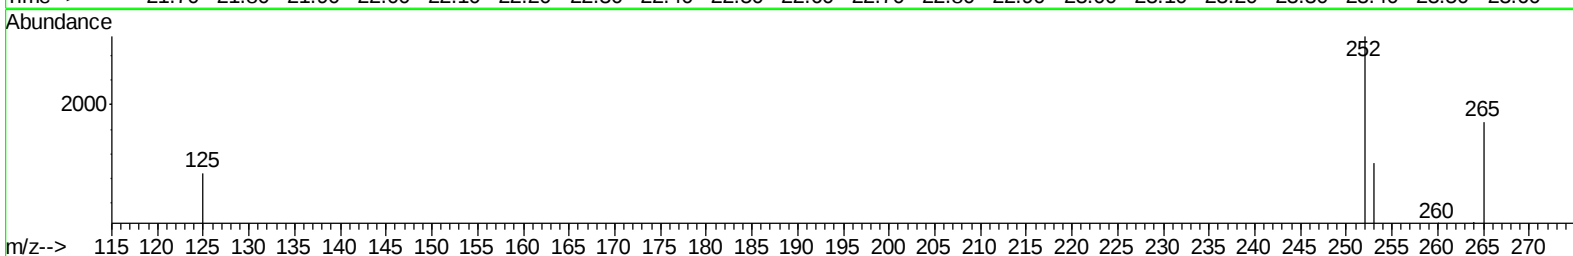


Data File : BN009269.D
Acq On : 30 Dec 2019 20:42
Operator : JU
Sample : K6322-10DL 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Dec 31 01:04:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 00:59:26 2019
Response via : Initial Calibration

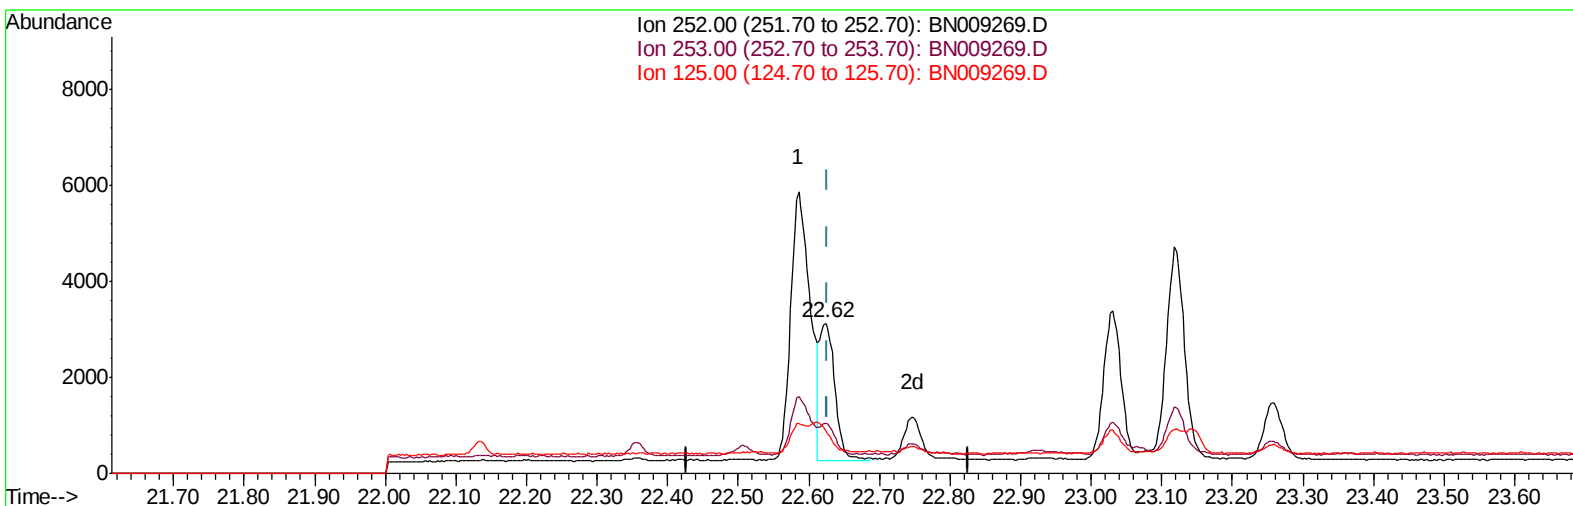

TIC: BN009269.D

(22) Benzo(k)fluoranthene

22.624min (-0.003) 0.12ng/ul m

response 4256

Ion	Exp%	Act%
252.00	100	100
253.00	24.20	33.56#
125.00	15.50	28.17#
0.00	0.00	0.00