
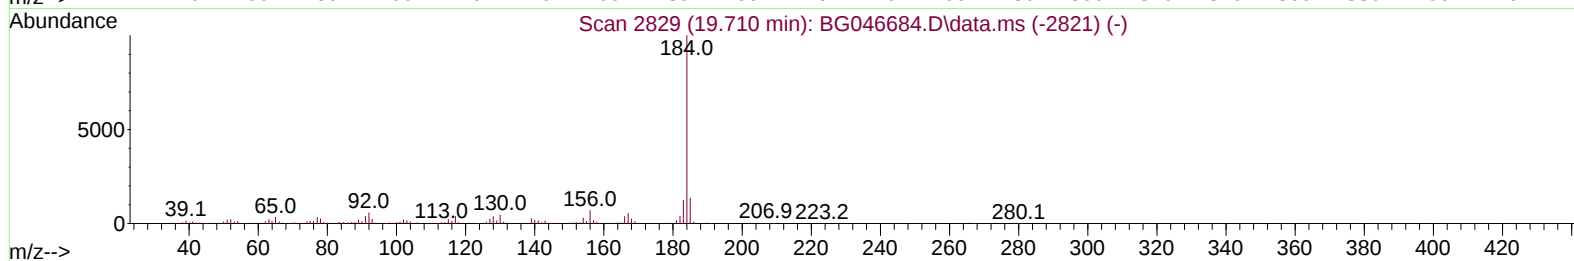
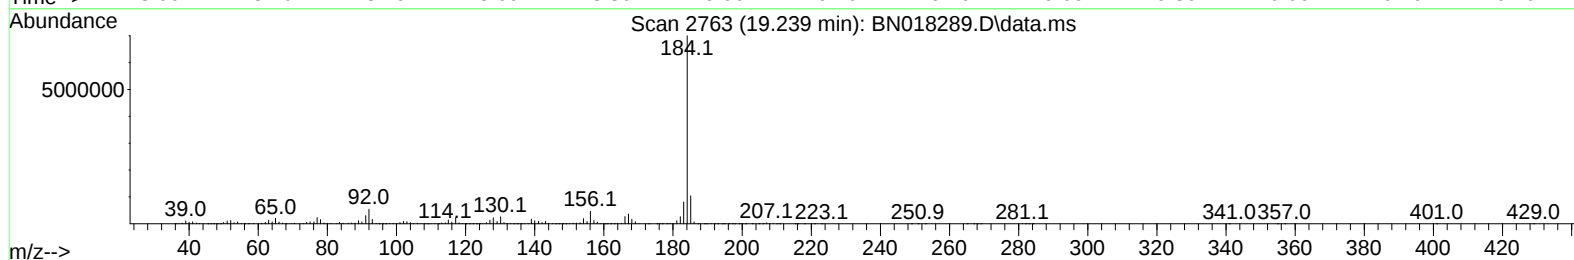


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN123021\
Data File : BN018289.D
Acq On : 30 Dec 2021 09:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 08:26:37 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 31 08:26:32 2021
Response via : Initial Calibration

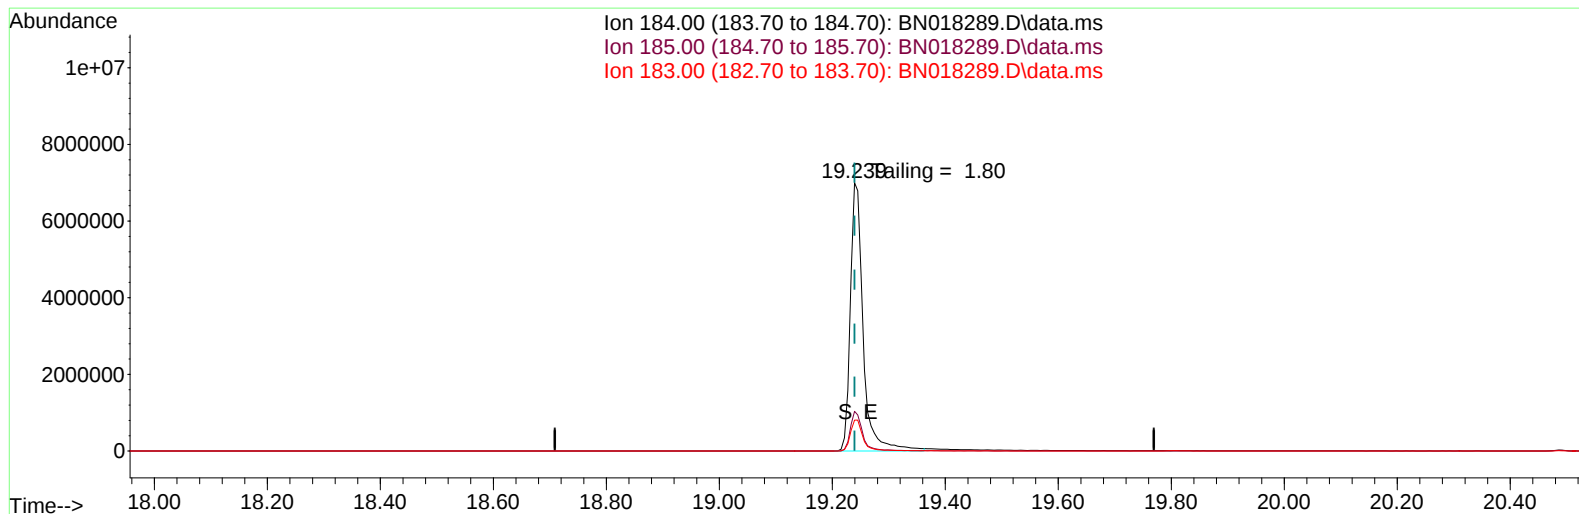

TIC: BN018289.D\data.ms

(77) Benzidine




19.239min (0.000) 2929230.56 ng m

response 11196533

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.82
183.00	13.20	11.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN123021\
 Data File : BN018289.D
 Acq On : 30 Dec 2021 09:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 31 08:26:37 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 31 08:26:32 2021
 Response via : Initial Calibration

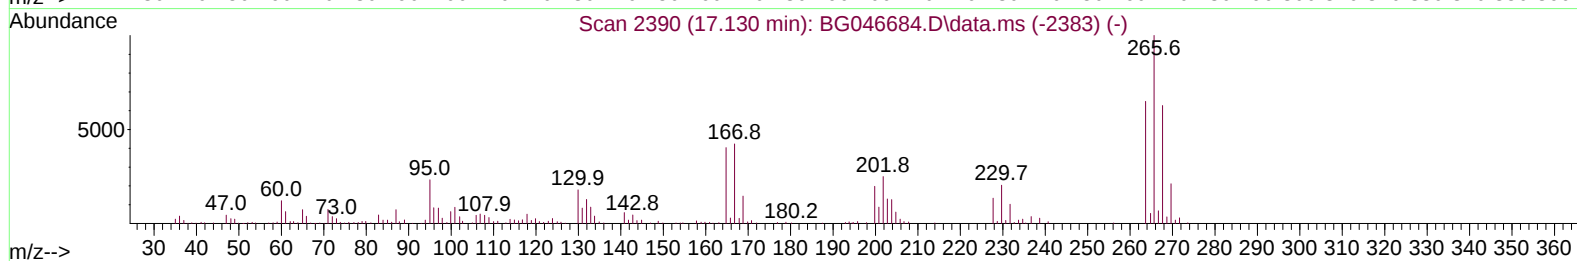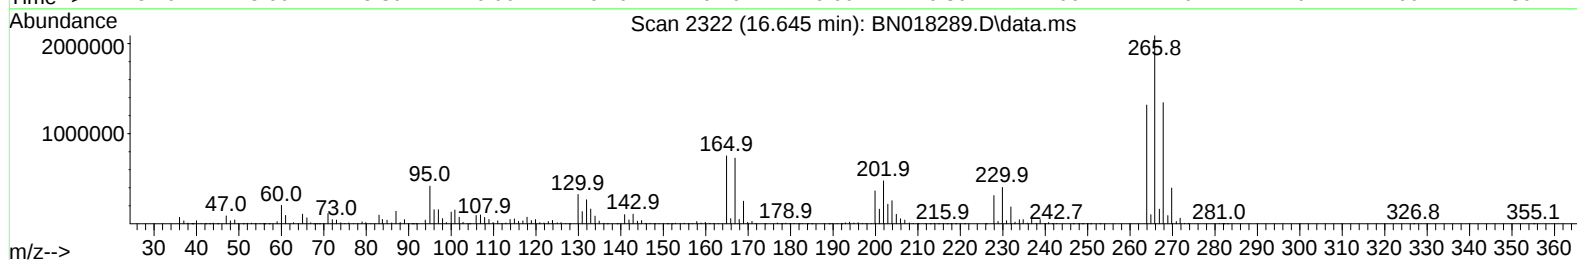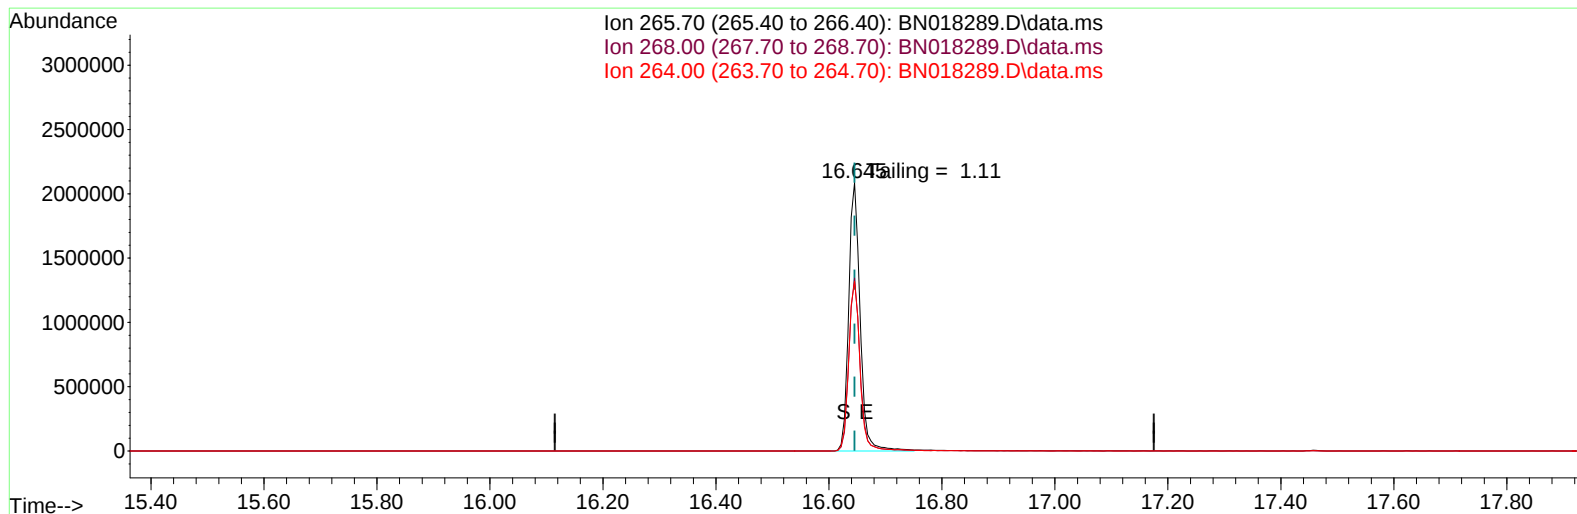

TIC: BN018289.D\data.ms

(70) Pentachlorophenol (C)

16.645min (0.000) 31024.92 ng

response 2972839

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.47
264.00	61.60	63.20
0.00	0.00	0.00