


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN123021\
 Data File : BN018289.D
 Acq On : 30 Dec 2021 09:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN122921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 29 16:08:47 2021

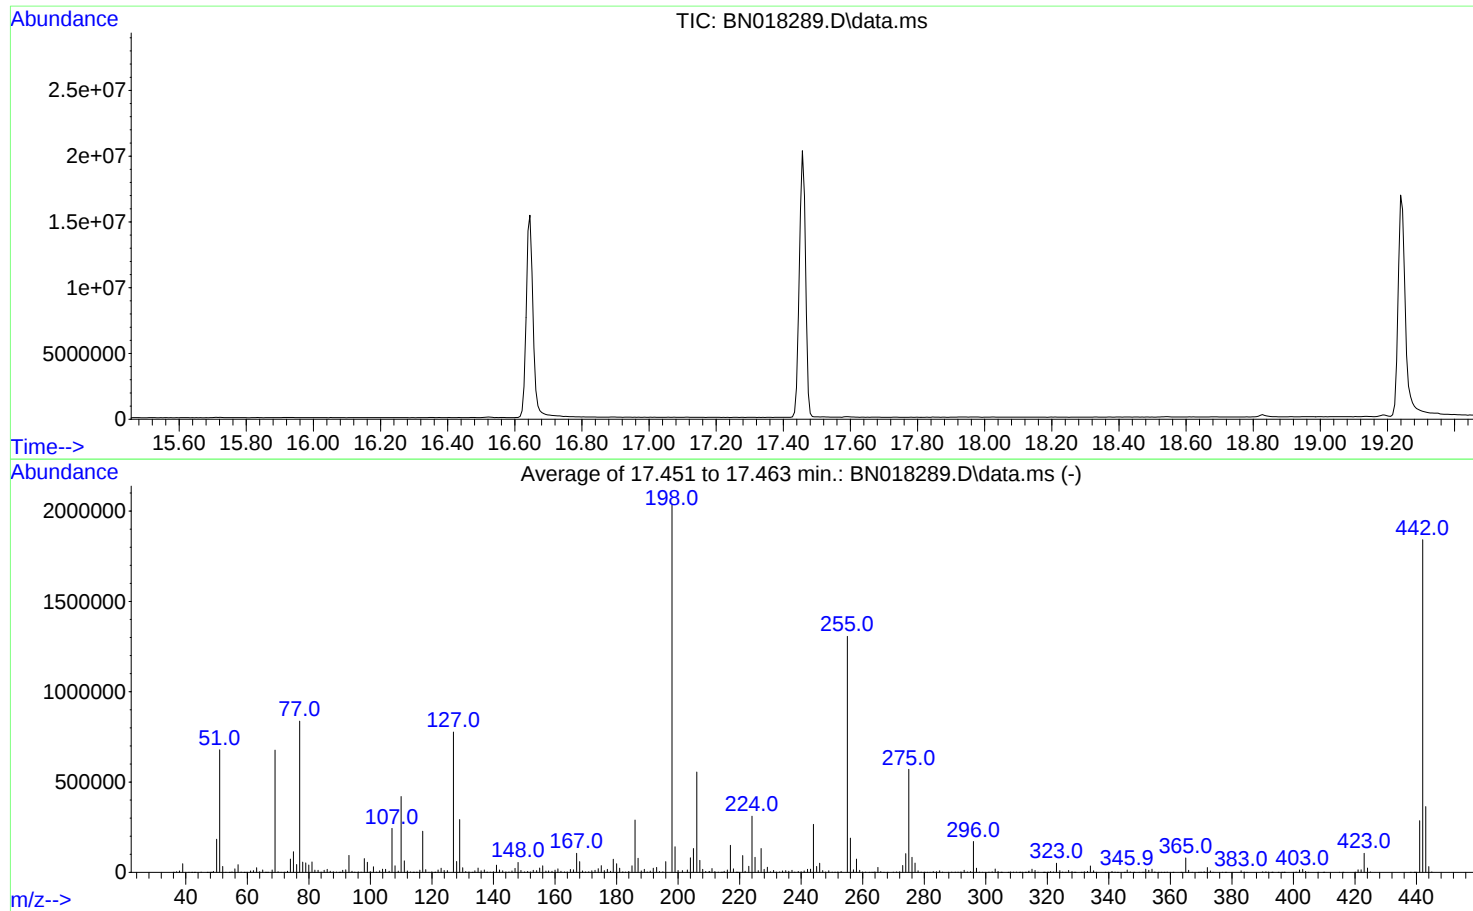




AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	679039	PASS
68	69	0.00	2	2.0	13230	PASS
69	198	0.00	100	33.2	677046	PASS
70	69	0.00	2	0.5	3603	PASS
127	198	10	80	38.2	777152	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	2036395	PASS
199	198	5	9	7.0	141899	PASS
275	198	10	60	28.0	570389	PASS
365	198	1	100	3.9	80008	PASS
441	198	0.01	100	14.1	286165	PASS
442	442	50	100	100.0	1841152	PASS
443	442	15	24	19.8	363733	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN123021\
Data File : BN018289.D
Acq On : 30 Dec 2021 09:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 31 08:26:37 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 31 08:26:32 2021
Response via : Initial Calibration

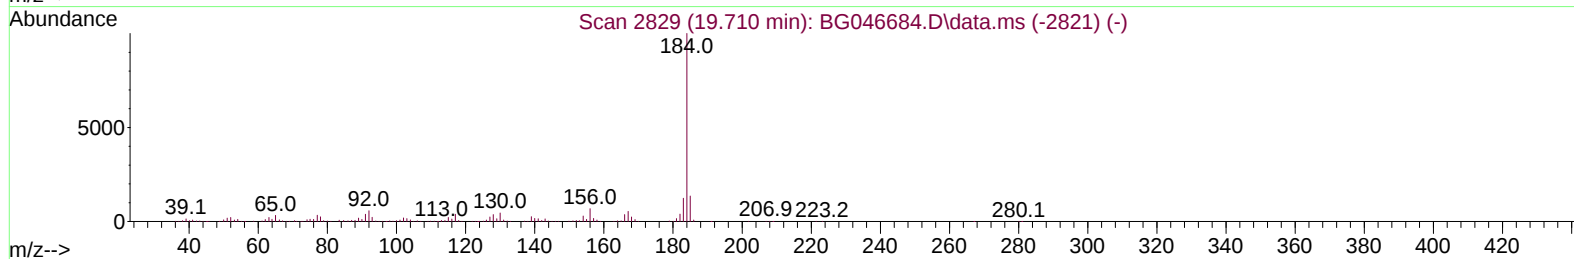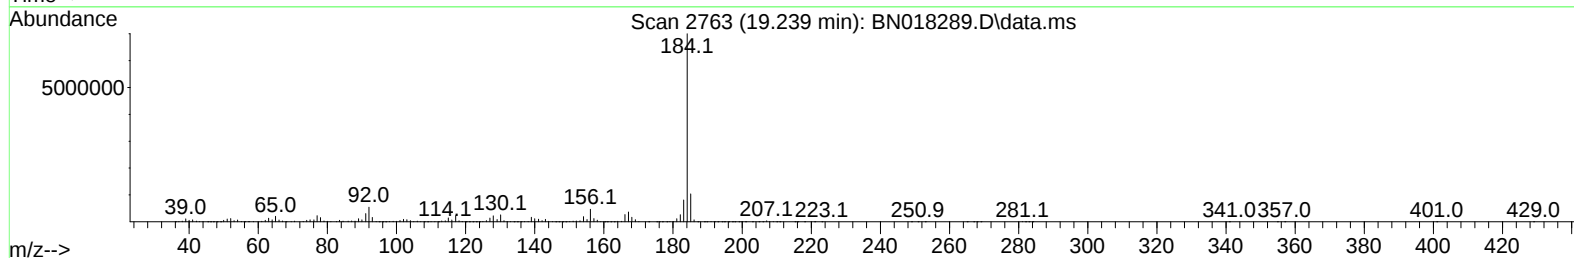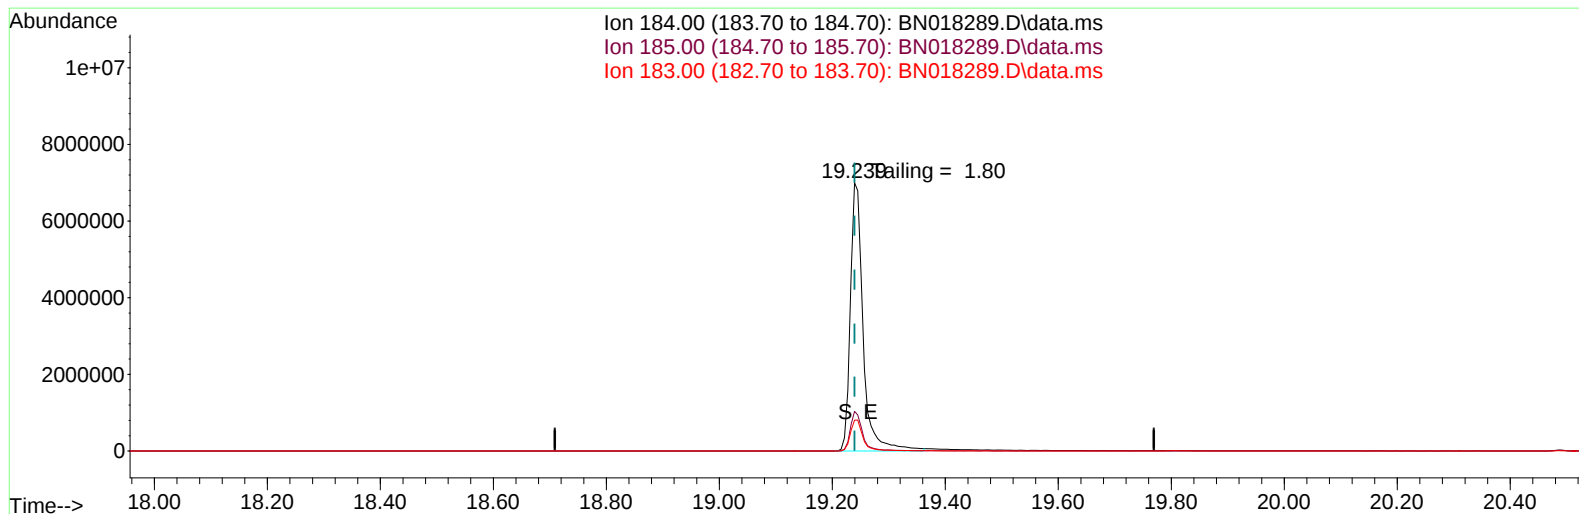

TIC: BN018289.D\data.ms

(77) Benzidine

19.239min (0.000) 2929230.56 ng m




response 11196533

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.82
183.00	13.20	11.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN123021\
Data File : BN018289.D
Acq On : 30 Dec 2021 09:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 31 08:26:37 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 31 08:26:32 2021
Response via : Initial Calibration

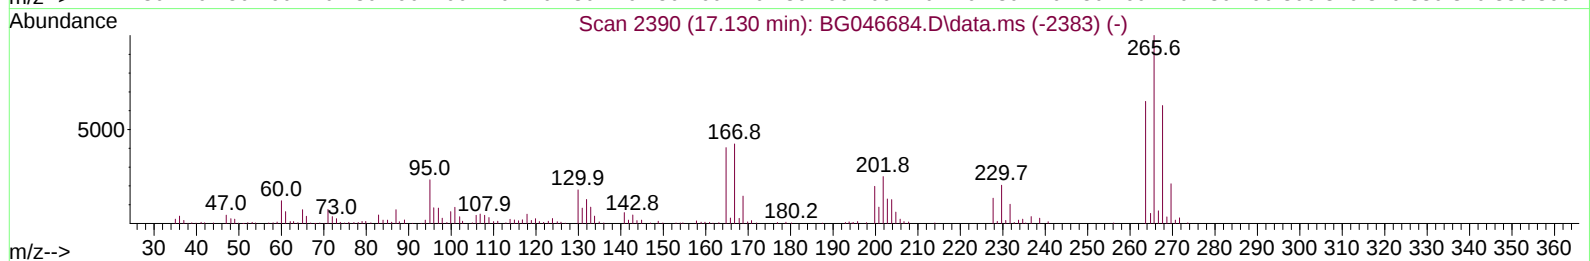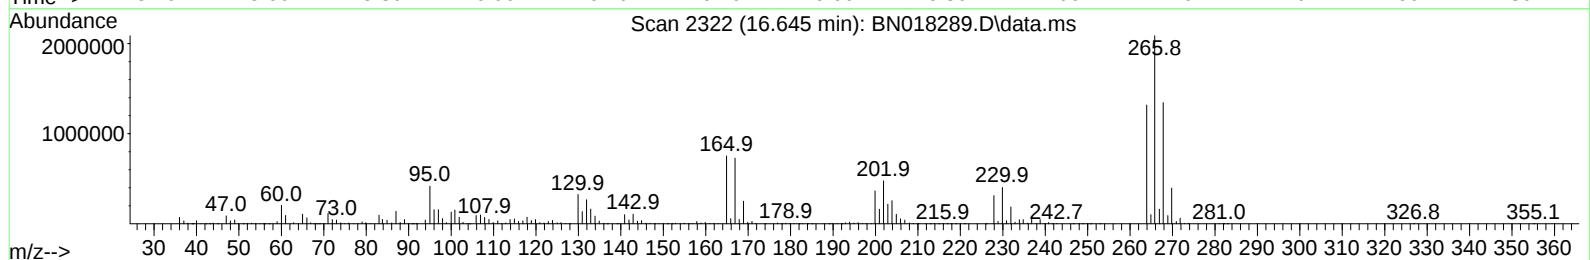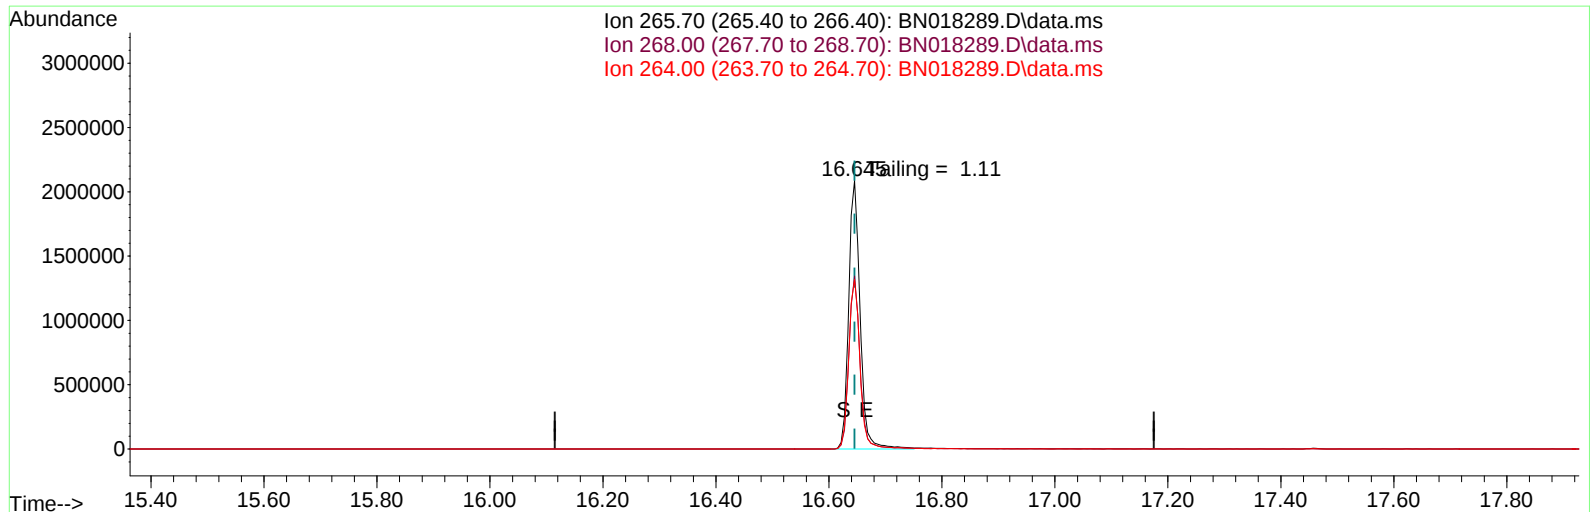

TIC: BN018289.D\data.ms

(70) Pentachlorophenol (C)

16.645min (0.000) 31024.92 ng

response 2972839

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.47
264.00	61.60	63.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/30/2021	BNA_N	<u>BN018289.D</u>
Compound Name	Response	Retention Time
DDT	7527681	20.486
DDD	451464	20.045
DDE	24241	19.539
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
475705	8003386	5.94

Instrument :
BNA_N
ClientSampleId :
DFTPP