

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010322\
 Data File : BN018306.D
 Acq On : 03 Jan 2022 14:16
 Operator : CG/JU
 Sample : M5152-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG3C1

Quant Time: Jan 04 00:00:18 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 28 00:34:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.611	152	2395	0.400	ng/ul	0.00
4) Naphthalene-d8	10.387	136	9119	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.248	164	7457	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.989	188	19206	0.400	ng/ul	0.00
17) Chrysene-d12	21.187	240	24142	0.400	ng/ul	0.00
23) Perylene-d12	23.402	264	31250	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.067	96	11719	5.241	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.987	152	5299	0.334	ng/ul	0.00
18) Fluoranthene-d10	19.021	212	26772	0.374	ng/ul	0.00
Target Compounds						
15) Phenanthrene	17.032	178	3012	0.047	ng/ul#	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010322\
Data File : BN018306.D
Acq On : 03 Jan 2022 14:16
Operator : CG/JU
Sample : M5152-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG3C1


Quant Time: Jan 04 00:00:18 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 28 00:34:45 2021
Response via : Initial Calibration

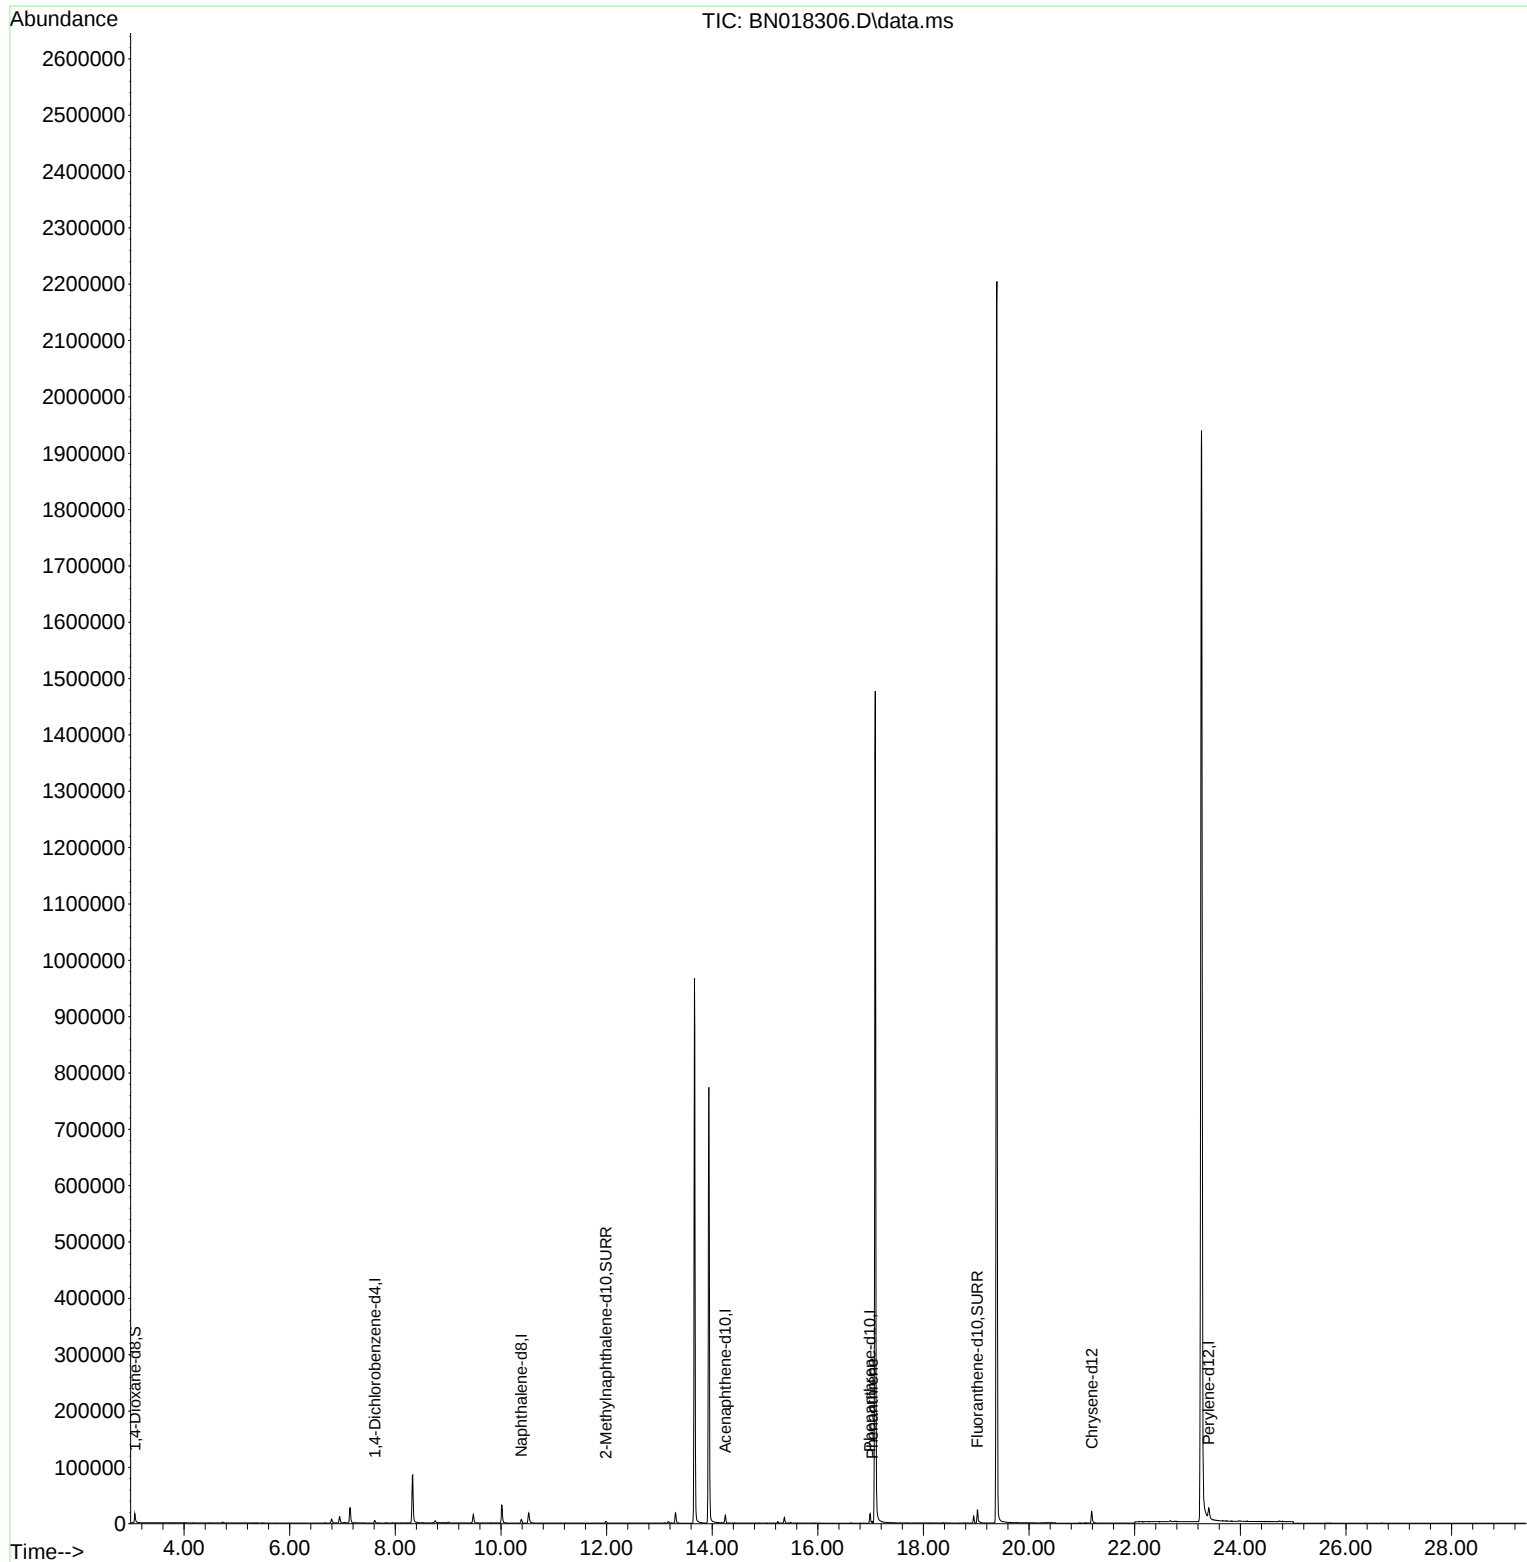

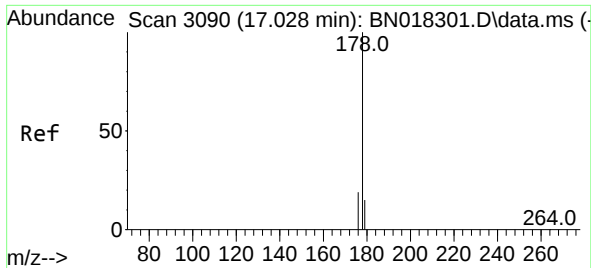

#15
 Phenanthrene
 Concen: 0.047 ng/ul
 RT: 17.032 min Scan# 3012
 Delta R.T. -0.000 min
 Lab File: BN018306.D
 Acq: 03 Jan 2022 14:16

Instrument :
 BNA_N
 ClientSampleId :
 BG3C1

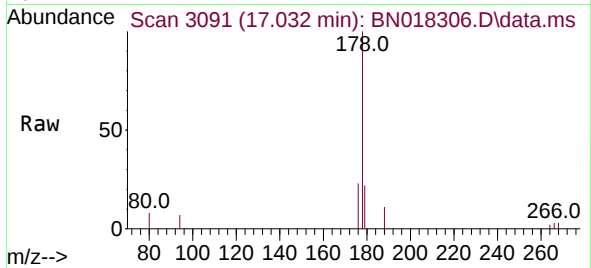

Tgt Ion:	178	Resp:	3012
Ion Ratio	Lower	Upper	
178	100		
179	21.7	12.2	18.4#
176	23.2	15.4	23.2#

