

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010322\
 Data File : BN018309.D
 Acq On : 03 Jan 2022 16:04
 Operator : CG/JU
 Sample : M5152-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG3D4

Quant Time: Jan 04 00:04:05 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 28 00:34:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.611	152	1930	0.400	ng/ul	0.00
4) Naphthalene-d8	10.388	136	7251	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.249	164	6052	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	16.987	188	15769	0.400	ng/ul	0.00
17) Chrysene-d12	21.186	240	19385	0.400	ng/ul	0.00
23) Perylene-d12	23.407	264	26655	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.067	96	8972	4.980	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.989	152	4590	0.364	ng/ul	0.00
18) Fluoranthene-d10	19.023	212	23365	0.407	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.105	88	265	0.132	ng/ul#	74
15) Phenanthrene	17.029	178	2525	0.048	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010322\
Data File : BN018309.D
Acq On : 03 Jan 2022 16:04
Operator : CG/JU
Sample : M5152-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG3D4

Quant Time: Jan 04 00:04:05 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 28 00:34:45 2021
Response via : Initial Calibration




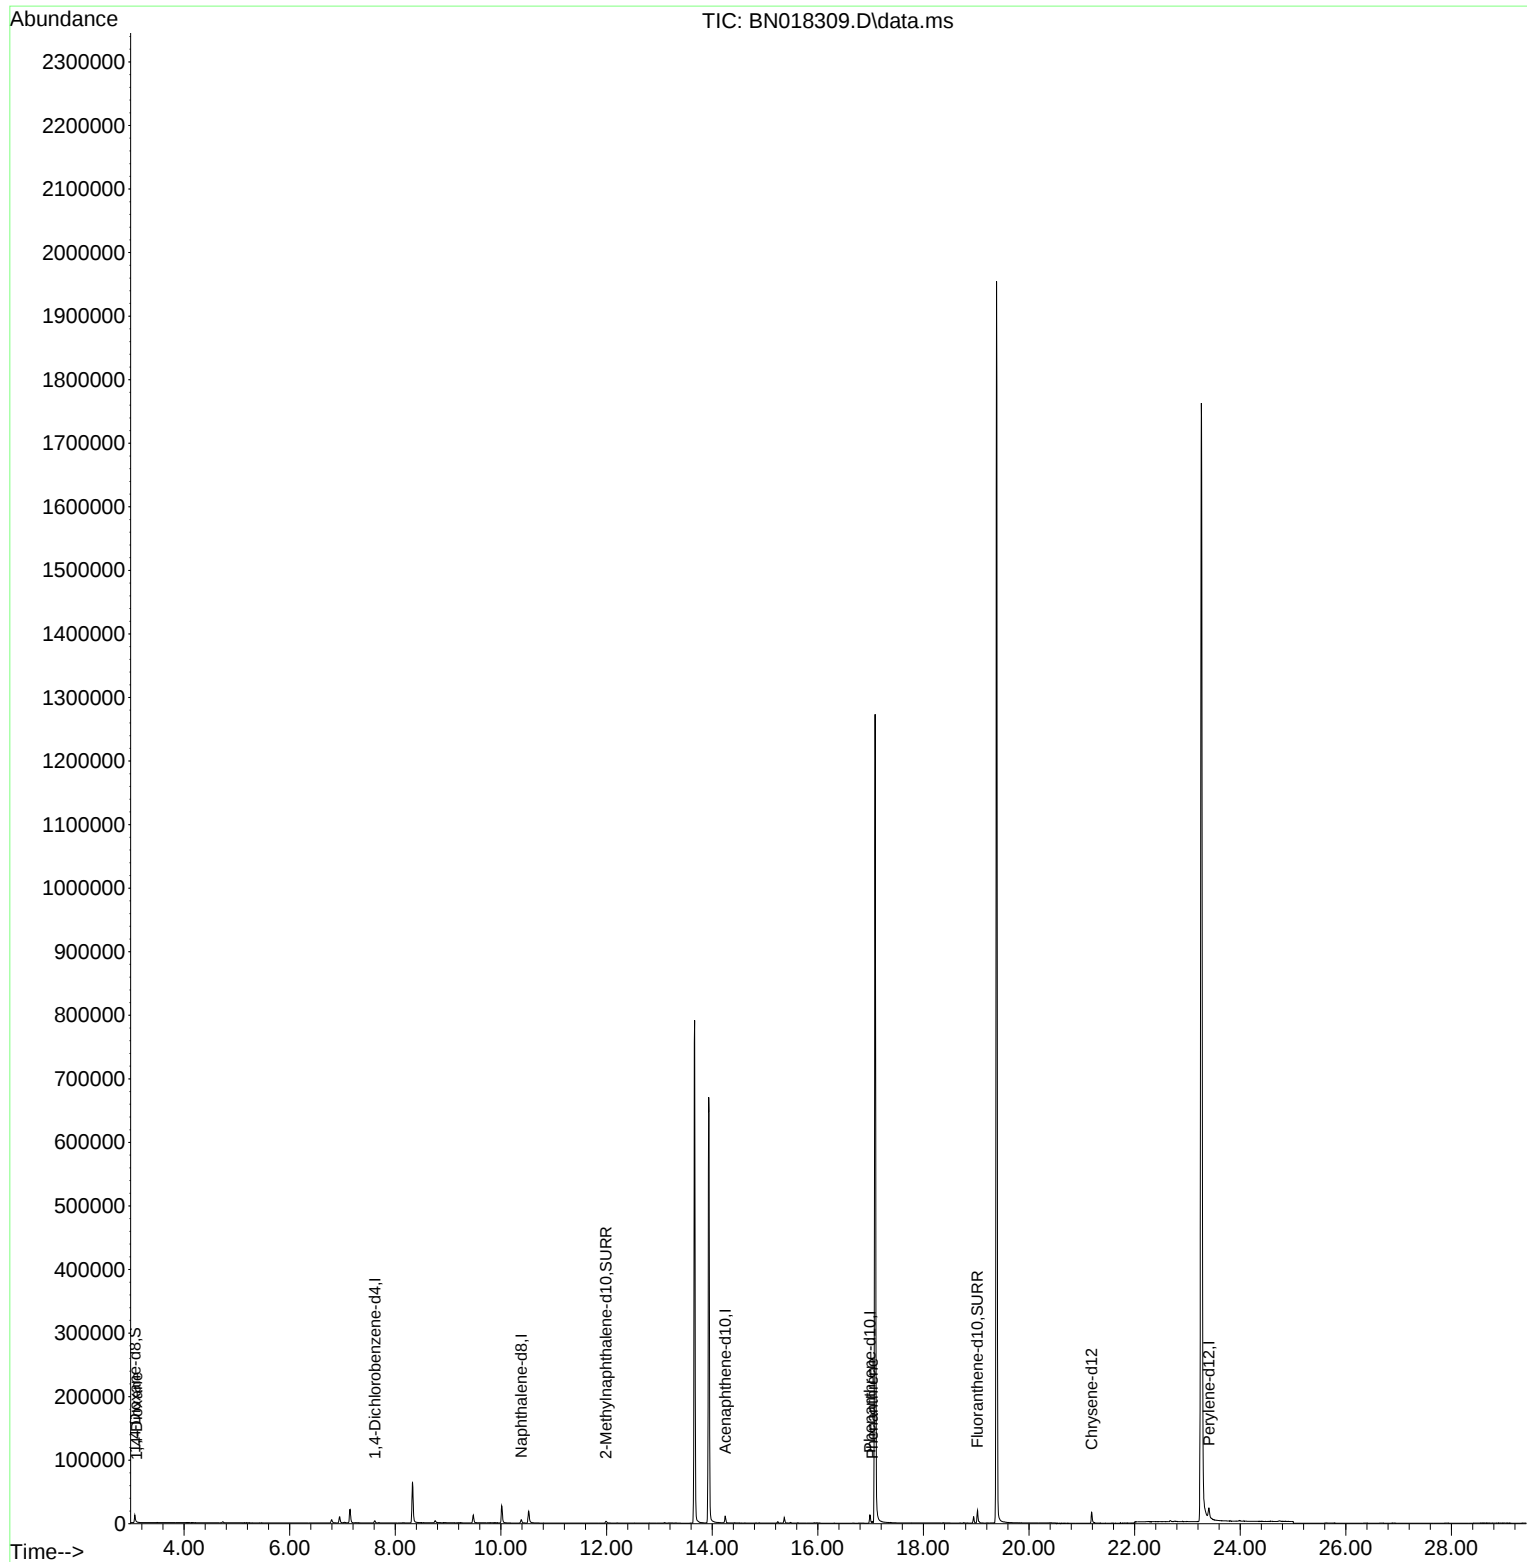


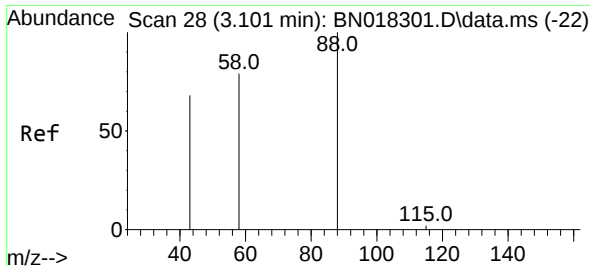

#2
 1,4-Dioxane
 Concen: 0.132 ng/ul
 RT: 3.105 min Scan# 24
 Delta R.T. 0.000 min
 Lab File: BN018309.D
 Acq: 03 Jan 2022 16:04

Instrument :
 BNA_N
 ClientSampleId :
 BG3D4

Tgt Ion: 88 Resp: 265
 Ion Ratio Lower Upper
 88 100
 43 65.2 47.8 71.8
 58 24.1 46.2 69.2#

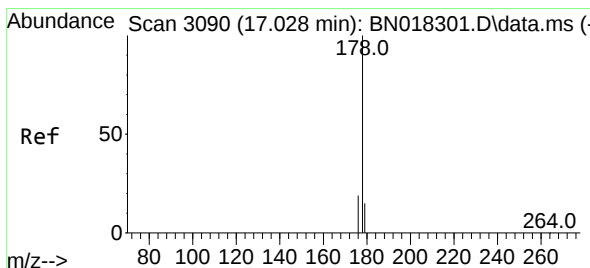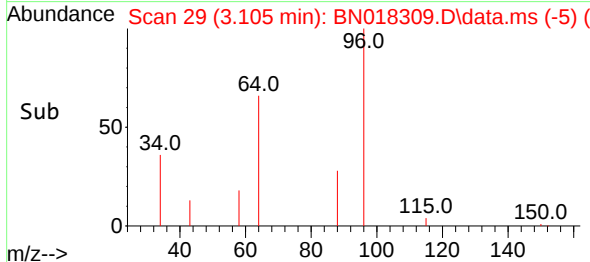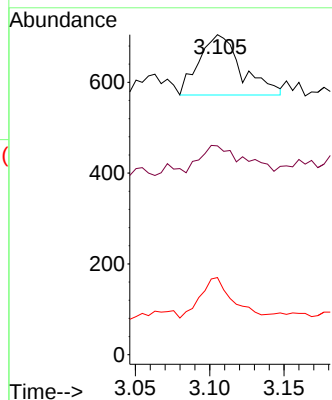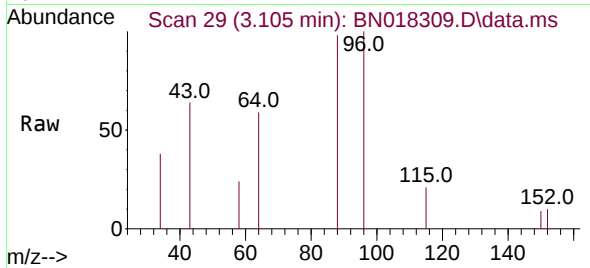

#15
 Phenanthrene
 Concen: 0.048 ng/ul
 RT: 17.029 min Scan# 3090
 Delta R.T. -0.003 min
 Lab File: BN018309.D
 Acq: 03 Jan 2022 16:04

Tgt Ion: 178 Resp: 2525
 Ion Ratio Lower Upper
 178 100
 179 22.3 12.2 18.4#
 176 23.8 15.4 23.2#

