

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010322\
 Data File : BN018310.D
 Acq On : 03 Jan 2022 16:40
 Operator : CG/JU
 Sample : M5152-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG3E5

Quant Time: Jan 04 00:04:12 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 28 00:34:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.611	152	1545	0.400	ng/ul	0.00
4) Naphthalene-d8	10.383	136	5749	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.249	164	4841	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.991	188	12857	0.400	ng/ul	0.00
17) Chrysene-d12	21.186	240	17455	0.400	ng/ul	0.00
23) Perylene-d12	23.404	264	25900	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.067	96	6781	4.701	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.983	152	3479	0.348	ng/ul	0.00
18) Fluoranthene-d10	19.023	212	17927	0.347	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.438	128	724	0.042	ng/ul#	65
15) Phenanthrene	17.029	178	2304	0.054	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010322\
Data File : BN018310.D
Acq On : 03 Jan 2022 16:40
Operator : CG/JU
Sample : M5152-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG3E5

Quant Time: Jan 04 00:04:12 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 28 00:34:45 2021
Response via : Initial Calibration




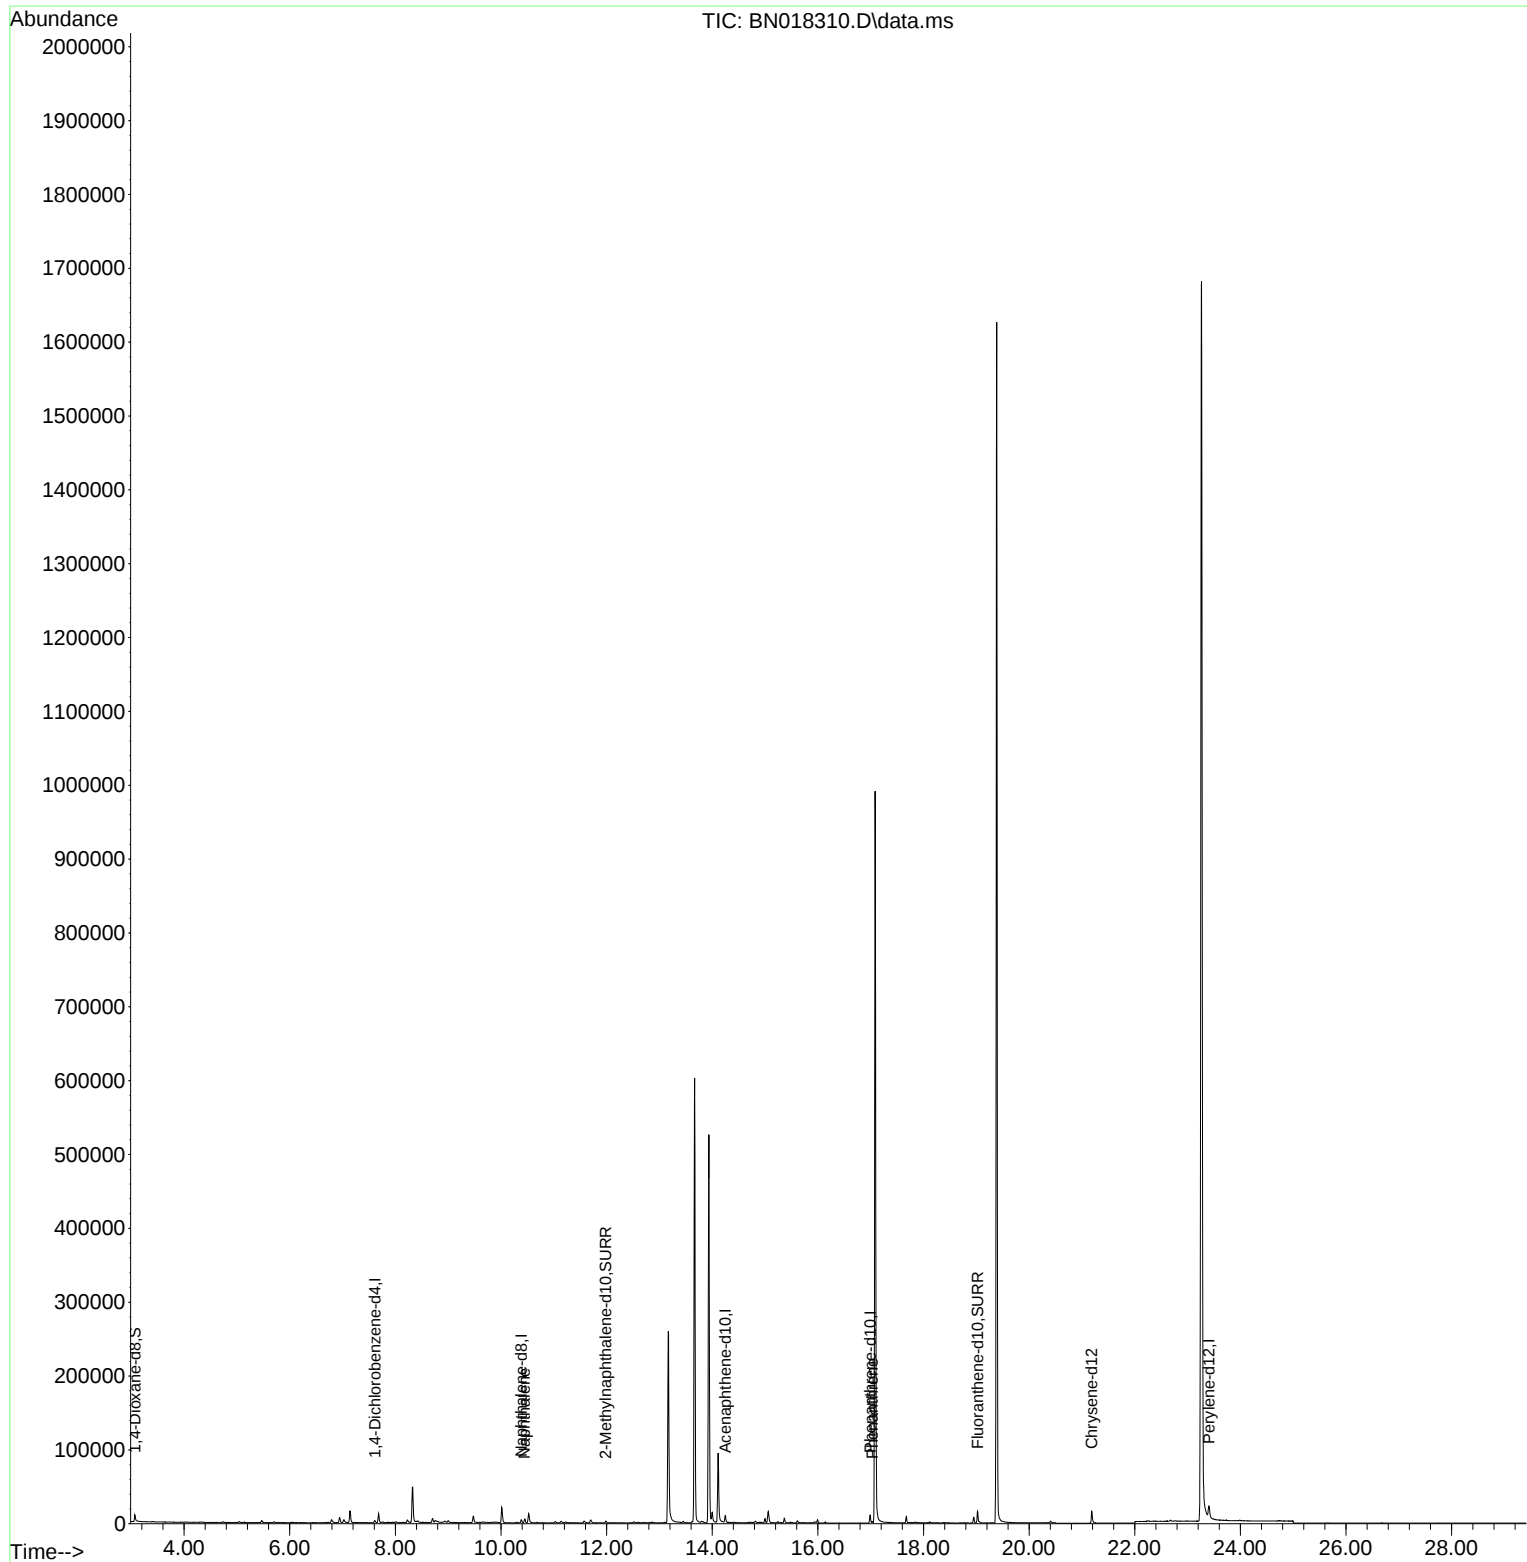


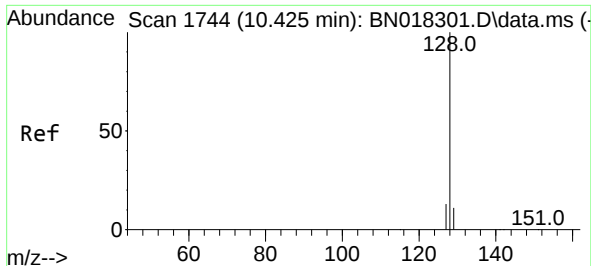

#5
Naphthalene
Concen: 0.042 ng/ul
RT: 10.438 min Scan# 1746
Delta R.T. 0.001 min
Lab File: BN018310.D
Acq: 03 Jan 2022 16:40

Instrument :
BNA_N
ClientSampleId :
BG3E5

Tgt Ion:128 Resp: 724
Ion Ratio Lower Upper
128 100
129 27.1 9.4 14.0#
127 26.2 11.0 16.6#

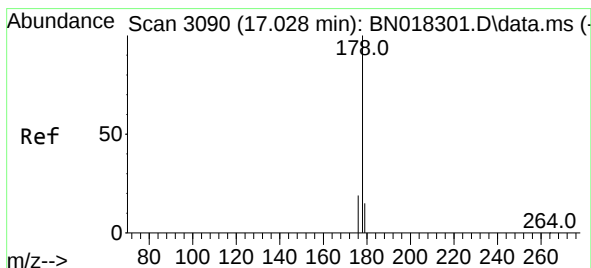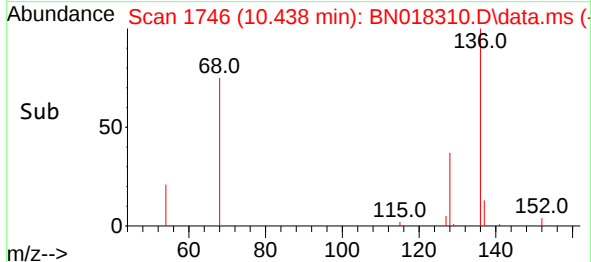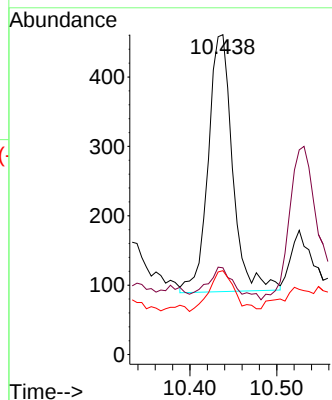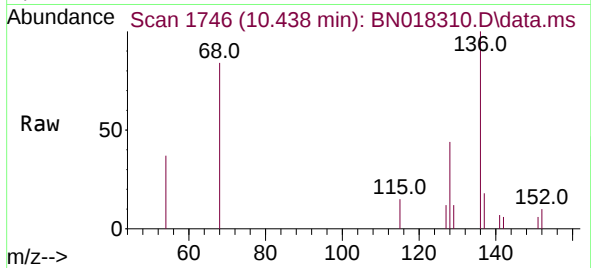

#15
Phenanthrene
Concen: 0.054 ng/ul
RT: 17.029 min Scan# 3090
Delta R.T. -0.003 min
Lab File: BN018310.D
Acq: 03 Jan 2022 16:40

Tgt Ion:178 Resp: 2304
Ion Ratio Lower Upper
178 100
179 23.3 12.2 18.4#
176 24.3 15.4 23.2#

