

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010322\
 Data File : BN018319.D
 Acq On : 03 Jan 2022 22:03
 Operator : CG/JU
 Sample : M5091-15
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG3C7

Quant Time: Jan 04 00:06:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 28 00:34:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.611	152	2299	0.400	ng/ul	0.00
4) Naphthalene-d8	10.387	136	8887	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.248	164	7046	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	16.990	188	18795	0.400	ng/ul	0.00
17) Chrysene-d12	21.181	240	24261	0.400	ng/ul	0.00
23) Perylene-d12	23.399	264	31306	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.067	96	9023	4.204	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.987	152	4522	0.293	ng/ul	0.00
18) Fluoranthene-d10	19.021	212	23783	0.331	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.101	88	237	0.099	ng/ul#	59
15) Phenanthrene	17.028	178	1673	0.027	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010322\
Data File : BN018319.D
Acq On : 03 Jan 2022 22:03
Operator : CG/JU
Sample : M5091-15
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG3C7

Quant Time: Jan 04 00:06:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 28 00:34:45 2021
Response via : Initial Calibration




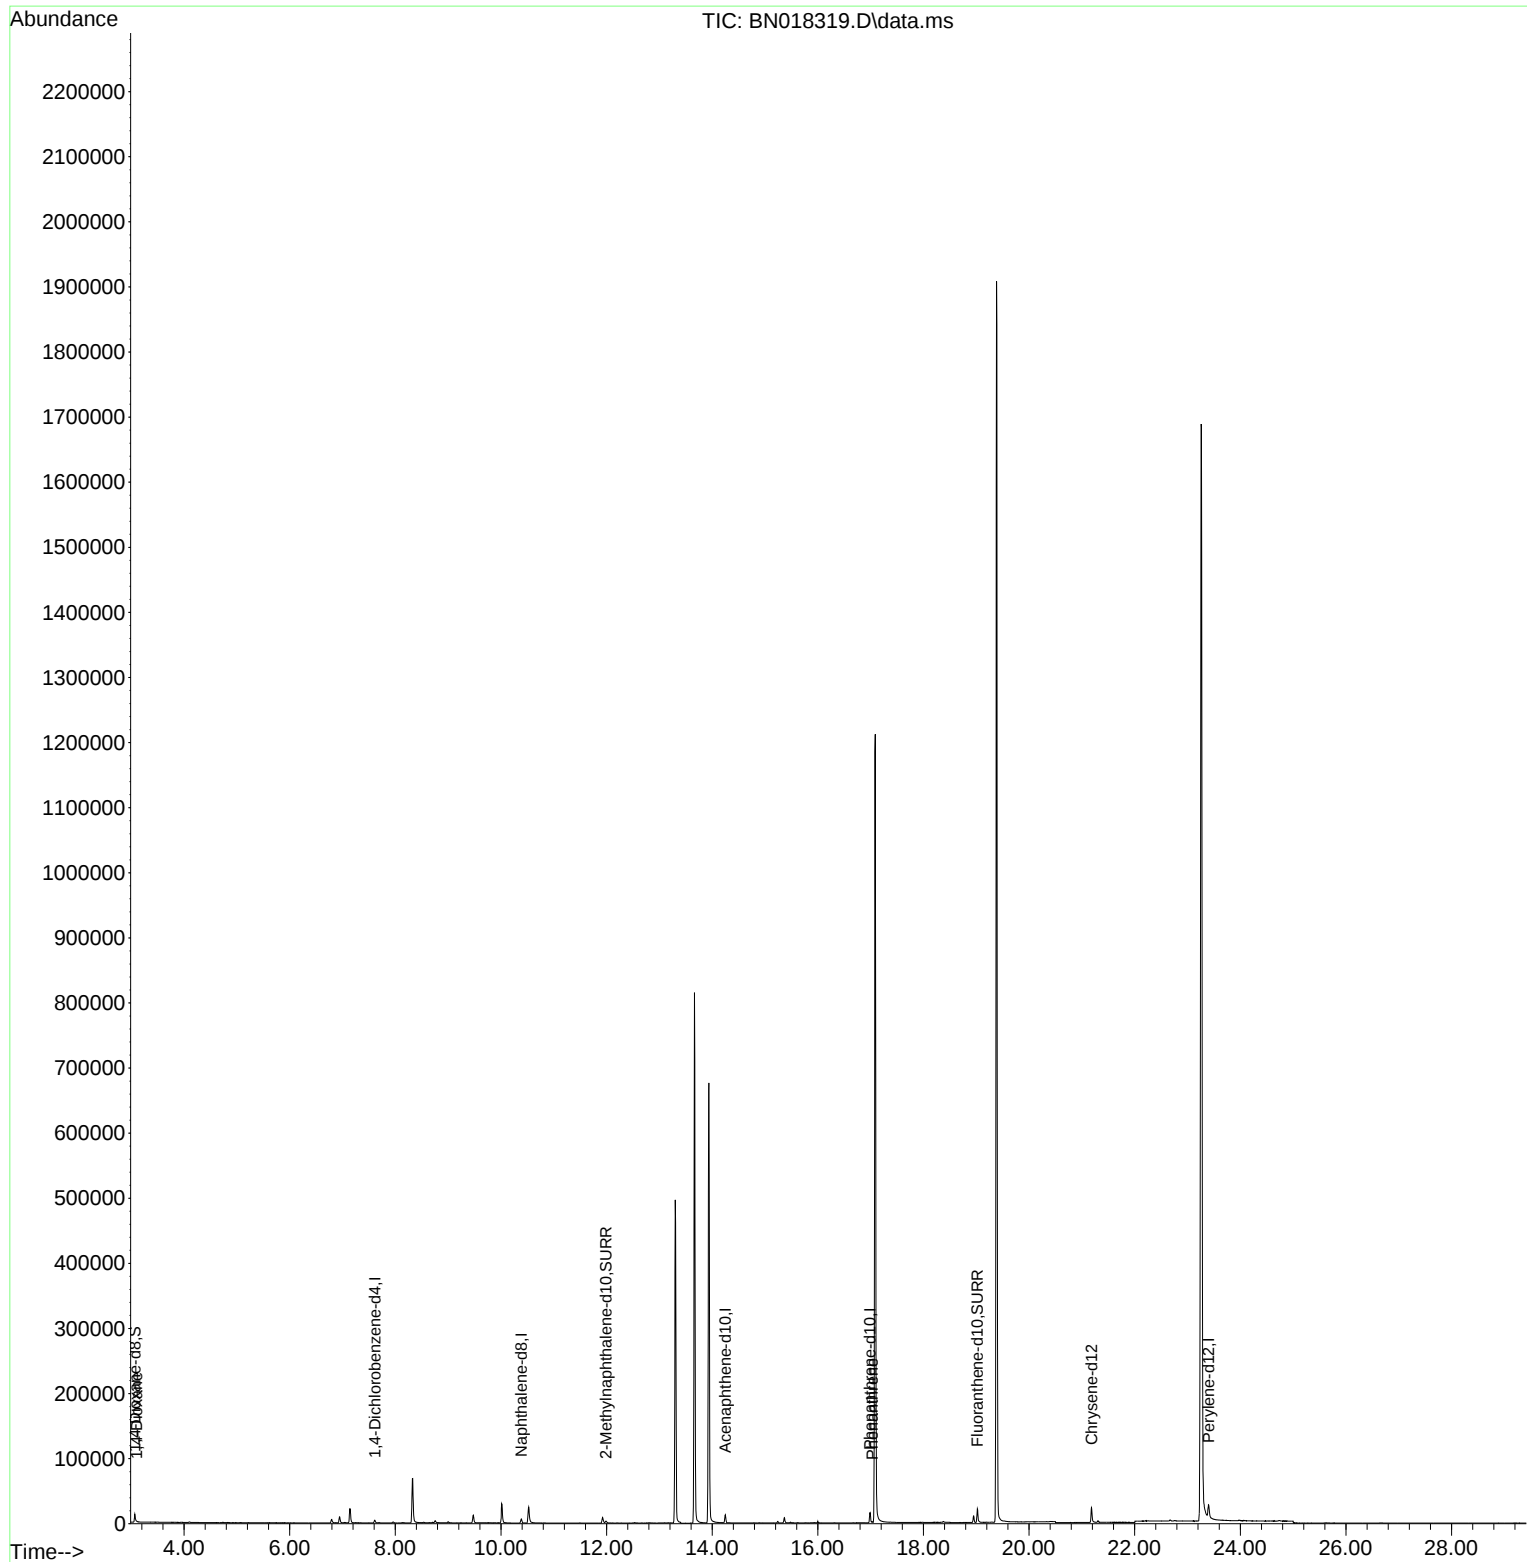


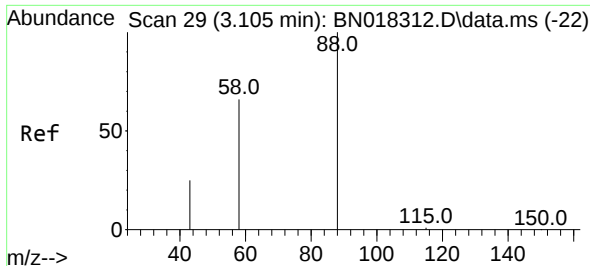

#2
 1,4-Dioxane
 Concen: 0.099 ng/ul
 RT: 3.101 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN018319.D
 Acq: 03 Jan 2022 22:03

Instrument :
 BNA_N
 ClientSampleId :
 BG3C7

Tgt Ion: 88 Resp: 237
 Ion Ratio Lower Upper
 88 100
 43 98.7 47.8 71.8#
 58 35.8 46.2 69.2#

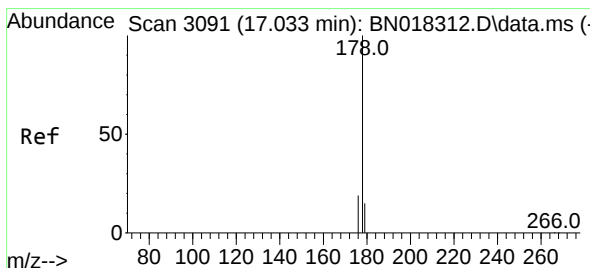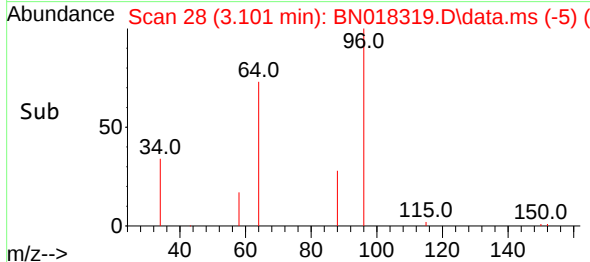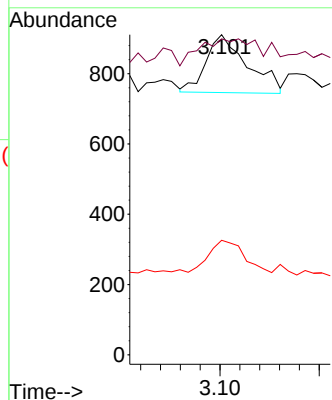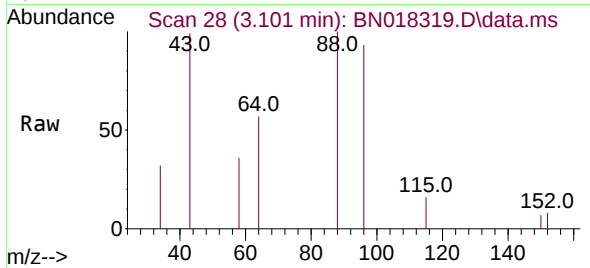

#15
 Phenanthrene
 Concen: 0.027 ng/ul
 RT: 17.028 min Scan# 3090
 Delta R.T. -0.004 min
 Lab File: BN018319.D
 Acq: 03 Jan 2022 22:03

Tgt Ion: 178 Resp: 1673
 Ion Ratio Lower Upper
 178 100
 179 29.2 12.2 18.4#
 176 30.2 15.4 23.2#

