

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010322\
 Data File : BN018324.D
 Acq On : 04 Jan 2022 01:03
 Operator : CG/JU
 Sample : M5173-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG3D4

Quant Time: Jan 04 02:10:27 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 28 00:34:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.611	152	1966	0.400	ng/ul	0.00
4) Naphthalene-d8	10.383	136	7680	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.245	164	6291	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	16.987	188	16710	0.400	ng/ul	0.00
17) Chrysene-d12	21.186	240	21134	0.400	ng/ul	0.00
23) Perylene-d12	23.398	264	30141	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.067	96	9036	4.923	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.989	152	4718	0.353	ng/ul	0.00
18) Fluoranthene-d10	19.023	212	24930	0.398	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.438	128	471	0.021	ng/ul#	59
15) Phenanthrene	17.029	178	2631	0.048	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010322\
Data File : BN018324.D
Acq On : 04 Jan 2022 01:03
Operator : CG/JU
Sample : M5173-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG3D4

Quant Time: Jan 04 02:10:27 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 28 00:34:45 2021
Response via : Initial Calibration




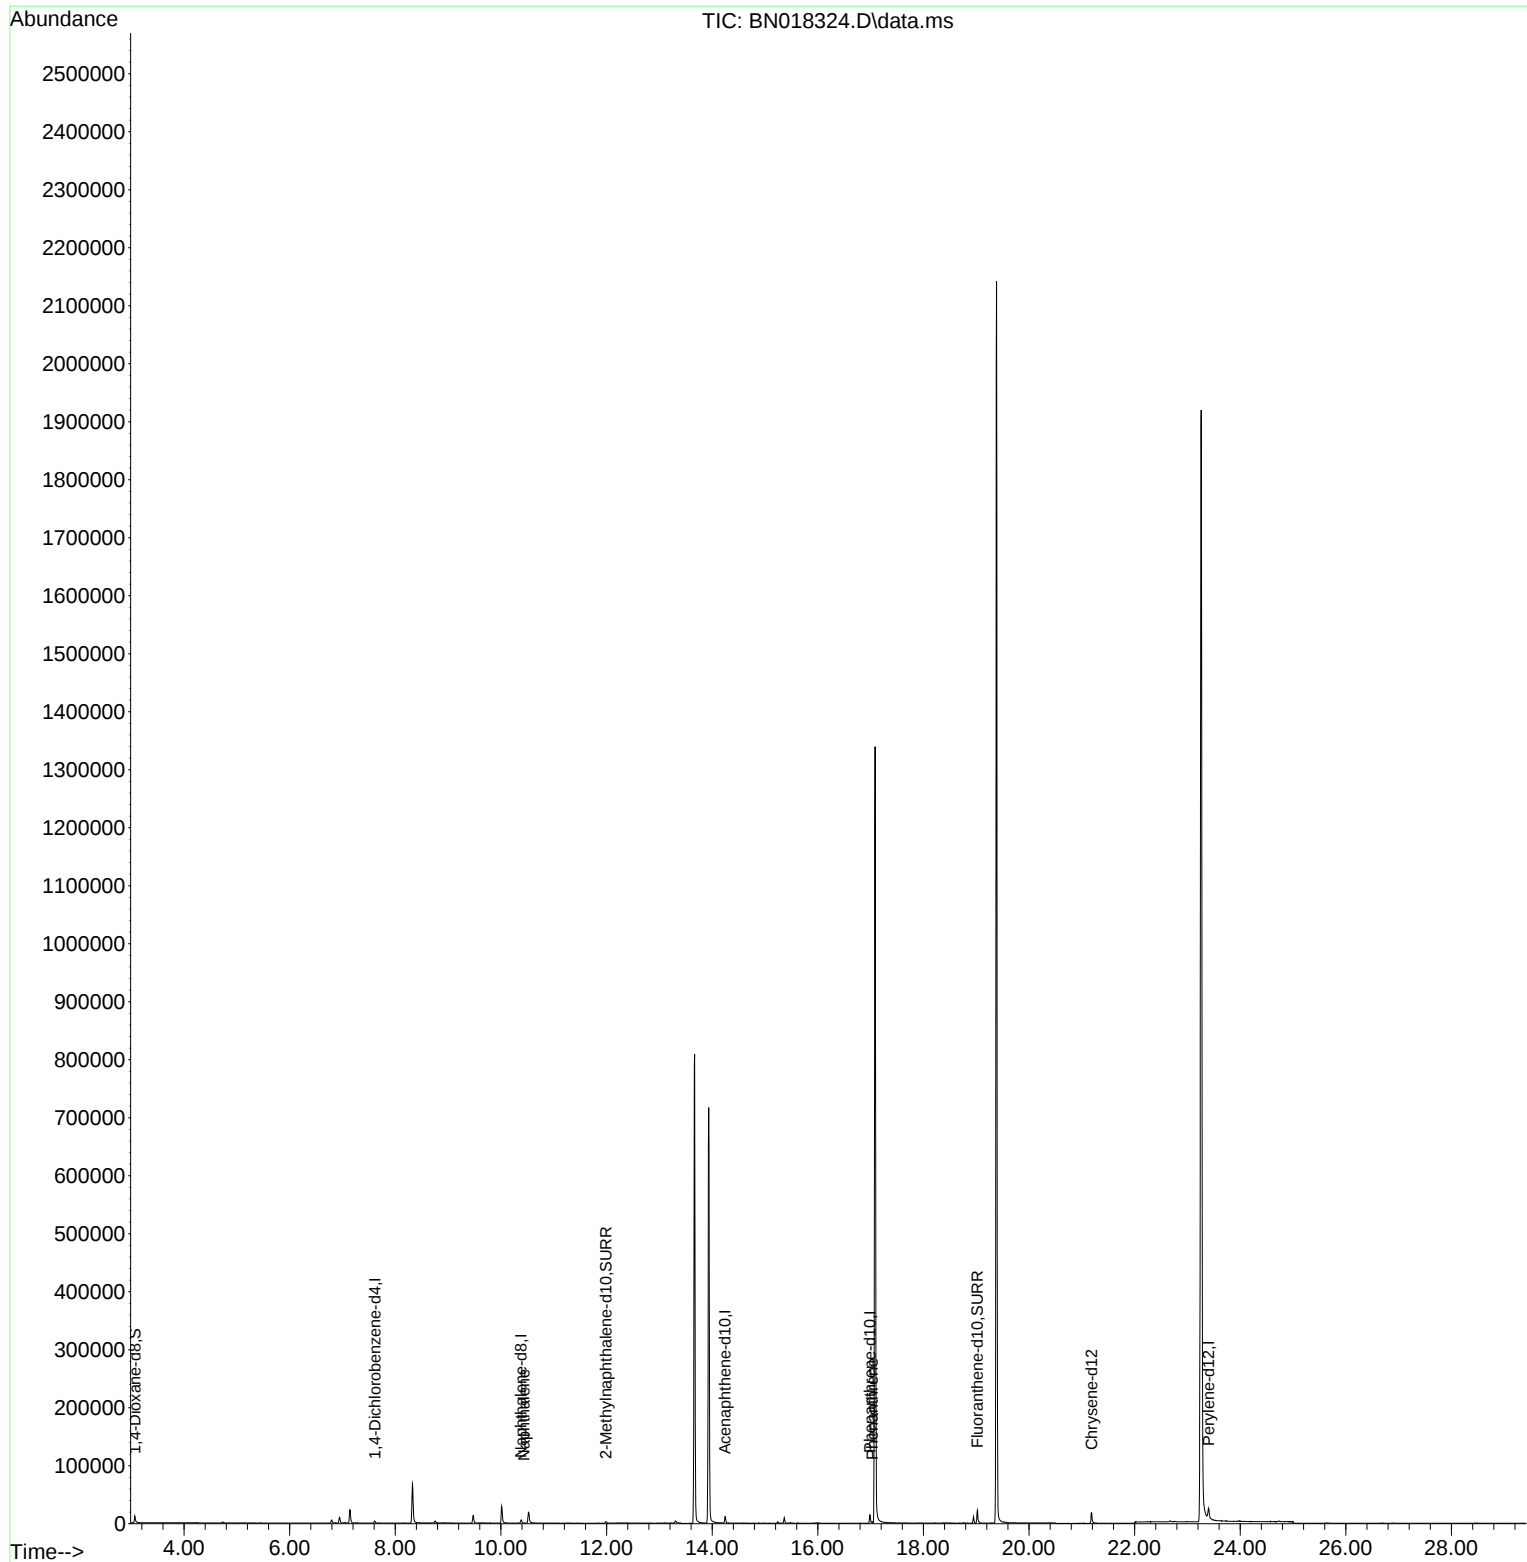


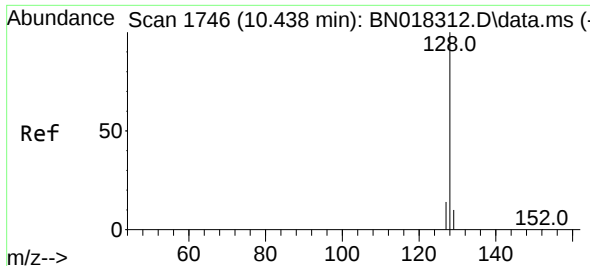

#5
Naphthalene
Concen: 0.021 ng/ul
RT: 10.438 min Scan# 11
Delta R.T. 0.001 min
Lab File: BN018324.D
Acq: 04 Jan 2022 01:03

Instrument :
BNA_N
ClientSampleId :
BG3D4

Tgt Ion:128 Resp: 471
Ion Ratio Lower Upper
128 100
129 31.6 9.4 14.0#
127 26.6 11.0 16.6#

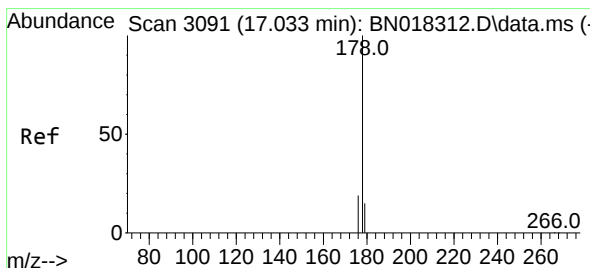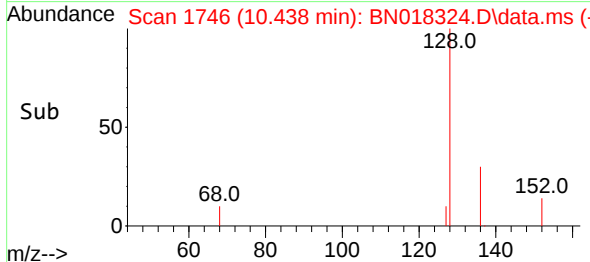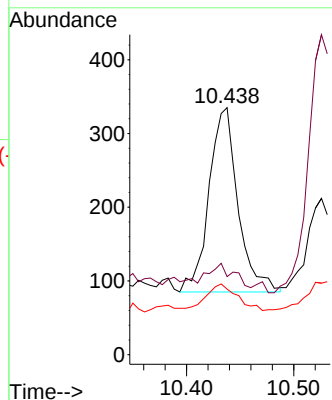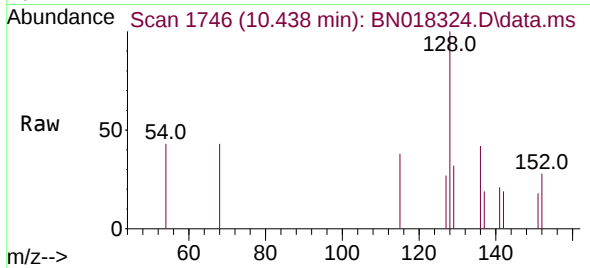

#15
Phenanthrene
Concen: 0.048 ng/ul
RT: 17.029 min Scan# 3090
Delta R.T. -0.003 min
Lab File: BN018324.D
Acq: 04 Jan 2022 01:03

Tgt Ion:178 Resp: 2631
Ion Ratio Lower Upper
178 100
179 22.5 12.2 18.4#
176 22.6 15.4 23.2

