
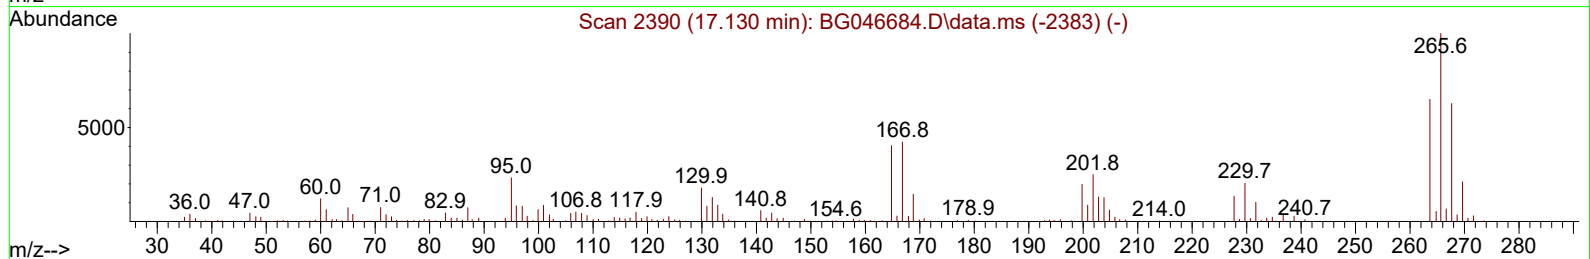
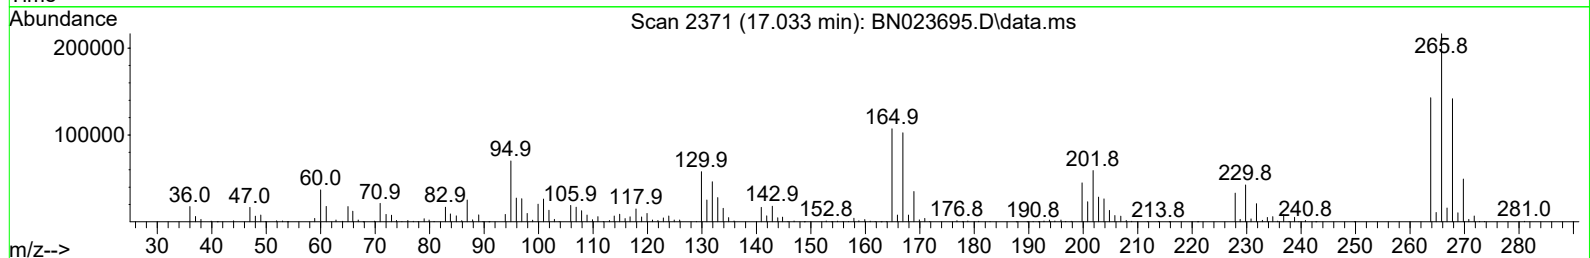


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011823\
Data File : BN023695.D
Acq On : 18 Jan 2023 09:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 07:41:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 07:41:16 2023
Response via : Initial Calibration

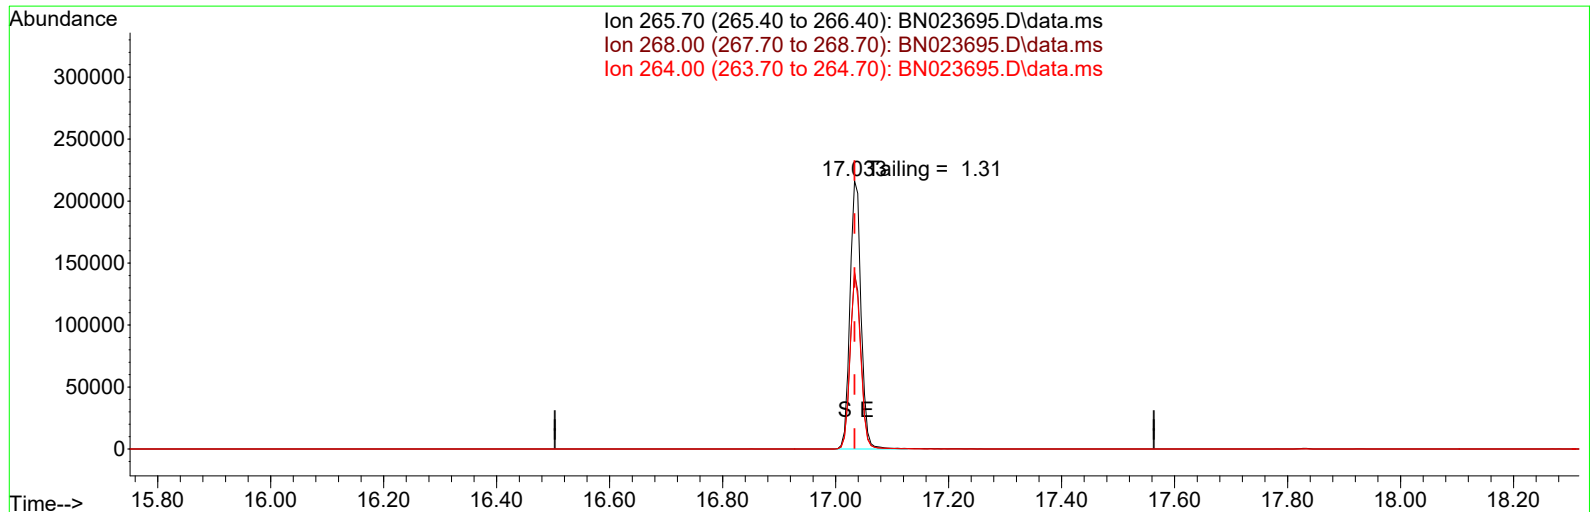

TIC: BN023695.D\data.ms

(70) Pentachlorophenol (C)




17.033min (0.000) 21464.10 ng

response 296463

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.47
264.00	61.60	66.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011823\
Data File : BN023695.D
Acq On : 18 Jan 2023 09:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 07:41:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 07:41:16 2023
Response via : Initial Calibration

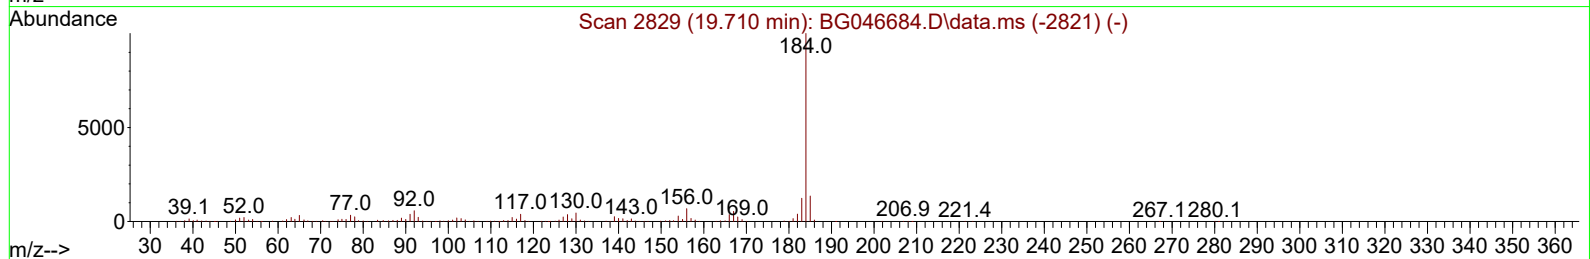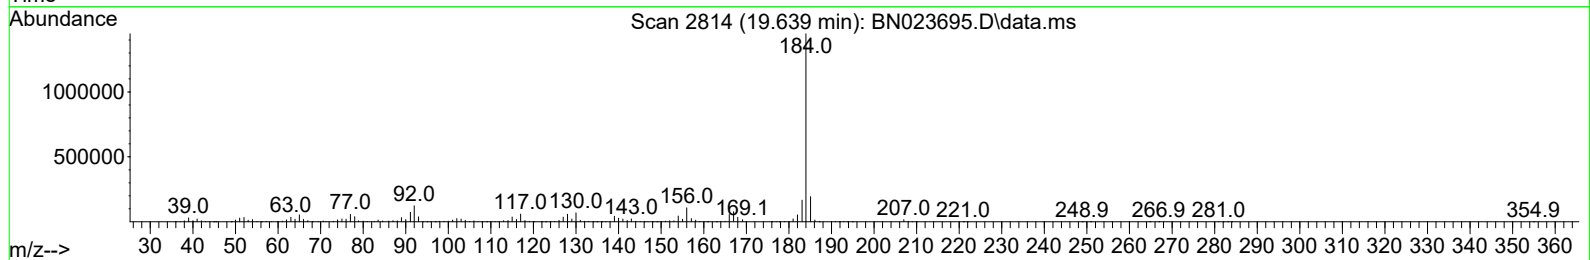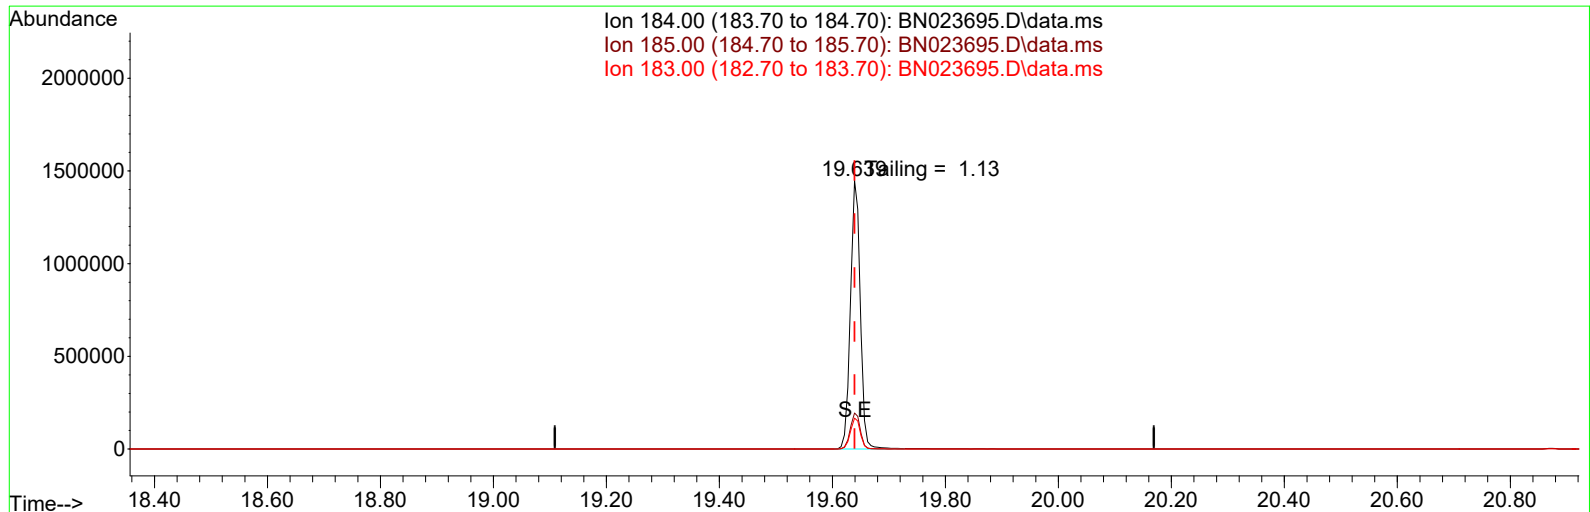

TIC: BN023695.D\data.ms

(77) Benzidine

19.639min (0.000) 59887.65 ng

response 1750064

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.40
183.00	13.20	11.53
0.00	0.00	0.00