
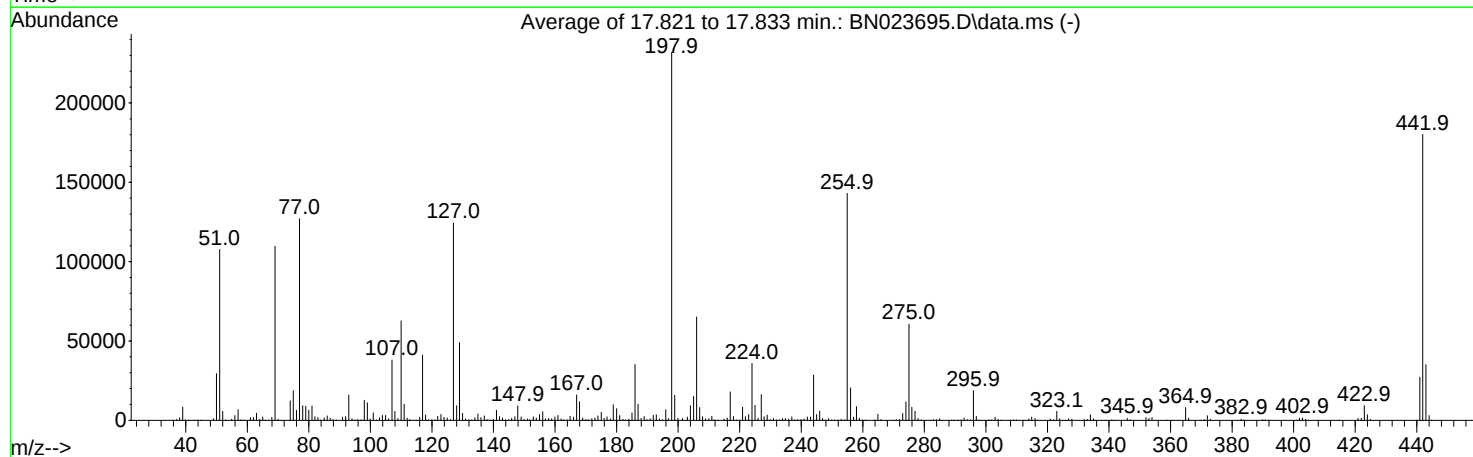


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011823\
 Data File : BN023695.D
 Acq On : 18 Jan 2023 09:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN011823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 19 01:19:57 2023

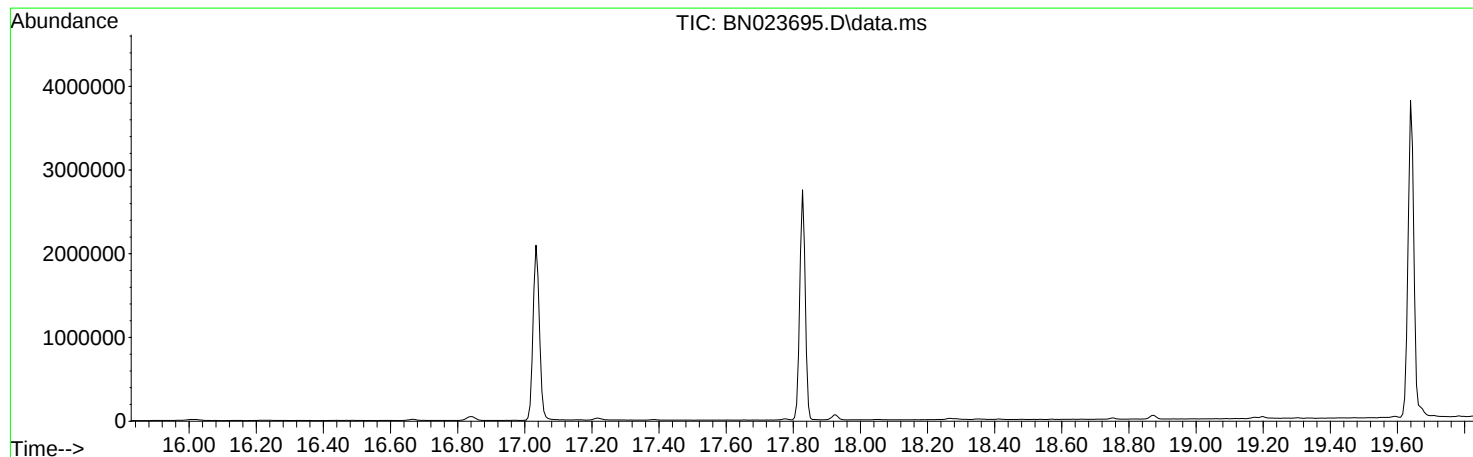




AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.4	107632	PASS
68	69	0.00	2	1.7	1894	PASS
69	198	0.00	100	47.3	109664	PASS
70	69	0.00	2	0.6	679	PASS
127	198	10	80	53.7	124443	PASS
197	198	0.00	2	0.5	1129	PASS
198	198	100	100	100.0	231872	PASS
199	198	5	9	6.8	15758	PASS
275	198	10	60	26.1	60552	PASS
365	198	1	100	3.5	8069	PASS
441	198	0.01	100	11.7	27176	PASS
442	442	50	100	100.0	180155	PASS
443	442	15	24	19.5	35053	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011823\
Data File : BN023695.D
Acq On : 18 Jan 2023 09:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 19 07:41:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 07:41:16 2023
Response via : Initial Calibration

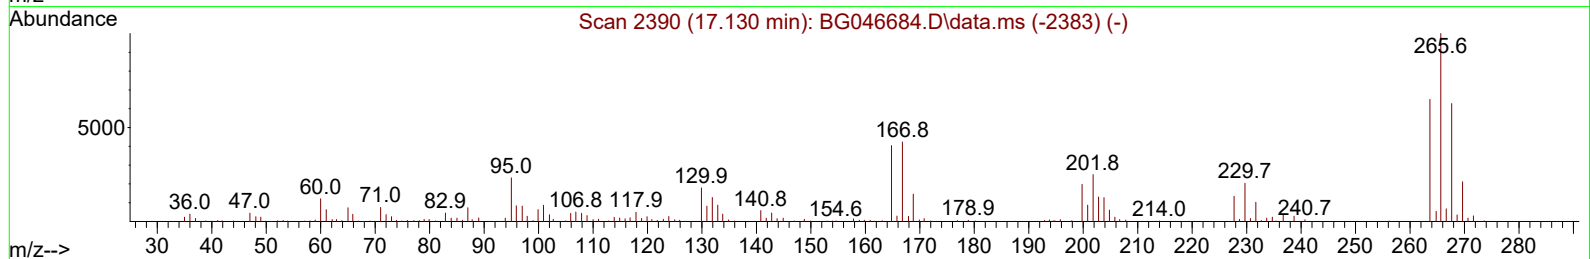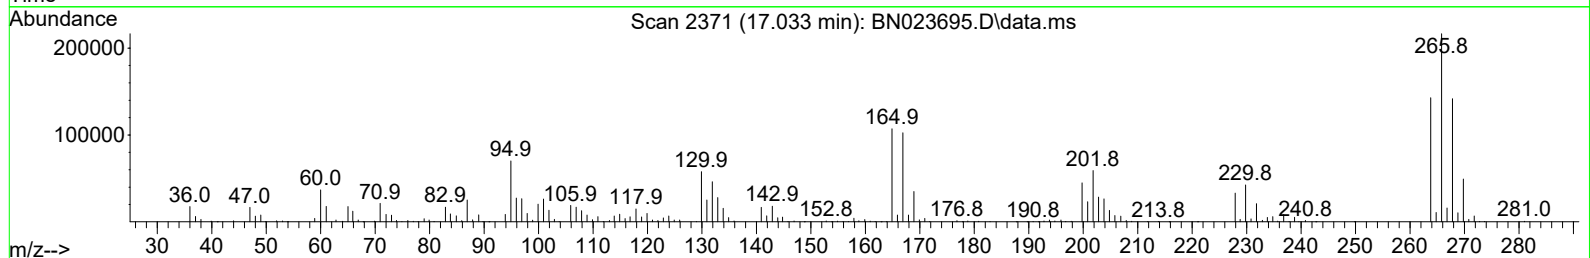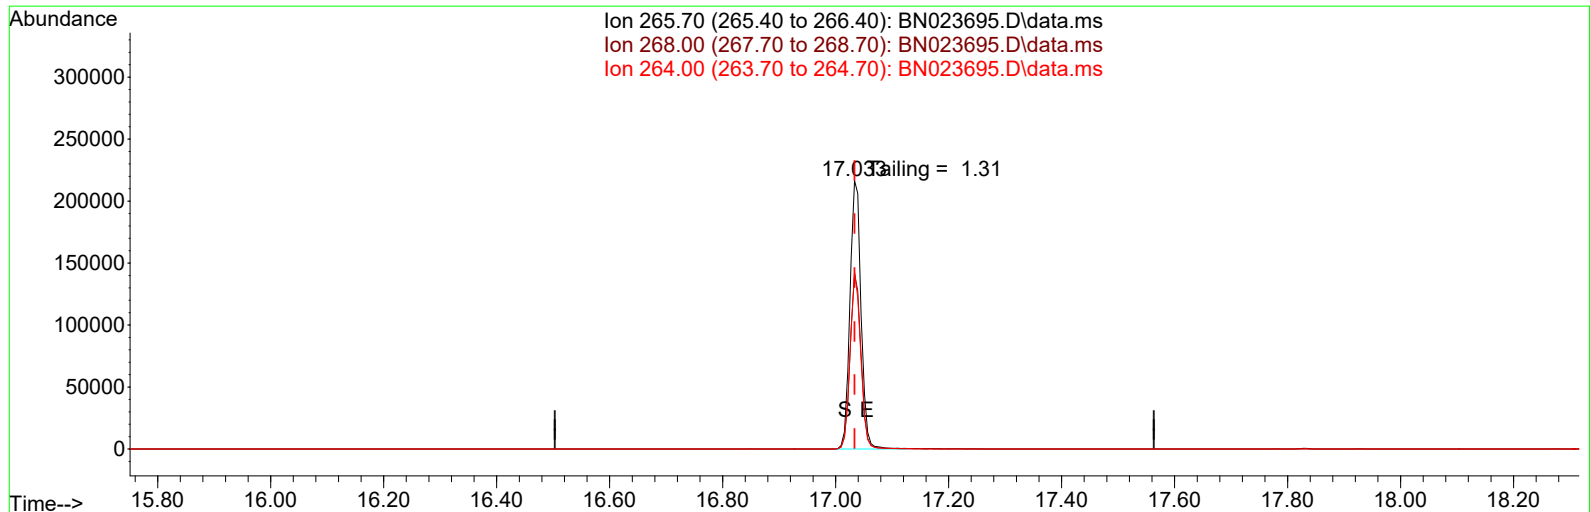

TIC: BN023695.D\data.ms

(70) Pentachlorophenol (C)

17.033min (0.000) 21464.10 ng




response 296463

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.47
264.00	61.60	66.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011823\
Data File : BN023695.D
Acq On : 18 Jan 2023 09:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 19 07:41:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 07:41:16 2023
Response via : Initial Calibration

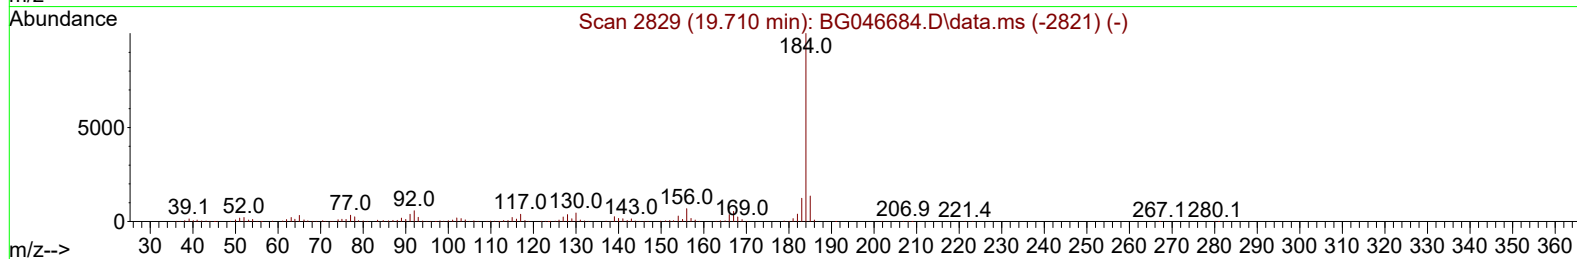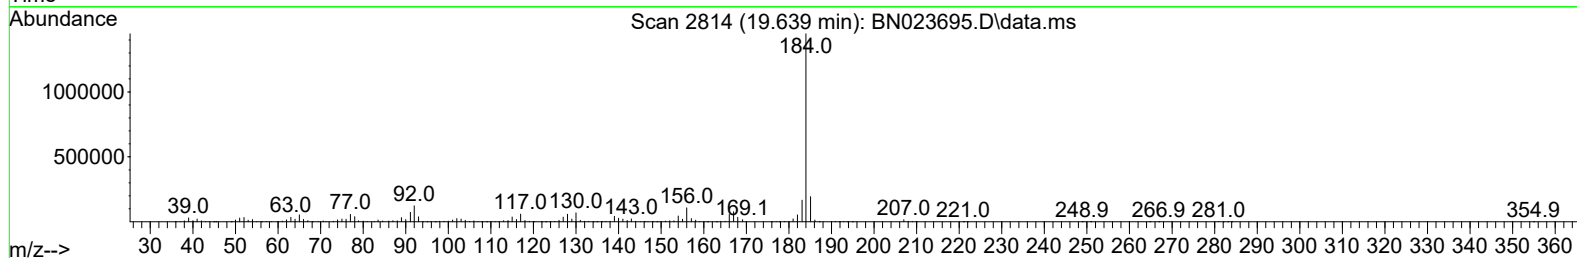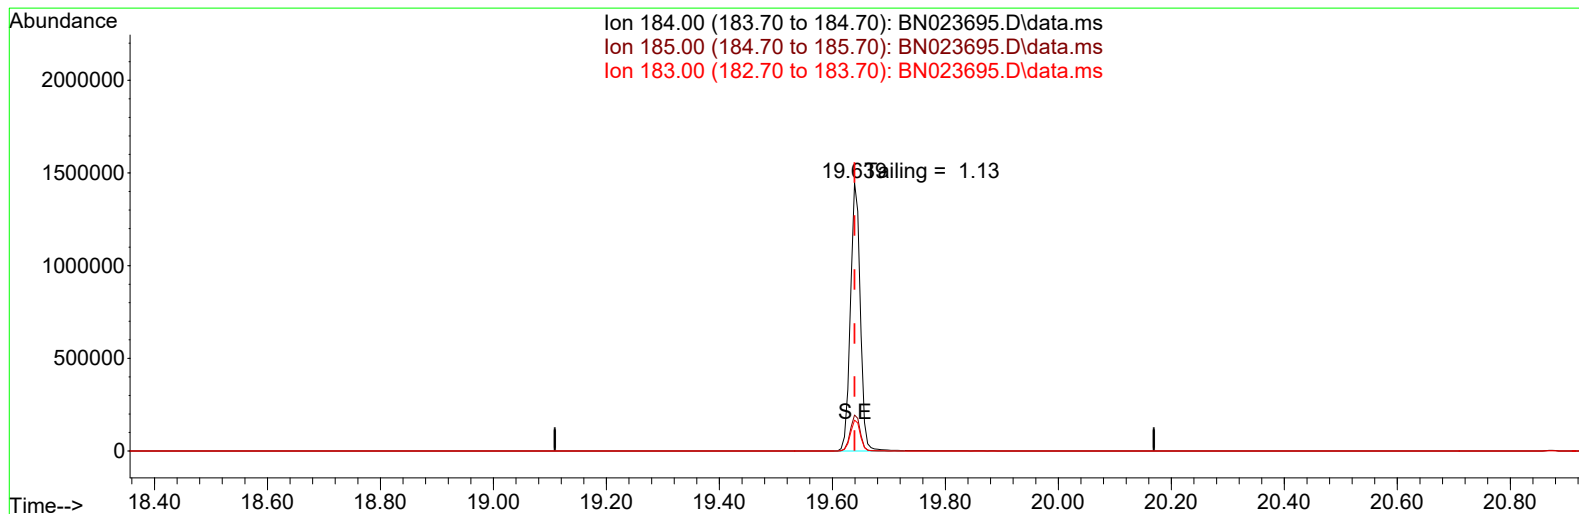

TIC: BN023695.D\data.ms

(77) Benzidine

19.639min (0.000) 59887.65 ng

response 1750064

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.40
183.00	13.20	11.53
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/18/2023	BNA_N	<u>BN023695.D</u>
Compound Name	Response	Retention Time
DDT	886840	20.874
DDD	28081	20.433
DDE	2023	19.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30104	916944	3.28

Instrument :
BNA_N
ClientSampleId :
DFTPP