




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011922\
Data File : BN018418.D
Acq On : 19 Jan 2022 15:40
Operator : CG/JU
Sample : N1129-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBM01

Manual IntegrationsAPPROVED

Quant Time: Jan 20 02:34:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 07 01:31:51 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/20/2022
Supervised By :mohammad ahmed 01/21/2022

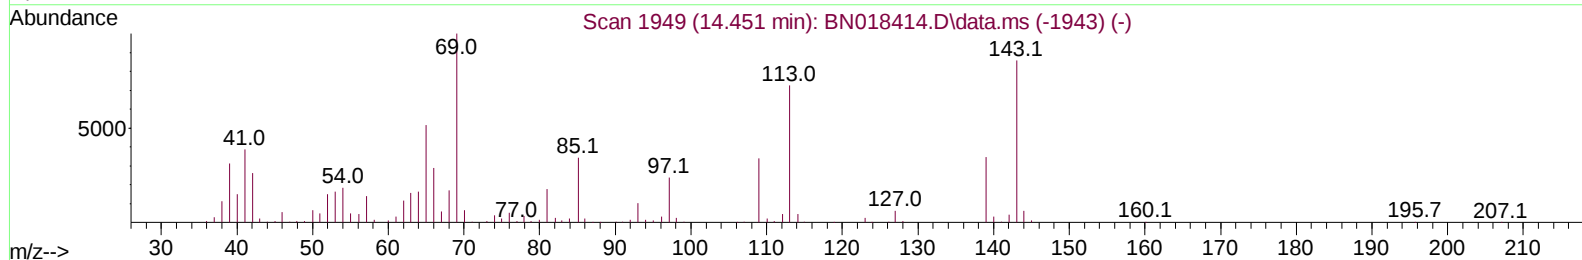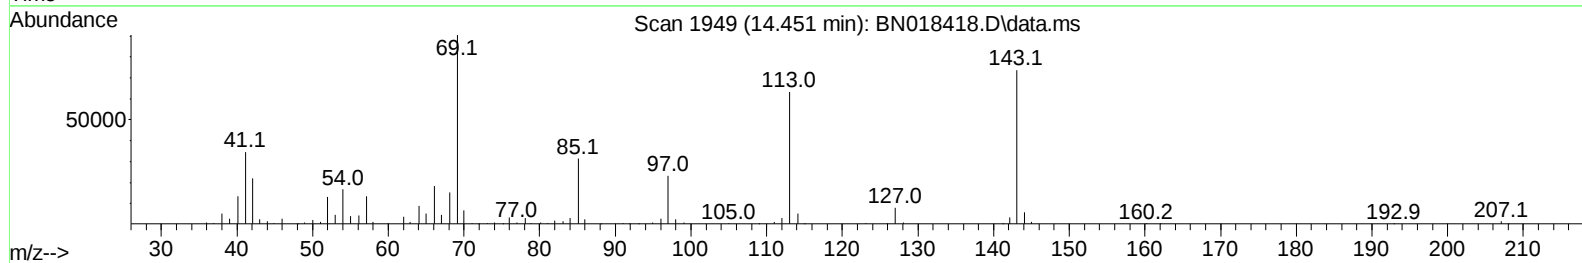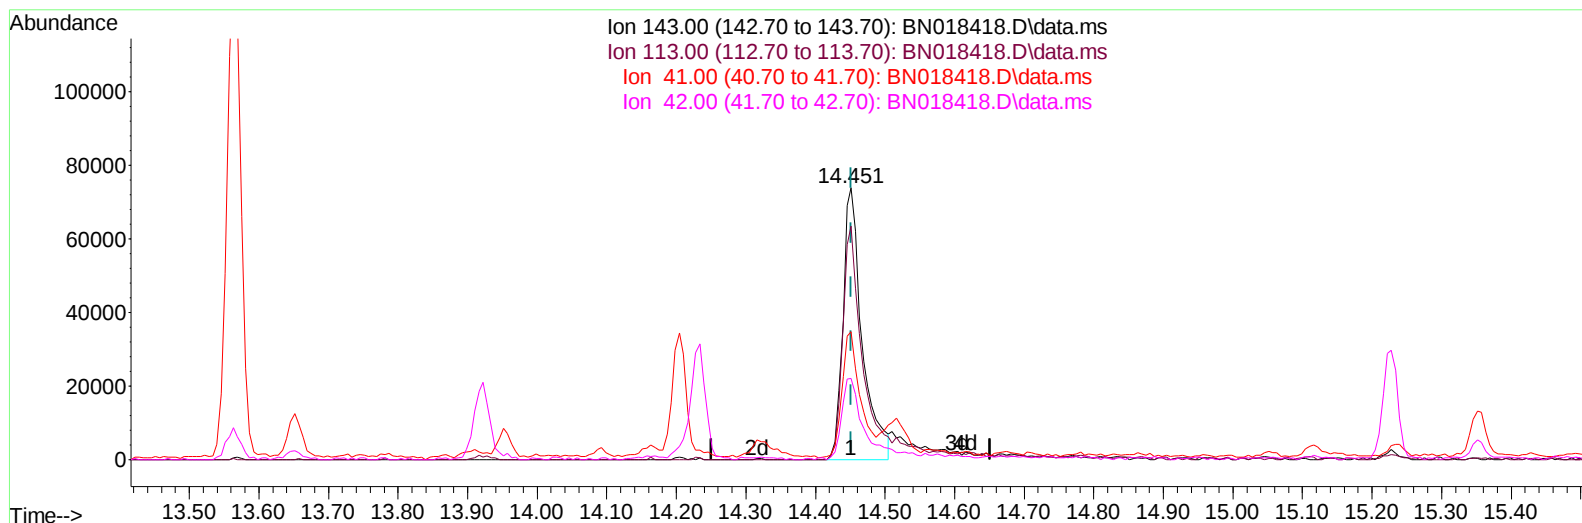

TIC: BN018418.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.451min (+ 0.000) 9.07 ng/u1

response 141700

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.00	85.97
41.00	43.80	46.97
42.00	29.00	29.85




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011922\
Data File : BN018418.D
Acq On : 19 Jan 2022 15:40
Operator : CG/JU
Sample : N1129-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBM01

Manual IntegrationsAPPROVED

Quant Time: Jan 20 02:34:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 07 01:31:51 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/20/2022
Supervised By :mohammad ahmed 01/21/2022

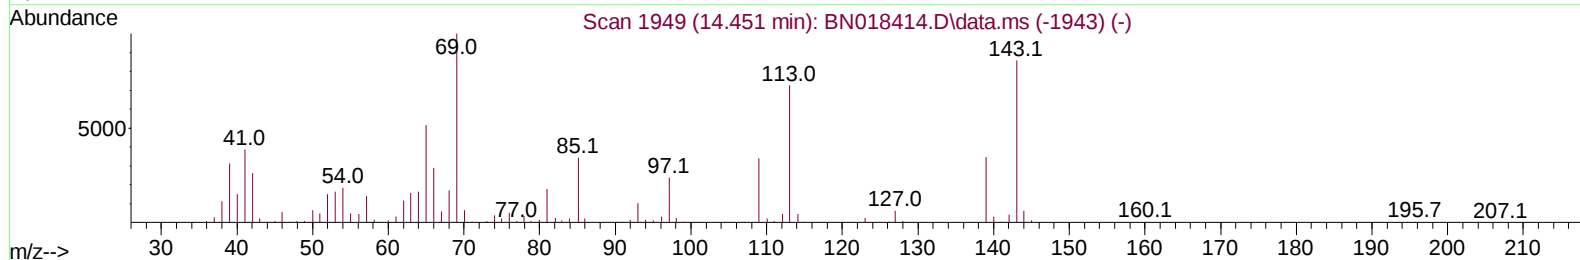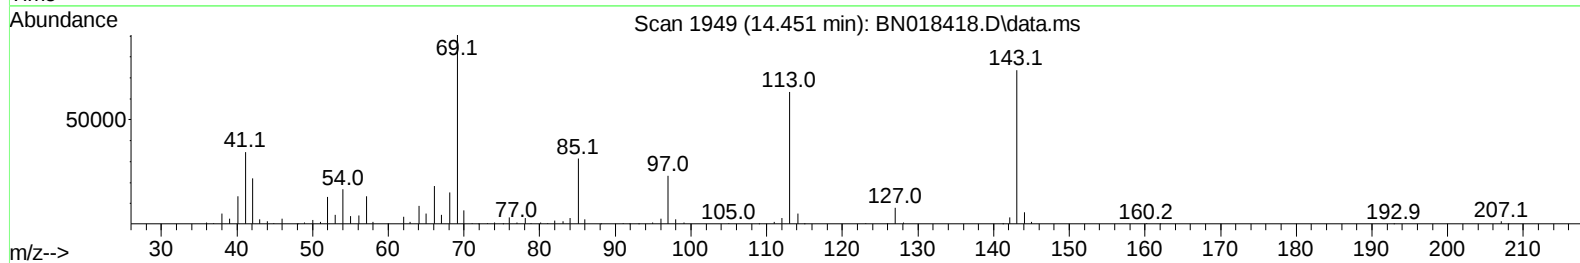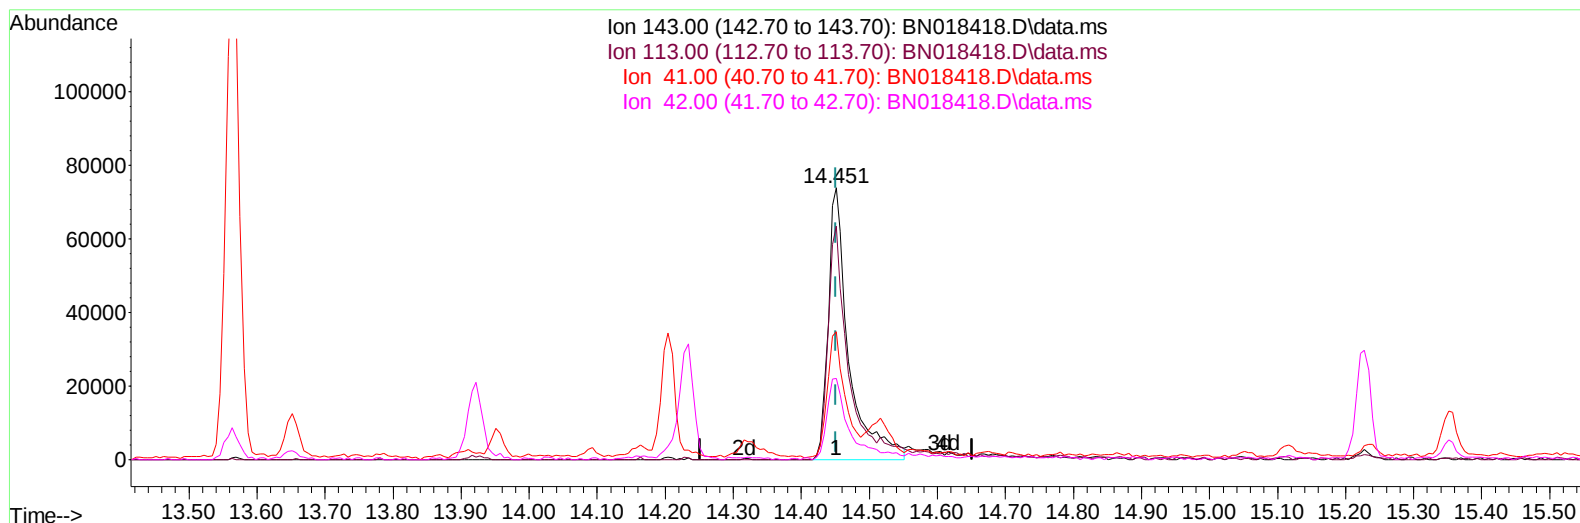

TIC: BN018418.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.451min (+ 0.000) 9.96 ng/ul m

response 155546

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.00	85.97
41.00	43.80	46.97
42.00	29.00	29.85

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011922\
 Data File : BN018418.D
 Acq On : 19 Jan 2022 15:40
 Operator : CG/JU
 Sample : N1129-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBM01

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/20/2022
 Supervised By :mohammad ahmed 01/21/2022

Quant Time: Jan 20 02:34:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 07 01:31:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.587	152	379859	20.000	ng/ul	0.00
20) Naphthalene-d8	10.363	136	1747414	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.234	164	1126714	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.975	188	2250962	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.175	240	2211224	20.000	ng/ul	# 0.00
88) Perylene-d12	23.392	264	2153404	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.064	96	28706	3.038	ng/uL	0.00
4) Pyridine-d5	3.470	84	189595	6.411	ng/ul	0.00
7) Phenol-d5	6.775	99	590153	15.986	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.928	67	412719	17.550	ng/ul	0.00
11) 2-Chlorophenol-d4	7.122	132	481471	17.805	ng/ul	0.00
15) 4-Methylphenol-d8	8.305	113	417248	14.319	ng/ul	-0.01
21) Nitrobenzene-d5	8.734	128	232560	17.869	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.458	143	263603	18.948	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.999	165	450905	17.840	ng/ul	0.00
31) 4-Chloroaniline-d4	10.505	131	559432	14.402	ng/ul	-0.01
46) Dimethylphthalate-d6	13.651	166	1636163	19.993	ng/ul	0.00
49) Acenaphthylene-d8	13.922	160	2034412	19.665	ng/ul	0.00
54) 4-Nitrophenol-d4	14.451	143	155546m	9.960	ng/ul	0.00
60) Fluorene-d10	15.228	176	1407626	20.387	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.351	200	172314	13.529	ng/ul	-0.01
73) Anthracene-d10	17.075	188	2128852	20.420	ng/ul	0.00
81) Pyrene-d10	19.375	212	2538801	20.015	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.251	264	2331981	21.759	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011922\
Data File : BN018418.D
Acq On : 19 Jan 2022 15:40
Operator : CG/JU
Sample : N1129-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBM01

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/20/2022
Supervised By :mohammad ahmed 01/21/2022

Quant Time: Jan 20 02:34:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 07 01:31:51 2022
Response via : Initial Calibration

