




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011922\
Data File : BN018421.D
Acq On : 19 Jan 2022 17:27
Operator : CG/JU
Sample : N1129-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBM05

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/20/2022
Supervised By :mohammad ahmed 01/21/2022

Quant Time: Jan 20 02:35:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 07 01:31:51 2022
Response via : Initial Calibration

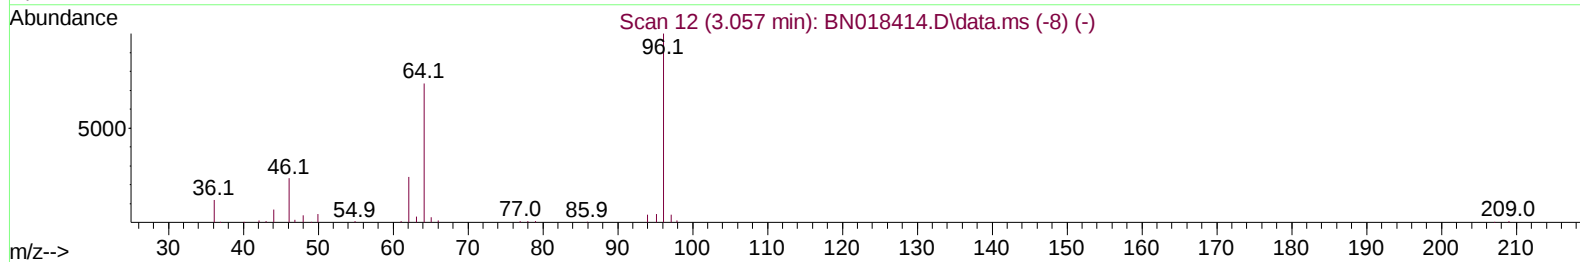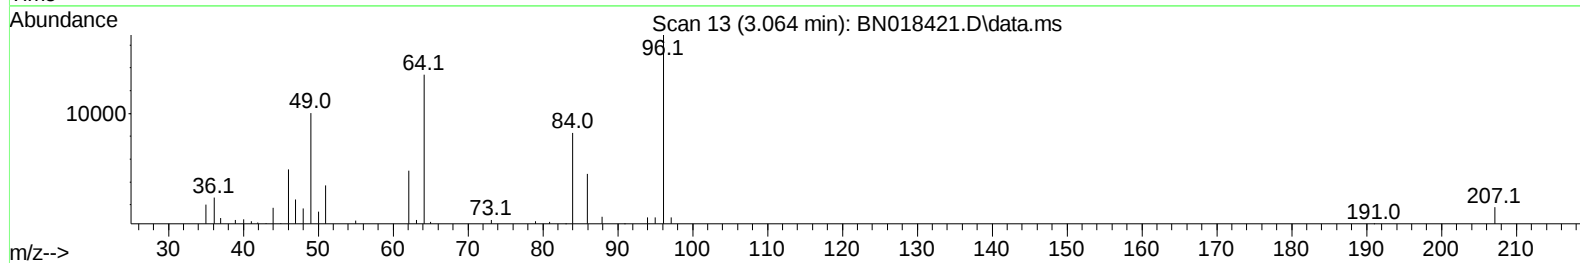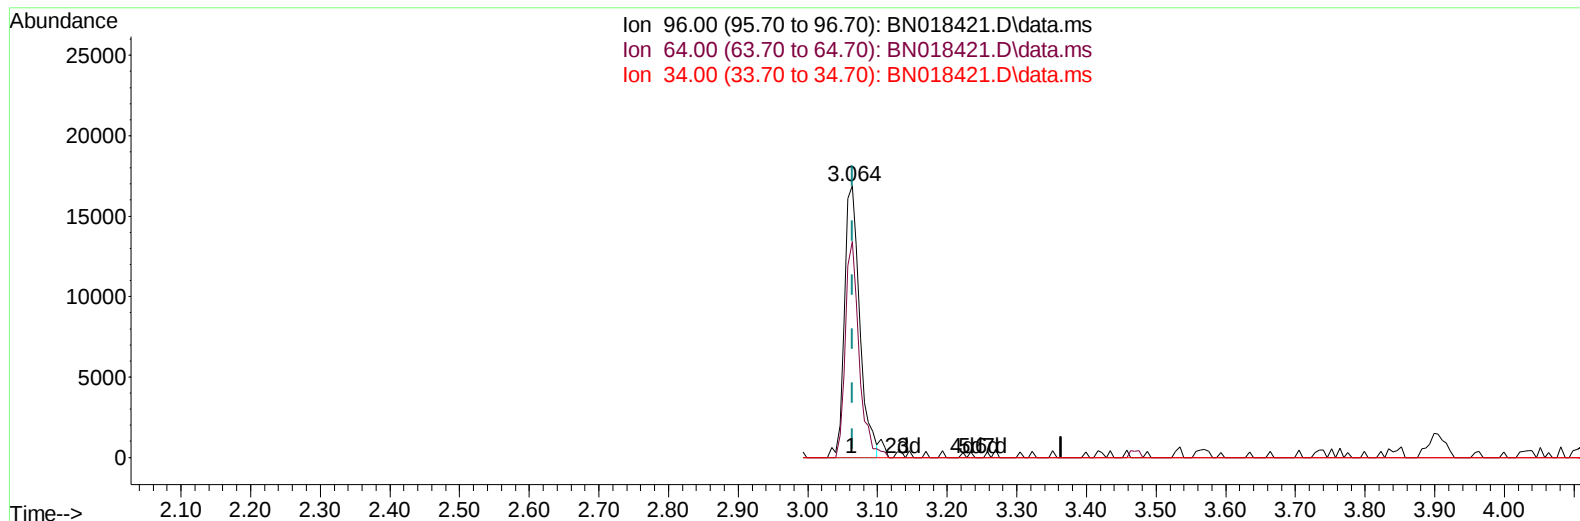

TIC: BN018421.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.064min (-0.000) 2.55 ng/uL

response 25727

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	73.80	79.53
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011922\
 Data File : BN018421.D
 Acq On : 19 Jan 2022 17:27
 Operator : CG/JU
 Sample : N1129-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBM05

Manual IntegrationsAPPROVED

Quant Time: Jan 20 02:35:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 07 01:31:51 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/20/2022
 Supervised By :mohammad ahmed 01/21/2022

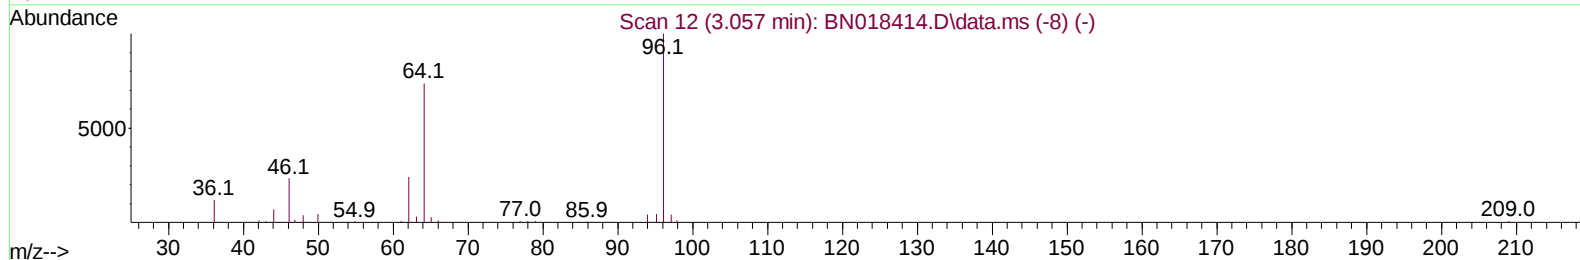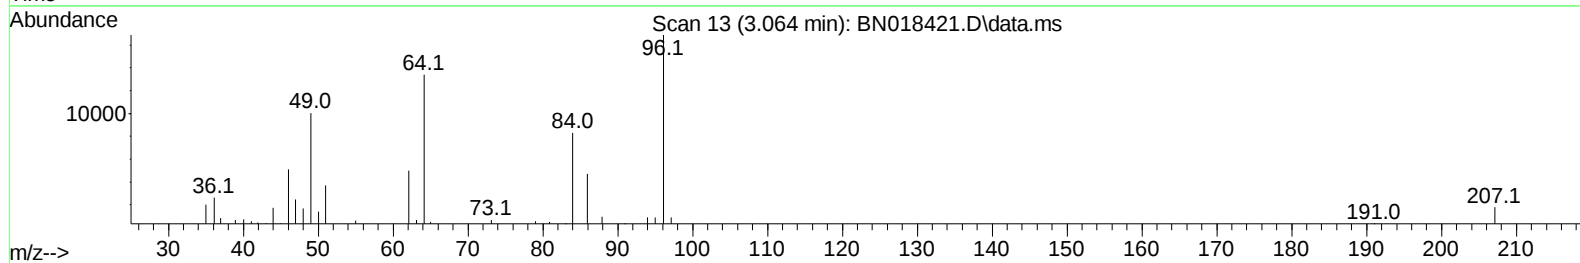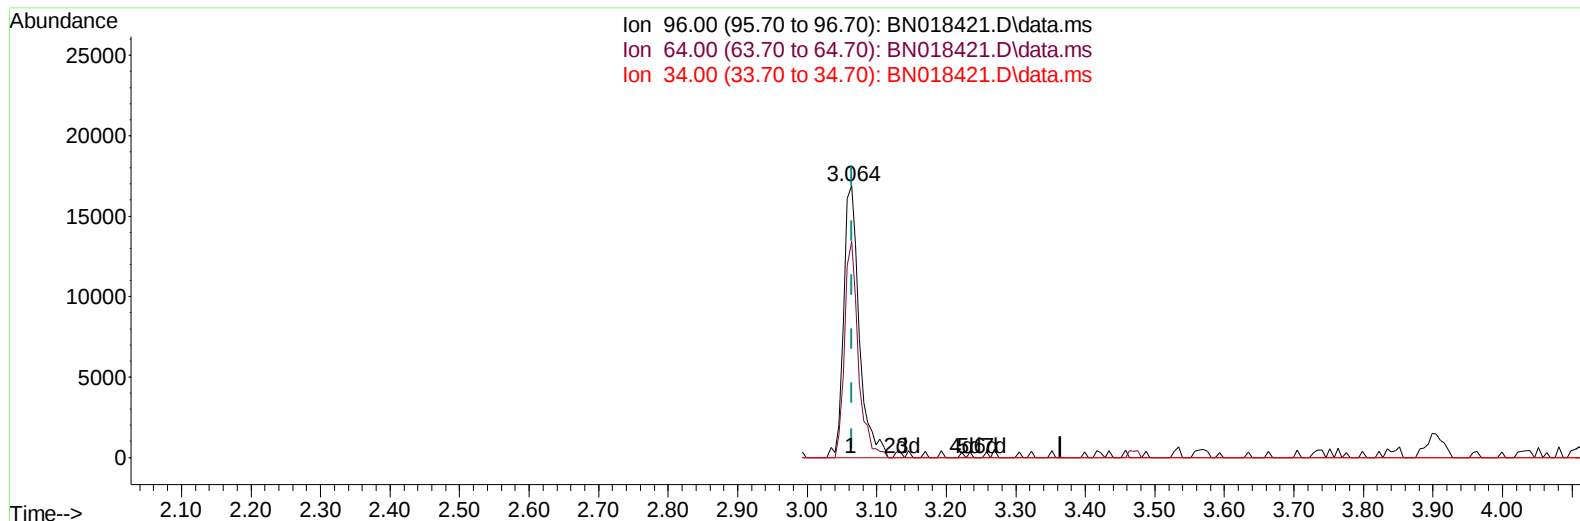

TIC: BN018421.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.064min (-0.000) 2.62 ng/uL m

response 26346

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	73.80	79.53
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011922\
 Data File : BN018421.D
 Acq On : 19 Jan 2022 17:27
 Operator : CG/JU
 Sample : N1129-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBM05

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/20/2022
 Supervised By :mohammad ahmed 01/21/2022

Quant Time: Jan 20 02:35:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 07 01:31:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.587	152	404974	20.000	ng/ul	0.00
20) Naphthalene-d8	10.369	136	1839786	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.234	164	1215614	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.975	188	2433126	20.000	ng/ul	0.00
79) Chrysene-d12	21.168	240	2362339	20.000	ng/ul	#-0.01
88) Perylene-d12	23.386	264	2248501	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.064	96	26346m	2.615	ng/uL	0.00
4) Pyridine-d5	3.469	84	203805	6.464	ng/ul	0.00
7) Phenol-d5	6.775	99	570738	14.501	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.928	67	387476	15.455	ng/ul	0.00
11) 2-Chlorophenol-d4	7.122	132	464797	16.122	ng/ul	0.00
15) 4-Methylphenol-d8	8.304	113	458975	14.774	ng/ul	-0.01
21) Nitrobenzene-d5	8.734	128	222192	16.215	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.457	143	241332	16.476	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.998	165	415217	15.603	ng/ul	0.00
31) 4-Chloroaniline-d4	10.504	131	579171	14.161	ng/ul	-0.01
46) Dimethylphthalate-d6	13.651	166	1532469	17.356	ng/ul	0.00
49) Acenaphthylene-d8	13.922	160	1841170	16.495	ng/ul	0.00
54) 4-Nitrophenol-d4	14.451	143	138096	8.196	ng/ul	0.00
60) Fluorene-d10	15.228	176	1289881	17.315	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.357	200	148455	10.783	ng/ul	0.00
73) Anthracene-d10	17.075	188	2031095	18.024	ng/ul	0.00
81) Pyrene-d10	19.374	212	2453618	18.106	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.251	264	2189424	19.565	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011922\
Data File : BN018421.D
Acq On : 19 Jan 2022 17:27
Operator : CG/JU
Sample : N1129-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBM05

Manual IntegrationsAPPROVED

Quant Time: Jan 20 02:35:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 07 01:31:51 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/20/2022
Supervised By :mohammad ahmed 01/21/2022

