




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011922\
Data File : BN018425.D
Acq On : 19 Jan 2022 20:26
Operator : CG/JU
Sample : PB142087BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK087

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/20/2022
Supervised By :mohammad ahmed 01/21/2022

Quant Time: Jan 20 02:38:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 07 01:31:51 2022
Response via : Initial Calibration

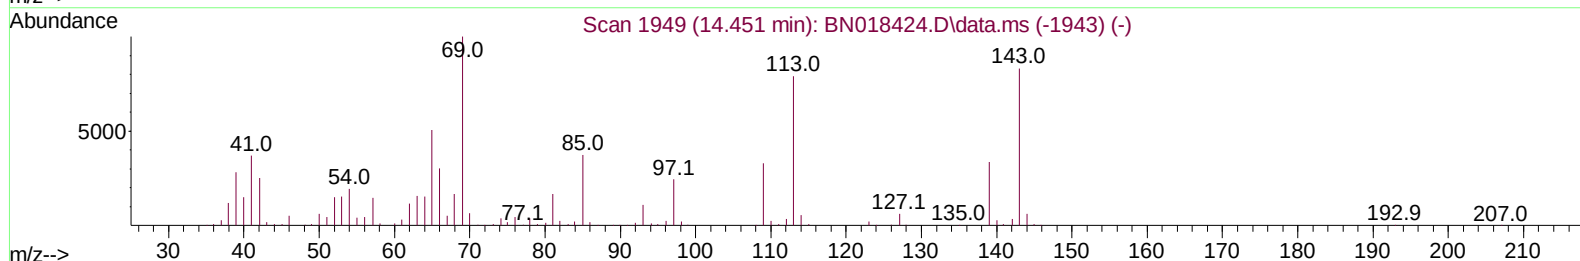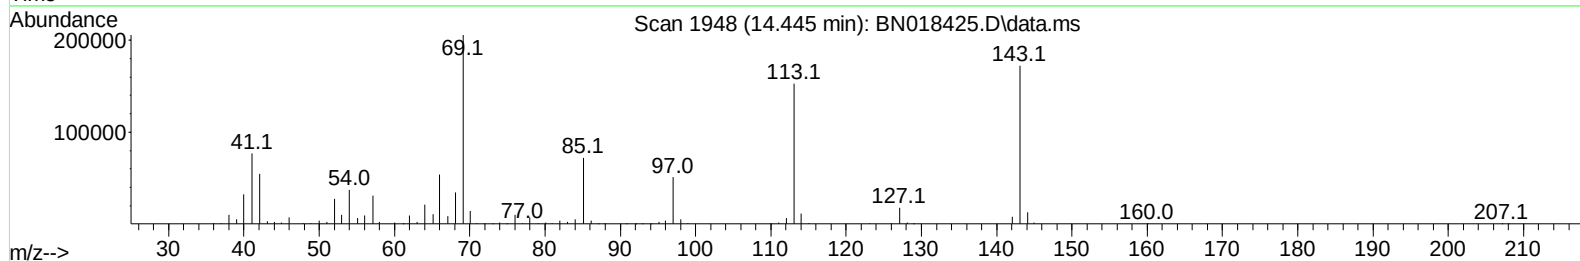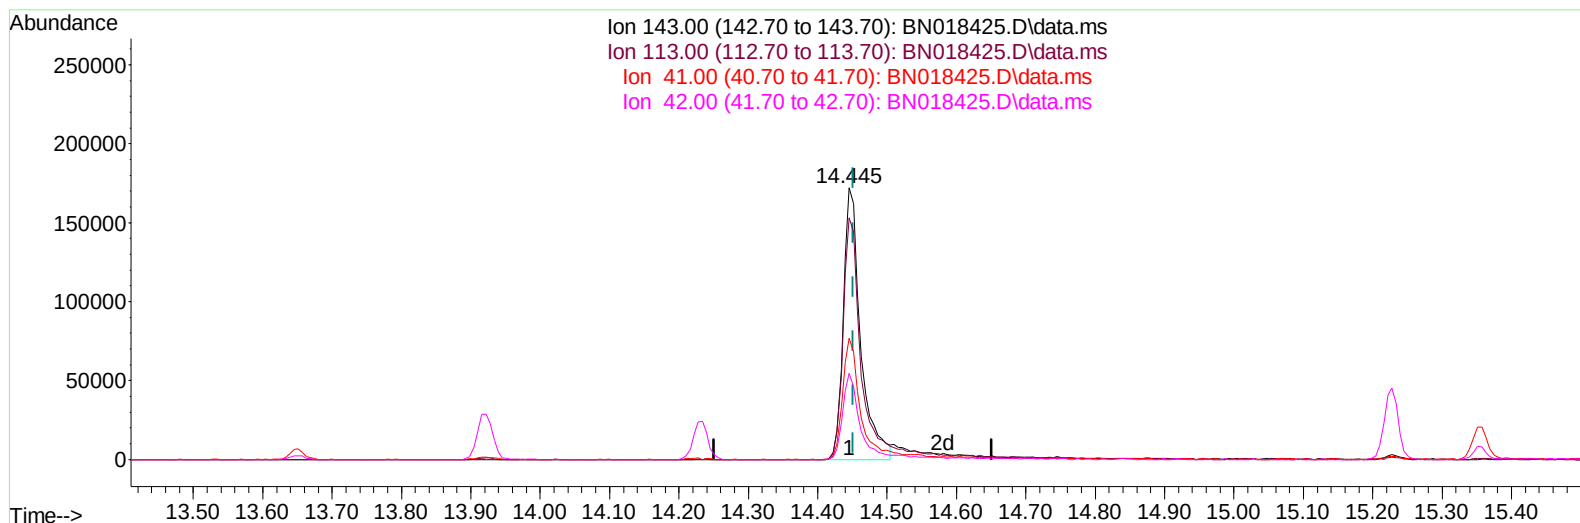

TIC: BN018425.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.445min (-0.006) 24.21 ng/ul

response 300052

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.00	88.95
41.00	43.80	44.69
42.00	29.00	31.77




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011922\
Data File : BN018425.D
Acq On : 19 Jan 2022 20:26
Operator : CG/JU
Sample : PB142087BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK087

Manual IntegrationsAPPROVED

Quant Time: Jan 20 02:38:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 07 01:31:51 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/20/2022
Supervised By :mohammad ahmed 01/21/2022

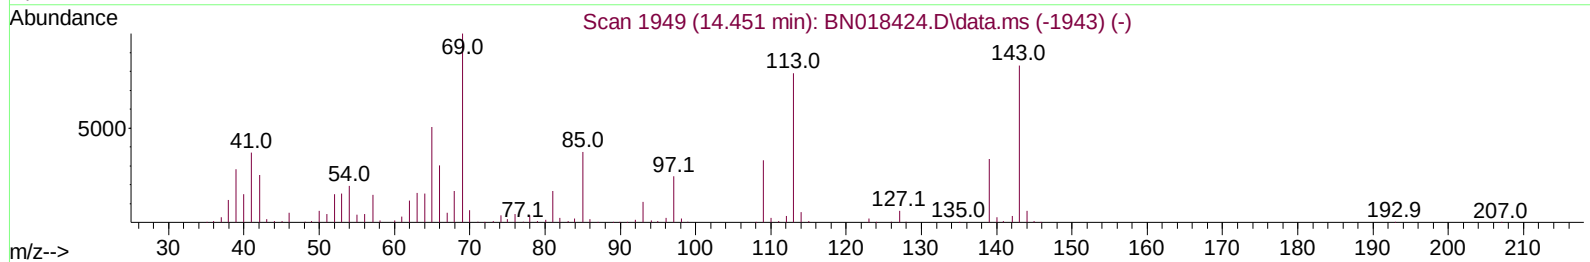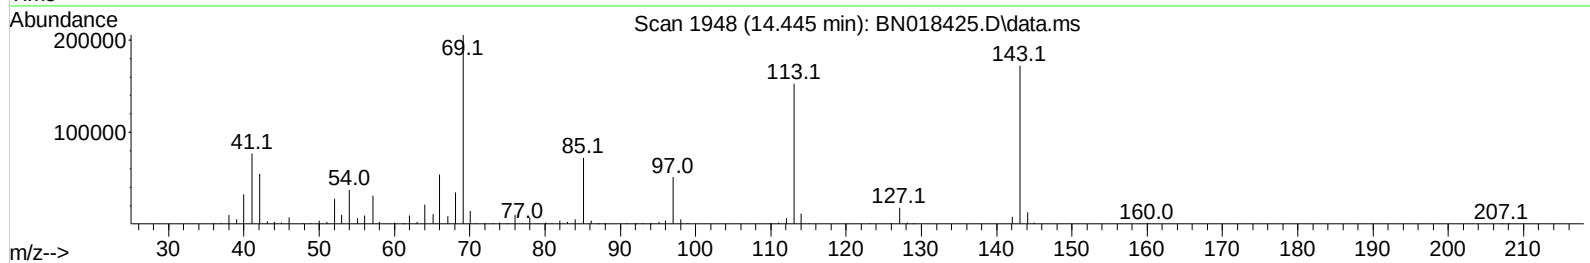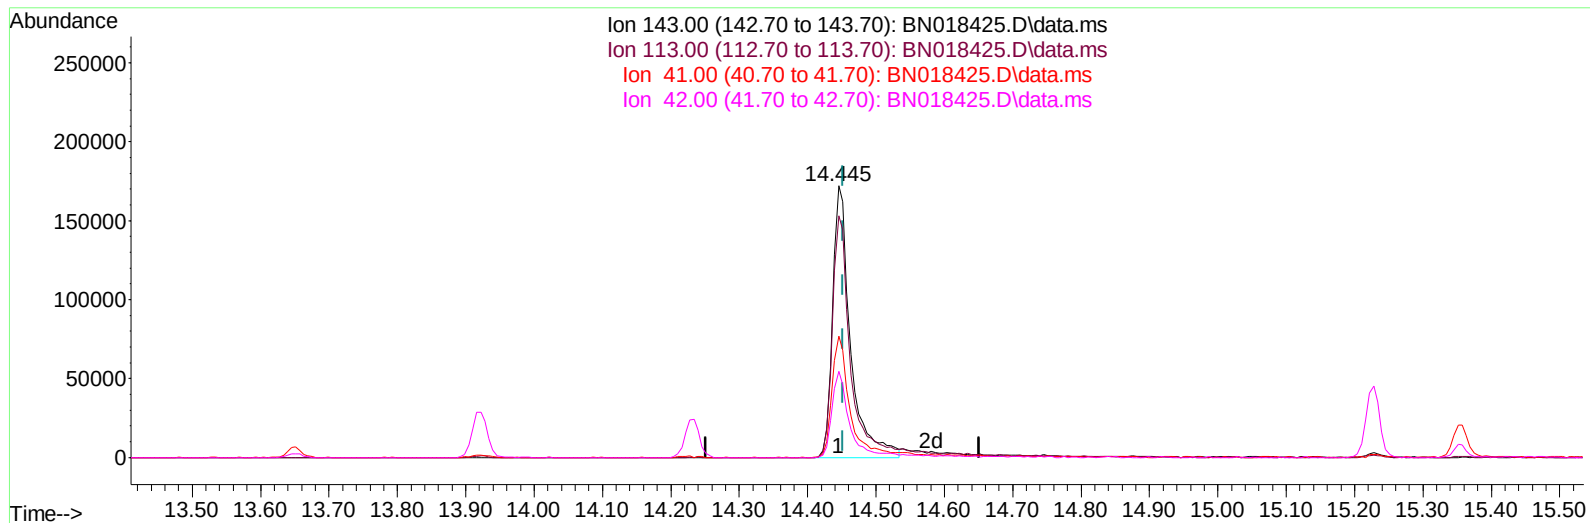

TIC: BN018425.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.445min (-0.006) 25.23 ng/ul m

response 312725

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	78.00	88.95
41.00	43.80	44.69
42.00	29.00	31.77

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011922\
 Data File : BN018425.D
 Acq On : 19 Jan 2022 20:26
 Operator : CG/JU
 Sample : PB142087BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK087

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/20/2022
 Supervised By :mohammad ahmed 01/21/2022

Quant Time: Jan 20 02:38:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 07 01:31:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.587	152	310637	20.000	ng/ul	0.00
20) Naphthalene-d8	10.369	136	1418526	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.234	164	894126	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.975	188	1814346	20.000	ng/ul	0.00
79) Chrysene-d12	21.174	240	1724867	20.000	ng/ul	# 0.00
88) Perylene-d12	23.392	264	1504961	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.064	96	40964	5.301	ng/uL	0.00
4) Pyridine-d5	3.464	84	713965	29.523	ng/ul	0.00
7) Phenol-d5	6.775	99	948667	31.423	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.928	67	605469	31.483	ng/ul	0.00
11) 2-Chlorophenol-d4	7.122	132	762763	34.492	ng/ul	0.00
15) 4-Methylphenol-d8	8.305	113	781046	32.776	ng/ul	-0.01
21) Nitrobenzene-d5	8.740	128	371140	35.128	ng/ul	0.00
24) 2-Nitrophenol-d4	9.457	143	434281	38.454	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.999	165	687907	33.527	ng/ul	0.00
31) 4-Chloroaniline-d4	10.504	131	1066587	33.824	ng/ul	-0.01
46) Dimethylphthalate-d6	13.651	166	2311503	35.593	ng/ul	0.00
49) Acenaphthylene-d8	13.922	160	2872946	34.994	ng/ul	0.00
54) 4-Nitrophenol-d4	14.445	143	312725m	25.234	ng/ul	0.00
60) Fluorene-d10	15.228	176	1931093	35.243	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.357	200	282504	27.517	ng/ul	0.00
73) Anthracene-d10	17.075	188	2957912	35.201	ng/ul	0.00
81) Pyrene-d10	19.375	212	3339104	33.747	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.251	264	2901073	38.733	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011922\
Data File : BN018425.D
Acq On : 19 Jan 2022 20:26
Operator : CG/JU
Sample : PB142087BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK087

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/20/2022
Supervised By :mohammad ahmed 01/21/2022

Quant Time: Jan 20 02:38:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 07 01:31:51 2022
Response via : Initial Calibration

