

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011922\
 Data File : BN018421.D
 Acq On : 19 Jan 2022 17:27
 Operator : CG/JU
 Sample : N1129-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBM05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.064	9	13	19	rBV2	52586	76038	1.11%	0.086%
2	3.469	79	82	100	rBV	368916	613860	8.97%	0.697%
3	3.711	118	123	128	rVB2	67588	111862	1.63%	0.127%
4	3.805	135	139	145	rVB	29521	43125	0.63%	0.049%
5	3.899	151	155	160	rVB5	23840	40200	0.59%	0.046%
6	4.034	174	178	183	rVB6	10275	13586	0.20%	0.015%
7	4.175	199	202	207	rVB5	17811	21050	0.31%	0.024%
8	4.711	288	293	303	rVB2	110705	181771	2.66%	0.206%
9	5.987	506	510	517	rVB	18985	29237	0.43%	0.033%
10	6.775	638	644	662	rBV	1088489	1839463	26.87%	2.087%
11	6.928	664	670	681	rBV	906901	1404073	20.51%	1.593%
12	7.122	697	703	714	rBV	1130785	1801674	26.32%	2.044%
13	7.234	718	722	729	rVB4	17740	27848	0.41%	0.032%
14	7.404	746	751	755	rBV3	10134	15438	0.23%	0.018%
15	7.587	775	782	792	rBV	1667578	2623033	38.31%	2.976%
16	7.669	792	796	802	rVB4	10695	20010	0.29%	0.023%
17	8.304	897	904	917	rBV	1291995	2102720	30.71%	2.386%
18	8.410	917	922	928	rVB4	16477	37337	0.55%	0.042%
19	8.740	967	978	989	rBV	1016558	1711746	25.00%	1.942%
20	8.916	1004	1008	1014	rBV8	15062	26885	0.39%	0.031%
21	9.210	1053	1058	1065	rVB2	35254	59711	0.87%	0.068%
22	9.457	1093	1100	1111	rBV	913527	1488788	21.75%	1.689%
23	9.946	1178	1183	1185	rBV5	8699	13593	0.20%	0.015%
24	9.998	1185	1192	1204	rVV	1291120	2172902	31.74%	2.466%
25	10.369	1247	1255	1264	rBV	2388693	3983321	58.18%	4.520%
26	10.504	1271	1278	1302	rBV	1065077	2076936	30.34%	2.357%
27	11.822	1499	1502	1508	rVB7	9693	17817	0.26%	0.020%
28	11.969	1522	1527	1535	rBV3	23828	41804	0.61%	0.047%
29	12.651	1639	1643	1648	rBV4	9871	15120	0.22%	0.017%
30	12.740	1654	1658	1665	rBV6	6626	15300	0.22%	0.017%
31	12.851	1673	1677	1681	rBV4	10712	16108	0.24%	0.018%
32	13.087	1710	1717	1721	rBV2	46230	73594	1.07%	0.084%
33	13.563	1791	1798	1802	rBV6	20284	35339	0.52%	0.040%
34	13.651	1807	1813	1821	rBV	2511542	3551070	51.87%	4.029%
35	13.922	1852	1859	1873	rBV	2862175	4183172	61.10%	4.747%
36	14.163	1896	1900	1905	rVB2	29963	37123	0.54%	0.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011922\
 Data File : BN018421.D
 Acq On : 19 Jan 2022 17:27
 Operator : CG/JU
 Sample : N1129-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBM05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Title : SVOA CALIBRATION

37	14.234	1905	1912	1920	rBV	3816562	5523756	80.68%	6.268%
38	14.310	1922	1925	1931	rVB6	15029	22675	0.33%	0.026%
39	14.451	1943	1949	1965	rBV	468806	1047942	15.31%	1.189%
40	14.669	1980	1986	1992	rBV6	37982	58240	0.85%	0.066%
41	14.875	2018	2021	2026	rVB2	18277	23073	0.34%	0.026%
42	15.063	2048	2053	2057	rVV4	31794	53824	0.79%	0.061%
43	15.116	2057	2062	2067	rVB4	25987	37320	0.55%	0.042%
44	15.228	2074	2081	2093	rBV	3574568	5183596	75.71%	5.882%
45	15.351	2096	2102	2112	rBV	860779	1267649	18.52%	1.438%
46	15.463	2118	2121	2126	rBV	19692	30735	0.45%	0.035%
47	15.610	2142	2146	2153	rVB8	11264	18541	0.27%	0.021%
48	15.675	2153	2157	2160	rBV4	11780	16797	0.25%	0.019%
49	15.869	2185	2190	2194	rBV7	14355	23597	0.34%	0.027%
50	15.928	2194	2200	2205	rBV9	19663	43000	0.63%	0.049%
51	16.139	2231	2236	2242	rVV8	17650	33075	0.48%	0.038%
52	16.386	2274	2278	2282	rBV5	11893	18359	0.27%	0.021%
53	16.480	2289	2294	2300	rVV10	8866	21145	0.31%	0.024%
54	16.557	2303	2307	2311	rBV6	14759	24745	0.36%	0.028%
55	16.733	2330	2337	2339	rBV7	14621	27862	0.41%	0.032%
56	16.769	2339	2343	2347	rVV2	34396	51686	0.75%	0.059%
57	16.928	2364	2370	2372	rBV4	32659	41695	0.61%	0.047%
58	16.975	2372	2378	2389	rVV	4424617	6444464	94.13%	7.313%
59	17.075	2389	2395	2409	rVV	3958527	5639222	82.37%	6.399%
60	17.186	2409	2414	2420	rVB3	79500	114654	1.67%	0.130%
61	17.286	2427	2431	2433	rBV5	15404	22873	0.33%	0.026%
62	17.675	2493	2497	2502	rVB2	42557	59805	0.87%	0.068%
63	17.792	2512	2517	2520	rBV6	10856	17740	0.26%	0.020%
64	17.898	2531	2535	2541	rVV2	86221	152542	2.23%	0.173%
65	17.957	2543	2545	2552	rVV	29859	47740	0.70%	0.054%
66	18.204	2582	2587	2589	rBV6	12525	19923	0.29%	0.023%
67	18.333	2606	2609	2616	rBV8	23469	44432	0.65%	0.050%
68	18.498	2633	2637	2640	rVB6	18917	27463	0.40%	0.031%
69	18.663	2662	2665	2667	rBV2	27331	30124	0.44%	0.034%
70	18.716	2671	2674	2678	rVV6	14796	22875	0.33%	0.026%
71	18.751	2678	2680	2688	rVB7	20369	30783	0.45%	0.035%
72	18.827	2690	2693	2695	rVV4	13831	15059	0.22%	0.017%
73	18.857	2695	2698	2701	rVB5	17184	21403	0.31%	0.024%
74	18.939	2708	2712	2716	rVB2	57779	79040	1.15%	0.090%
75	19.010	2716	2724	2728	rBV	54808	109669	1.60%	0.124%
76	19.063	2730	2733	2737	rVV6	15126	24087	0.35%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011922\
 Data File : BN018421.D
 Acq On : 19 Jan 2022 17:27
 Operator : CG/JU
 Sample : N1129-12
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBM05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Title : SVOA CALIBRATION

77	19.192	2751	2755	2763	rBV7	39824	84313	1.23%	0.096%
78	19.304	2770	2774	2777	rVB	52563	61991	0.91%	0.070%
79	19.374	2780	2786	2798	rVV	5042997	6730342	98.31%	7.637%
80	19.457	2798	2800	2805	rVV5	23353	30867	0.45%	0.035%
81	19.516	2807	2810	2816	rVB2	31194	36457	0.53%	0.041%
82	19.957	2882	2885	2888	rBV3	24986	23659	0.35%	0.027%
83	20.257	2933	2936	2938	rBV4	12608	19138	0.28%	0.022%
84	20.327	2940	2948	2954	rVV4	49634	112299	1.64%	0.127%
85	20.451	2966	2969	2973	rVB2	43884	43584	0.64%	0.049%
86	20.533	2980	2983	2986	rBV3	19802	22548	0.33%	0.026%
87	20.910	3043	3047	3055	rBV2	187759	361983	5.29%	0.411%
88	21.110	3078	3081	3086	rBV	65422	67919	0.99%	0.077%
89	21.174	3086	3092	3101	rBV2	4913816	6846265	100.00%	7.769%
90	21.351	3119	3122	3130	rVB	105773	133224	1.95%	0.151%
91	21.780	3192	3195	3199	rBV2	150683	178919	2.61%	0.203%
92	22.239	3270	3273	3279	rVB	202703	289134	4.22%	0.328%
93	22.751	3355	3360	3365	rBV	340789	497239	7.26%	0.564%
94	23.251	3437	3445	3452	rBV2	3262194	6230535	91.01%	7.070%
95	23.315	3452	3456	3462	rVV	369160	692728	10.12%	0.786%
96	23.392	3462	3469	3480	rVB2	3274816	6564973	95.89%	7.449%
97	23.968	3561	3567	3574	rVB	312785	614181	8.97%	0.697%
98	24.721	3690	3695	3707	rVB4	257622	577225	8.43%	0.655%
99	25.609	3838	3846	3862	rVB4	183527	554053	8.09%	0.629%
100	26.645	4016	4022	4032	rVB5	116112	338031	4.94%	0.384%




Sum of corrected areas: 88127471

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011922\
Data File : BN018421.D
Acq On : 19 Jan 2022 17:27
Operator : CG/JU
Sample : N1129-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBM05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

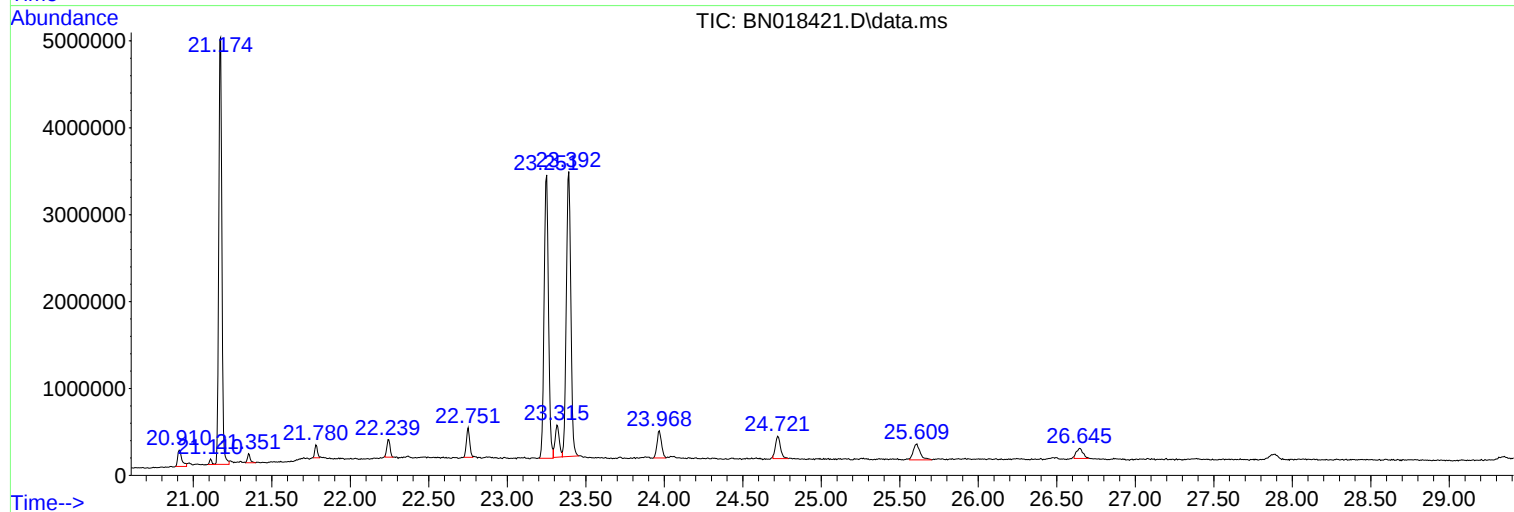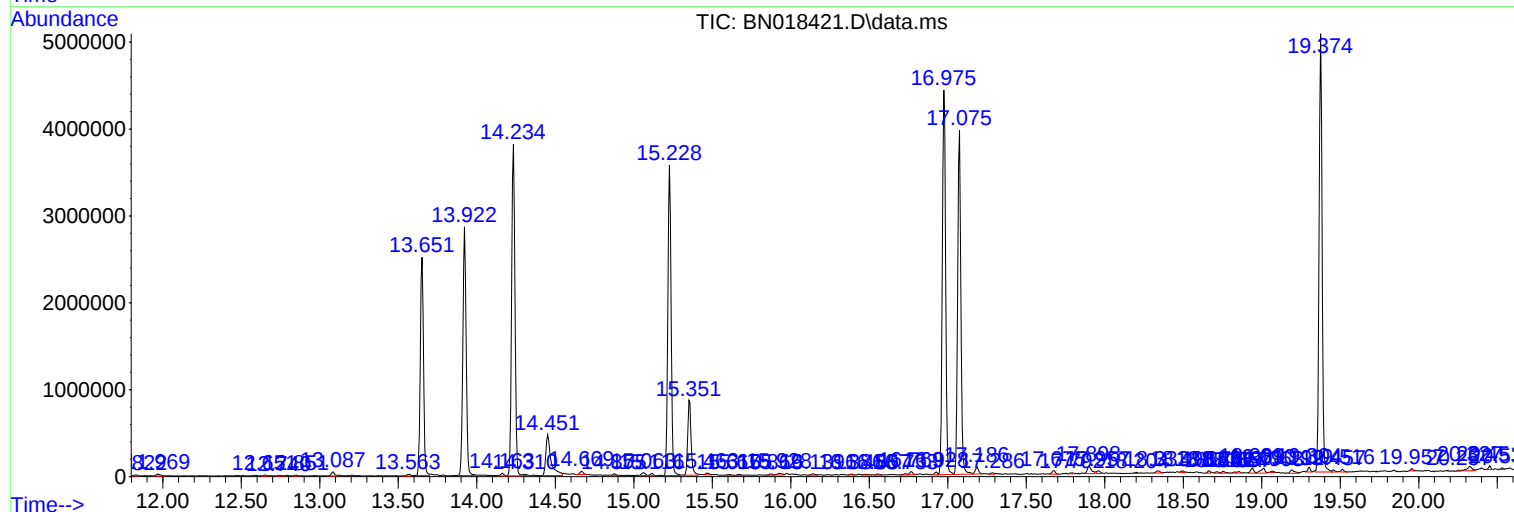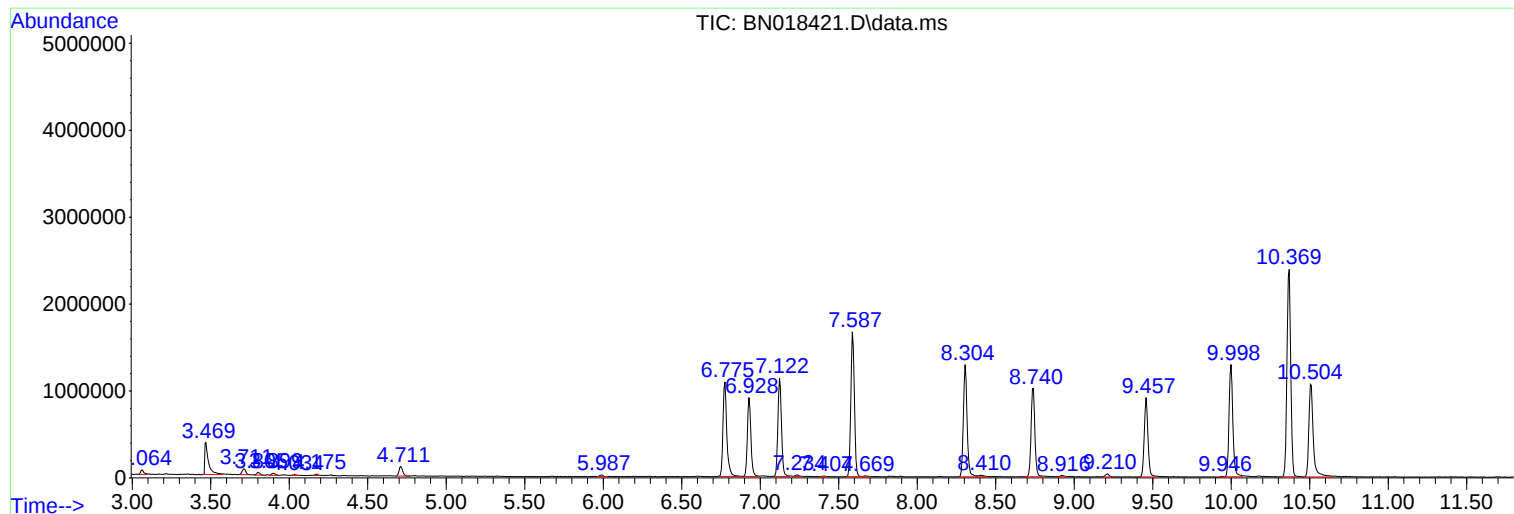

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011922\
Data File : BN018421.D
Acq On : 19 Jan 2022 17:27
Operator : CG/JU
Sample : N1129-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBM05










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
23.315	2.11 ng/ul	692728	Perylene-d12	23.386

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Tetracosane	338	C24H50	000646-31-1	94
2		Heptadecane, 9-octyl-	352	C25H52	007225-64-1	91
3		Tetracosane	338	C24H50	000646-31-1	91
4		Hexacosane	366	C26H54	000630-01-3	90
5		Docosane, 11-butyl-	366	C26H54	013475-76-8	90

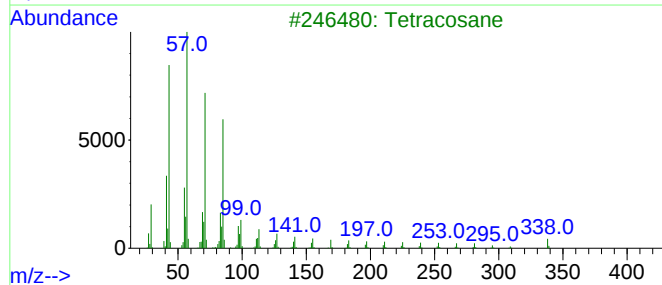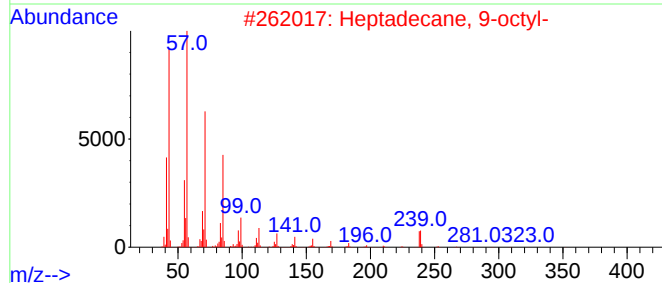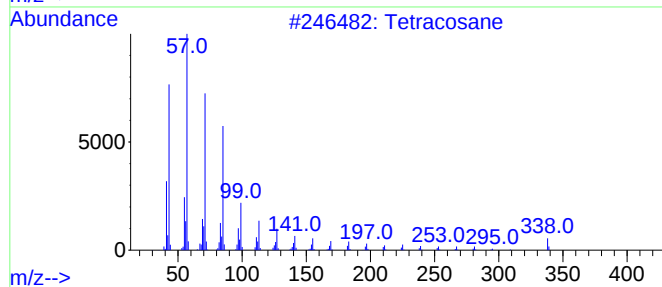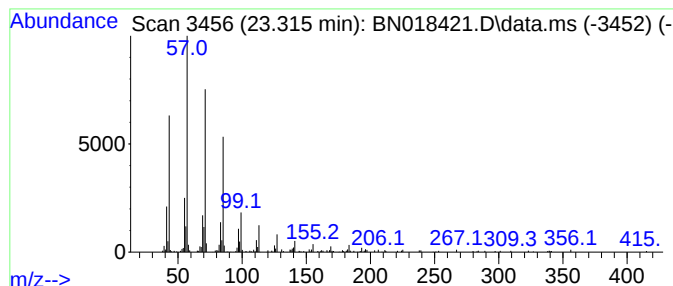

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011922\
Data File : BN018421.D
Acq On : 19 Jan 2022 17:27
Operator : CG/JU
Sample : N1129-12
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBM05

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	23.315	2.1	ng/u1	692728	6	23.386	6564970	20.0