
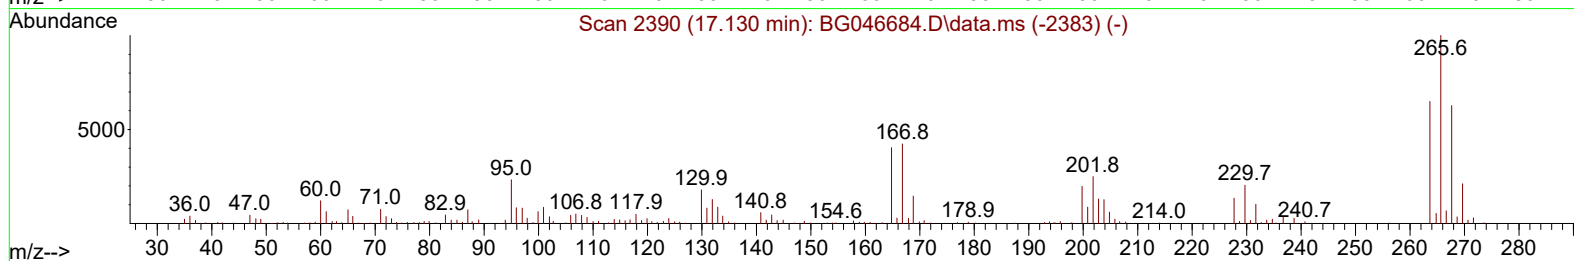
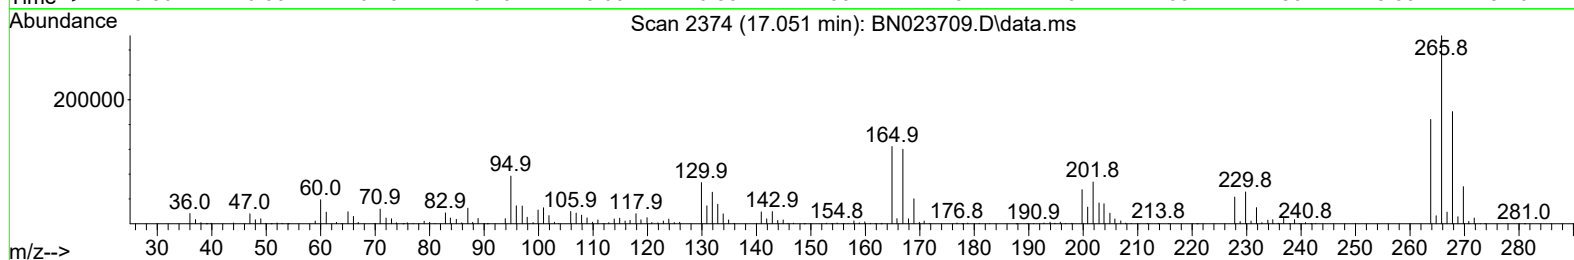


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011923\
 Data File : BN023709.D
 Acq On : 19 Jan 2023 08:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 20 05:01:38 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 20 05:01:34 2023
 Response via : Initial Calibration

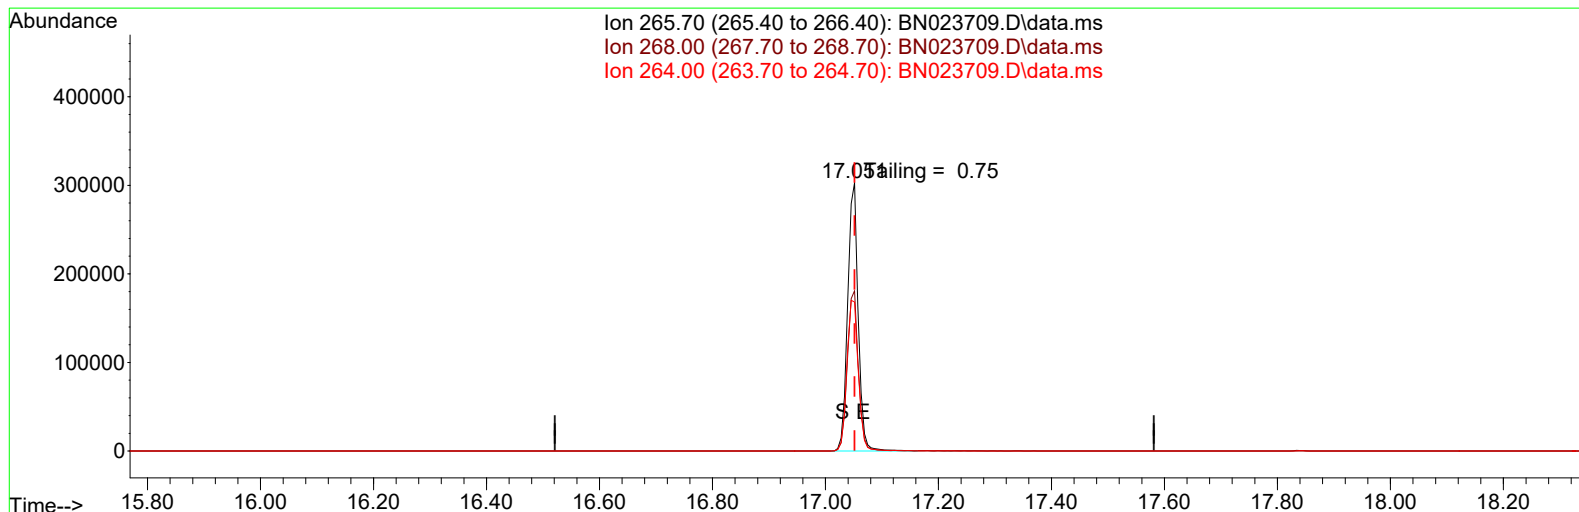

TIC: BN023709.D\data.ms

(70) Pentachlorophenol (C)




17.051min (0.000) 21872.19 ng

response 392901

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.73
264.00	61.60	55.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011923\
Data File : BN023709.D
Acq On : 19 Jan 2023 08:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 20 05:01:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 20 05:01:34 2023
Response via : Initial Calibration

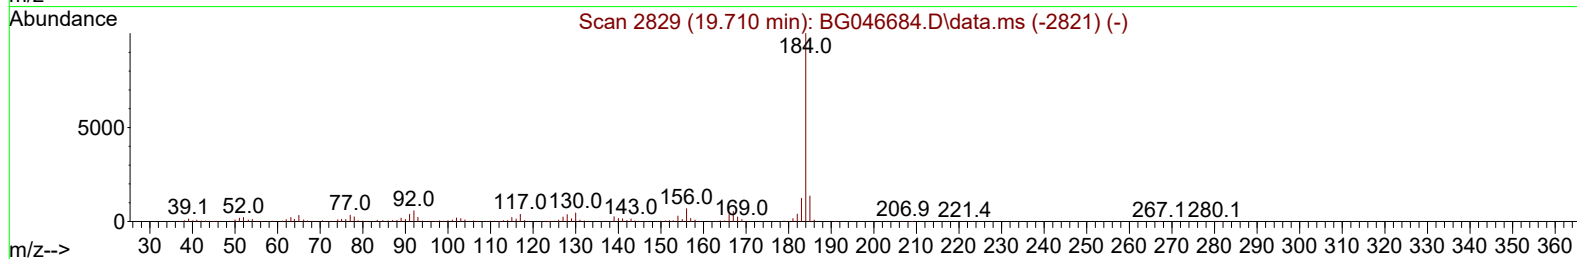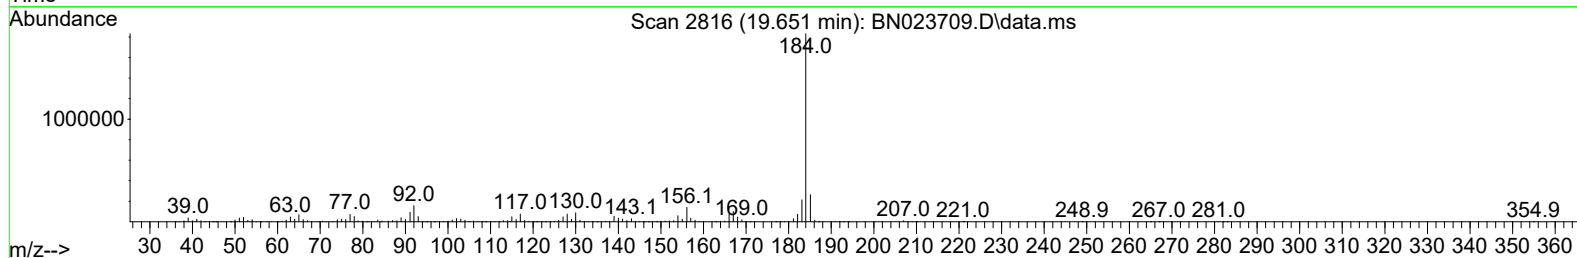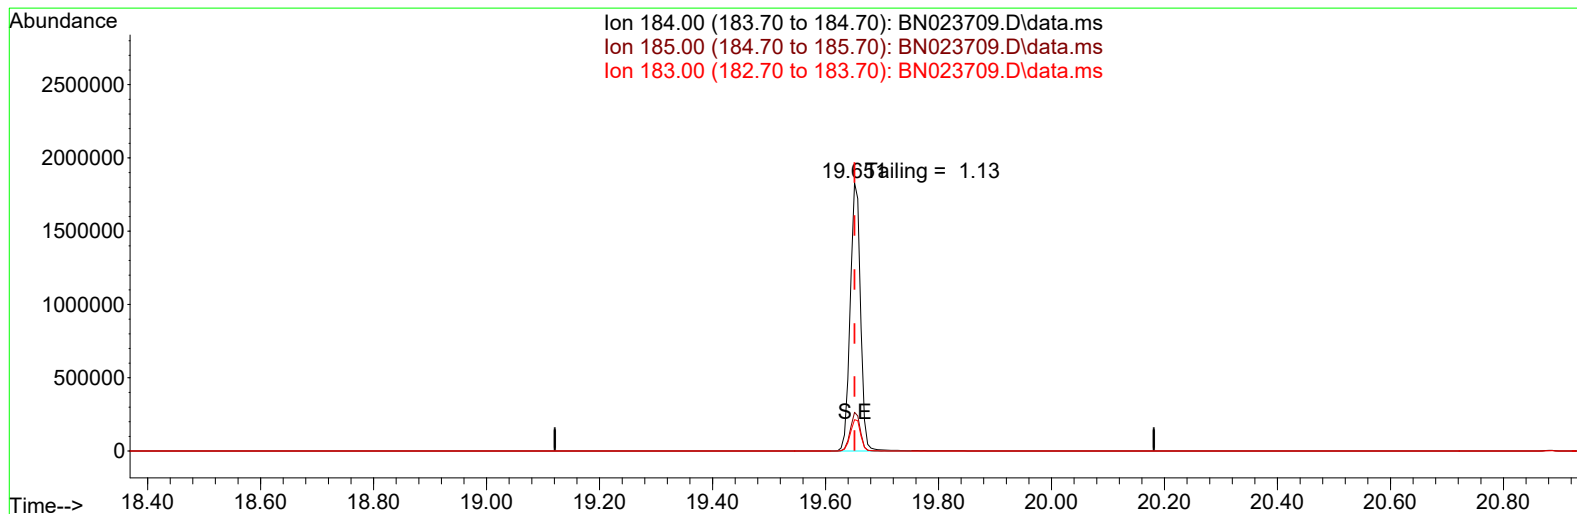

TIC: BN023709.D\data.ms

(77) Benzidine**19.651min (0.000) 332115.94 ng****response 2313697**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.43
183.00	13.20	11.71
0.00	0.00	0.00