
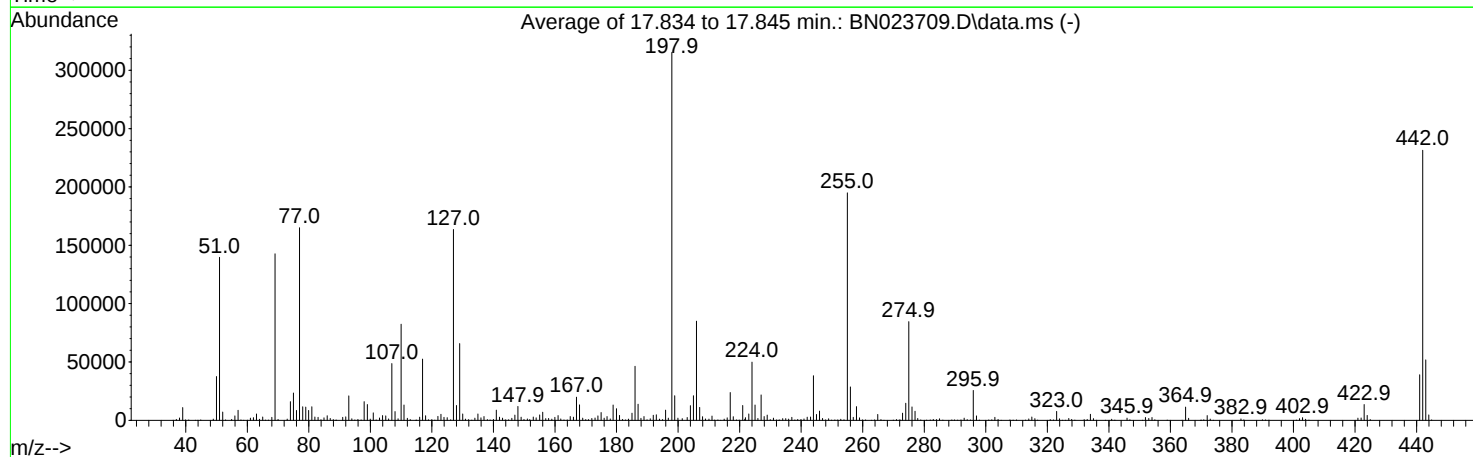


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011923\
 Data File : BN023709.D
 Acq On : 19 Jan 2023 08:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN011823.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 20 04:29:10 2023

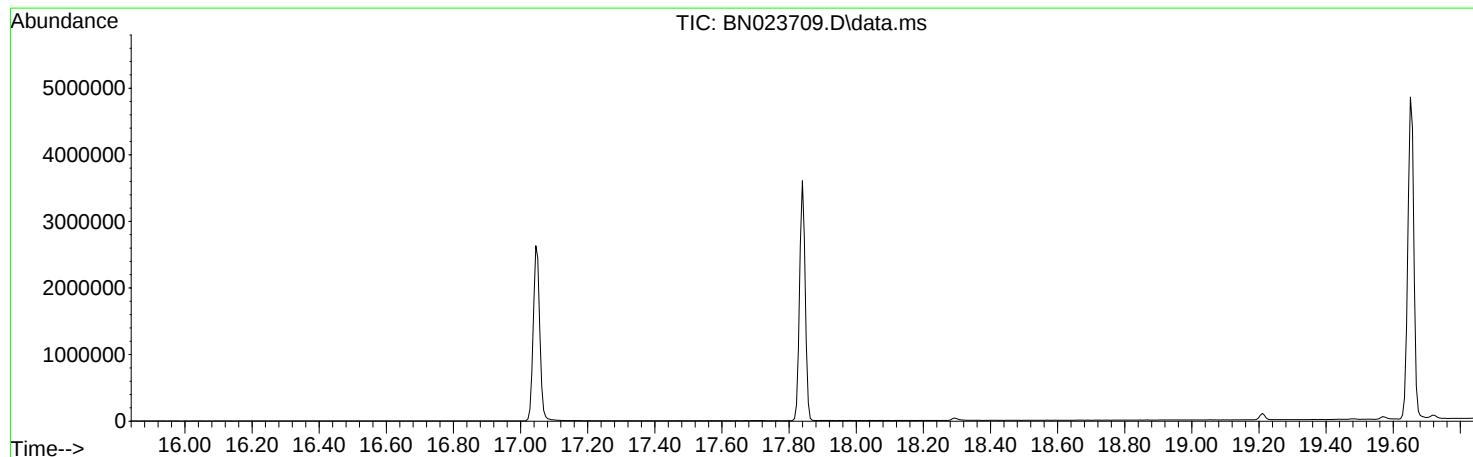




AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	139648	PASS
68	69	0.00	2	1.8	2510	PASS
69	198	0.00	100	45.3	142781	PASS
70	69	0.00	2	0.5	766	PASS
127	198	10	80	51.9	163627	PASS
197	198	0.00	2	0.6	1817	PASS
198	198	100	100	100.0	315307	PASS
199	198	5	9	6.7	21107	PASS
275	198	10	60	26.8	84557	PASS
365	198	1	100	3.6	11360	PASS
441	198	0.01	100	12.4	39075	PASS
442	442	50	100	100.0	231445	PASS
443	442	15	24	22.4	51795	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011923\
 Data File : BN023709.D
 Acq On : 19 Jan 2023 08:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jan 20 05:01:38 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 20 05:01:34 2023
 Response via : Initial Calibration

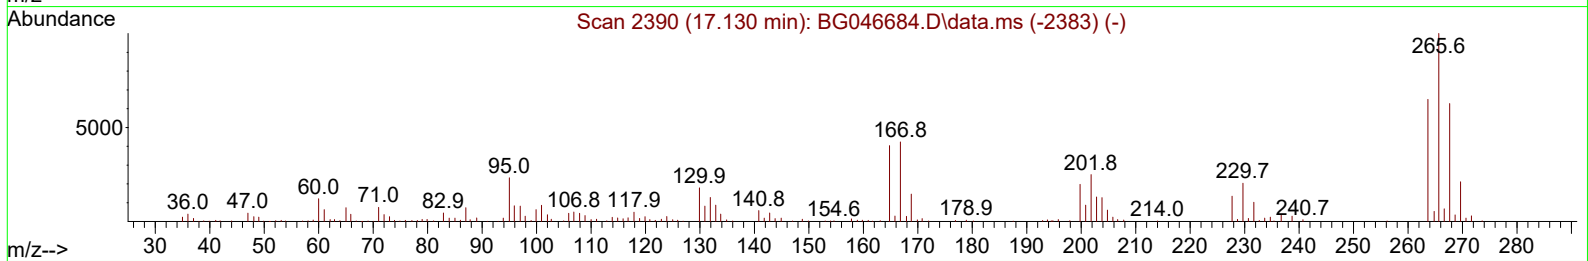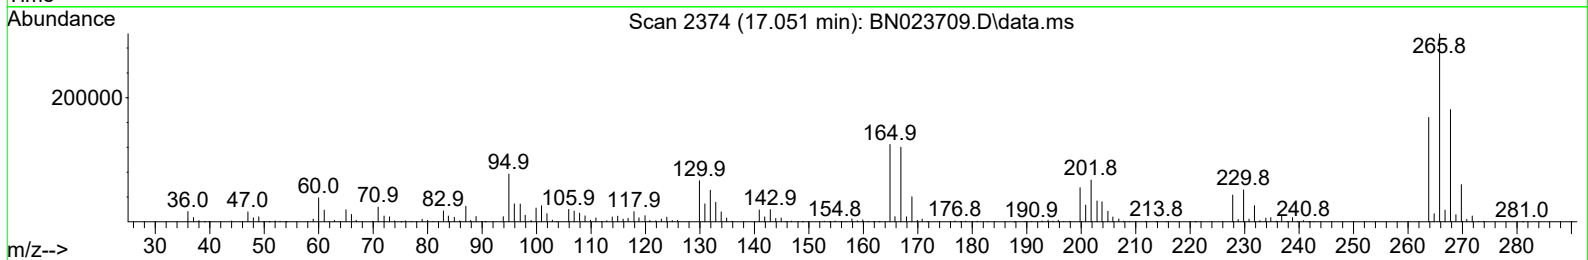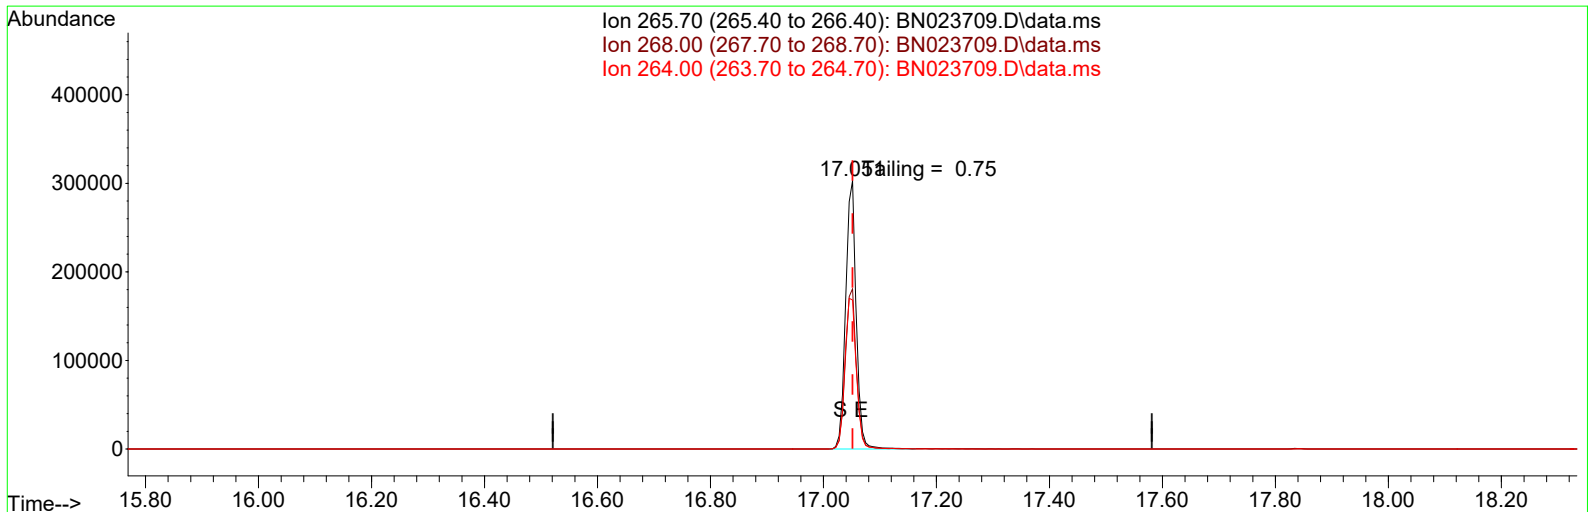

TIC: BN023709.D\data.ms

(70) Pentachlorophenol (C)

17.051min (0.000) 21872.19 ng




response 392901

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.73
264.00	61.60	55.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011923\
Data File : BN023709.D
Acq On : 19 Jan 2023 08:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 20 05:01:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 20 05:01:34 2023
Response via : Initial Calibration

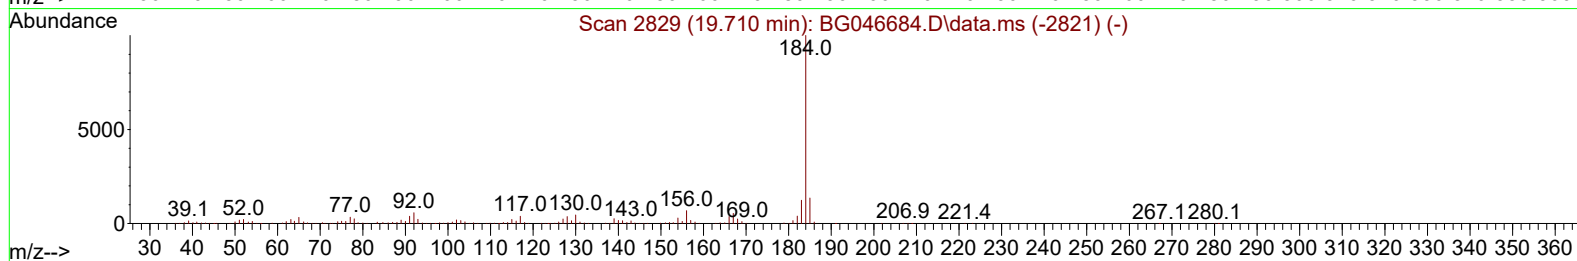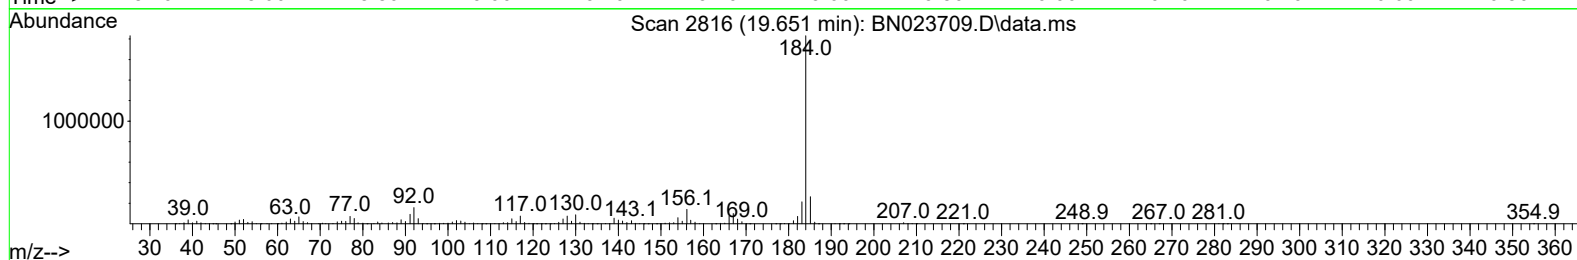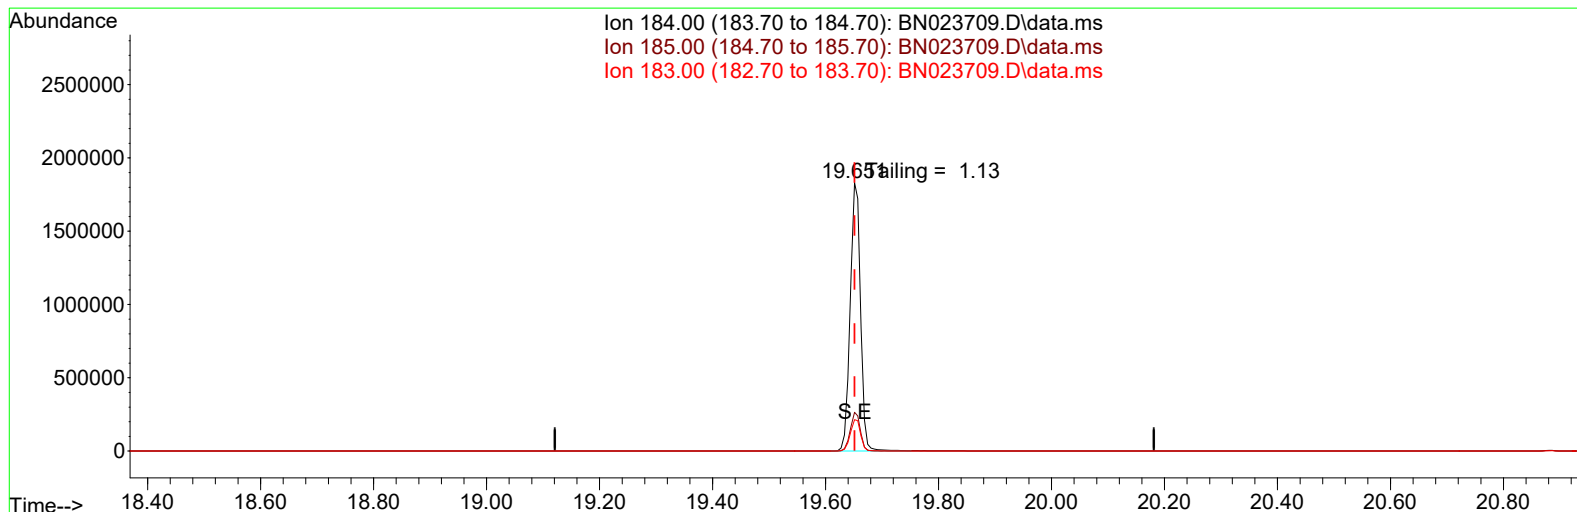

TIC: BN023709.D\data.ms

(77) Benzidine

19.651min (0.000) 332115.94 ng

response 2313697

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.43
183.00	13.20	11.71
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/19/2023	BNA_N	<u>BN023709.D</u>
Compound Name	Response	Retention Time
DDT	1102275	20.88
DDD	9110	20.492
DDE	63	19.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9173	1111448	0.83

Instrument :
BNA_N
ClientSampleId :
DFTPP