

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023728.D
 Acq On : 20 Jan 2023 15:39
 Operator : CG/JU
 Sample : O1145-11ME
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A43X9ME

Quant Time: Jan 20 21:57:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 05 03:34:47 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	213903	20.000	ng/ul	0.00
20) Naphthalene-d8	10.704	136	875431	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.540	164	539984	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.286	188	1153459	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	1124375	20.000	ng/ul	0.00
88) Perylene-d12	23.904	264	1216412	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	29838	6.003	ng/uL	0.04
4) Pyridine-d5	3.699	84	404734	27.138	ng/ul	0.03
7) Phenol-d5	7.058	99	576622	30.416	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	367349	31.586	ng/ul	0.00
11) 2-Chlorophenol-d4	7.422	132	465136	32.036	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	457177	30.214	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	225347	34.136	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	243041	34.779	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	429706	32.238	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	645130	30.770	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	1302986	32.438	ng/ul	0.00
49) Acenaphthylene-d8	14.234	160	1530519	34.388	ng/ul	0.00
54) 4-Nitrophenol-d4	14.740	143	231434	28.301	ng/ul	0.00
60) Fluorene-d10	15.534	176	1150288	33.513	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	133141	19.134	ng/ul	0.00
73) Anthracene-d10	17.386	188	1776218	34.412	ng/ul	0.00
81) Pyrene-d10	19.680	212	2133194	33.173	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.757	264	2046163	34.015	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.404	149	8591138	188.133	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023728.D
 Acq On : 20 Jan 2023 15:39
 Operator : CG/JU
 Sample : 01145-11ME
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A43X9ME

Quant Time: Jan 20 21:57:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 05 03:34:47 2023
 Response via : Initial Calibration

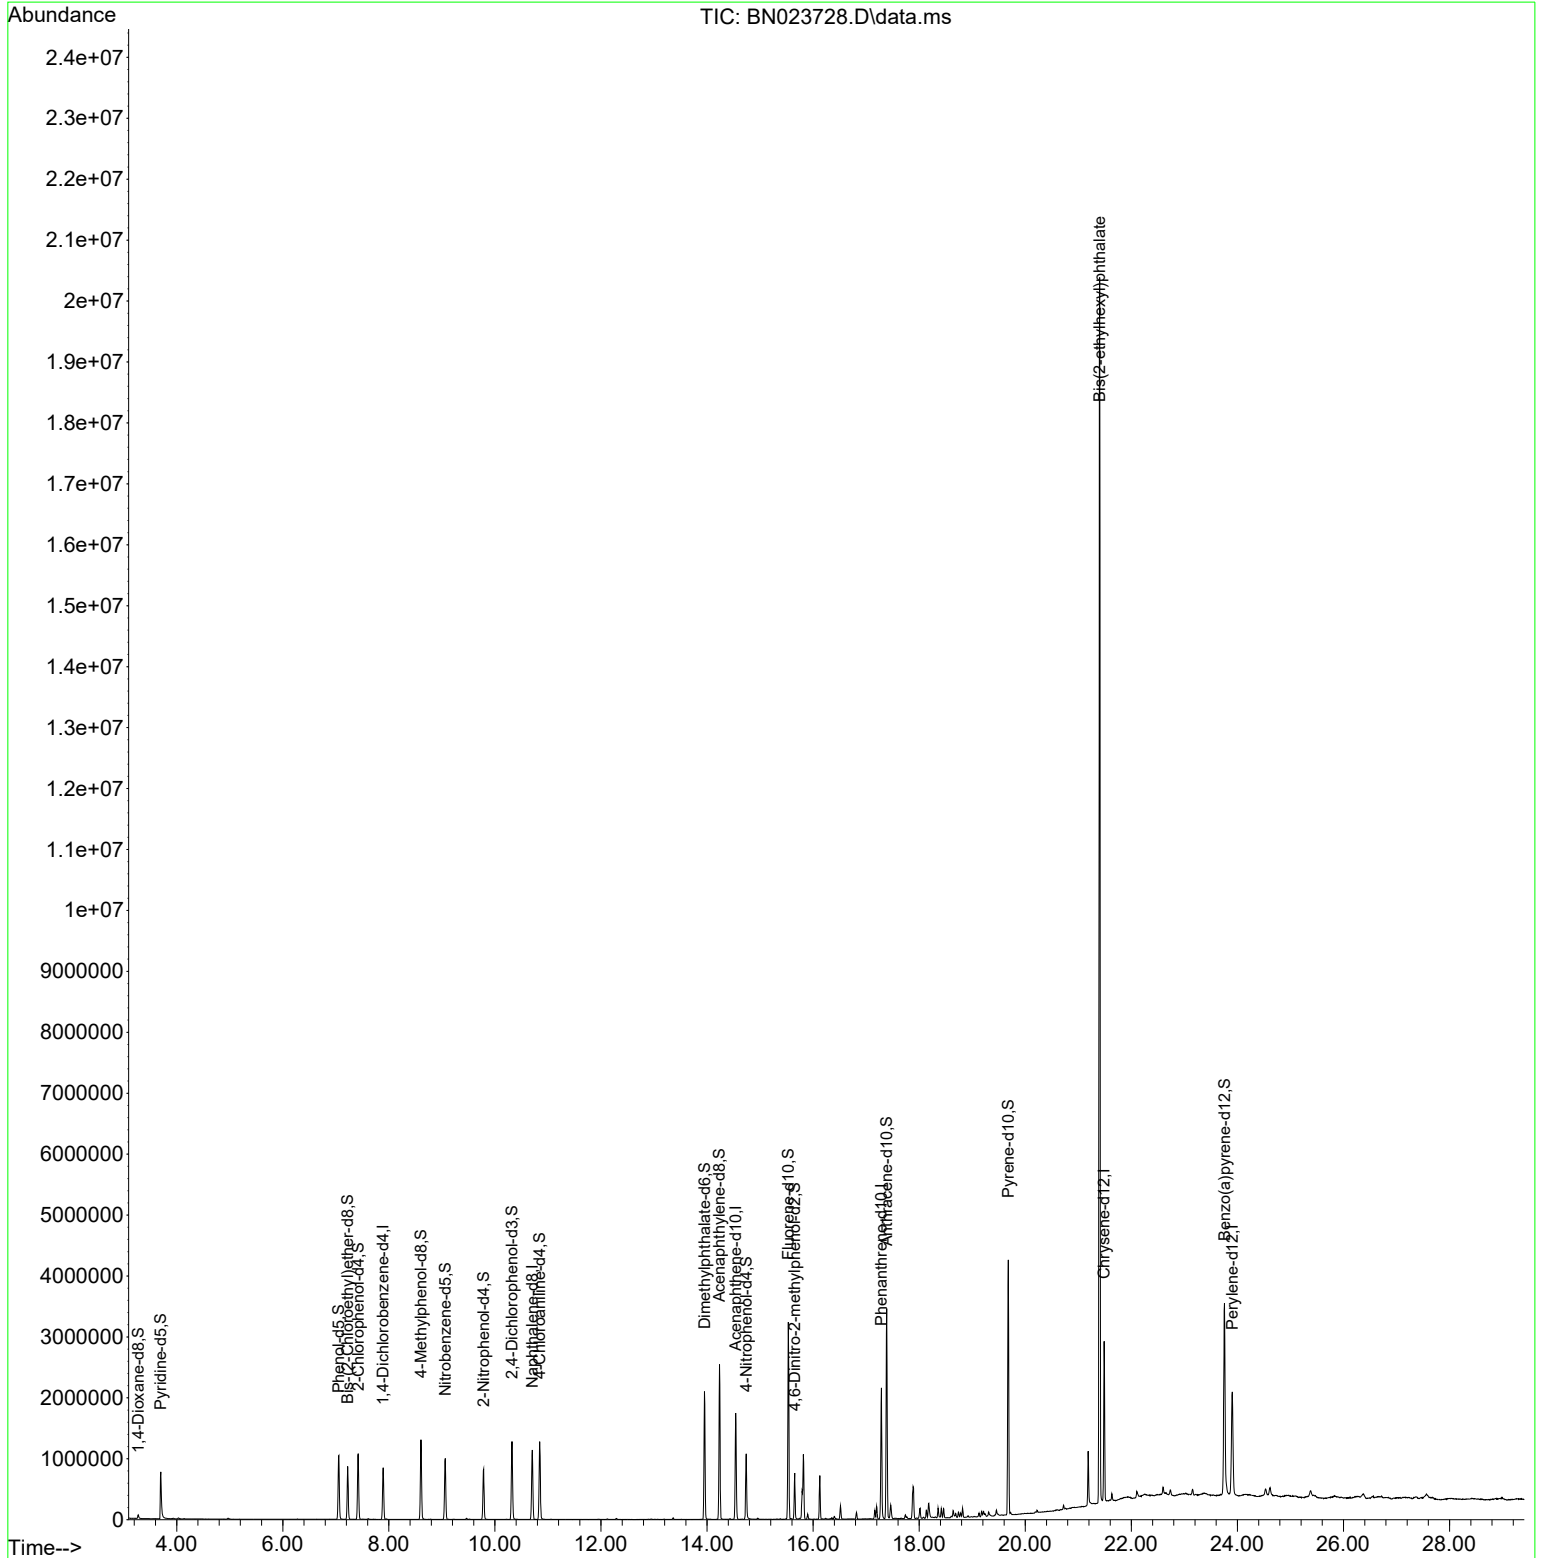

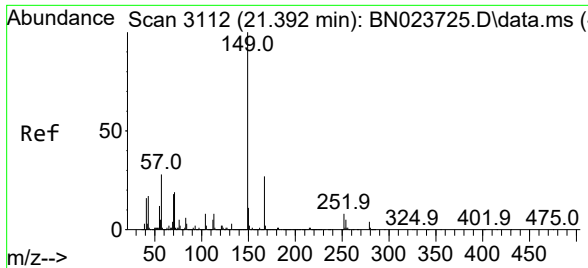

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 188.133 ng/ul
 RT: 21.404 min Scan# 3114
 Delta R.T. 0.013 min
 Lab File: BN023728.D
 Acq: 20 Jan 2023 15:39

Instrument :
 BNA_N
 ClientSampleId :
 A43X9ME

Tgt Ion:149 Resp: 8591138

Ion	Ratio	Lower	Upper
149	100		
167	28.6	22.0	33.0
279	5.8	3.4	5.2#

