

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023734.D
 Acq On : 20 Jan 2023 19:21
 Operator : CG/JU
 Sample : 01146-14ME
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4462ME

Quant Time: Jan 20 21:58:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 05 03:34:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	187767	20.000	ng/ul	0.00
20) Naphthalene-d8	10.705	136	805493	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.540	164	495033	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.287	188	1126948	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	930962	20.000	ng/ul	0.00
88) Perylene-d12	23.910	264	1127823	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.276	96	15345	3.517	ng/uL	0.04
4) Pyridine-d5	3.699	84	189298	14.459	ng/ul	0.03
7) Phenol-d5	7.052	99	294117	17.674	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	189232	18.536	ng/ul	0.00
11) 2-Chlorophenol-d4	7.422	132	236346	18.544	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	236564	17.810	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	114026	18.773	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	120791	18.786	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	218713	17.833	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	340607	17.656	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	723288	19.641	ng/ul	0.00
49) Acenaphthylene-d8	14.234	160	810178	19.856	ng/ul	0.00
54) 4-Nitrophenol-d4	14.740	143	110313	14.715	ng/ul	0.00
60) Fluorene-d10	15.534	176	628623	19.978	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	60026	8.830	ng/ul	0.00
73) Anthracene-d10	17.387	188	975881	19.351	ng/ul	0.00
81) Pyrene-d10	19.681	212	1095869	20.583	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.751	264	1099547	19.714	ng/ul	0.00


Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.416	149	17157148	453.773	ng/ul# 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023734.D
Acq On : 20 Jan 2023 19:21
Operator : CG/JU
Sample : 01146-14ME
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4462ME


Quant Time: Jan 20 21:58:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 05 03:34:47 2023
Response via : Initial Calibration

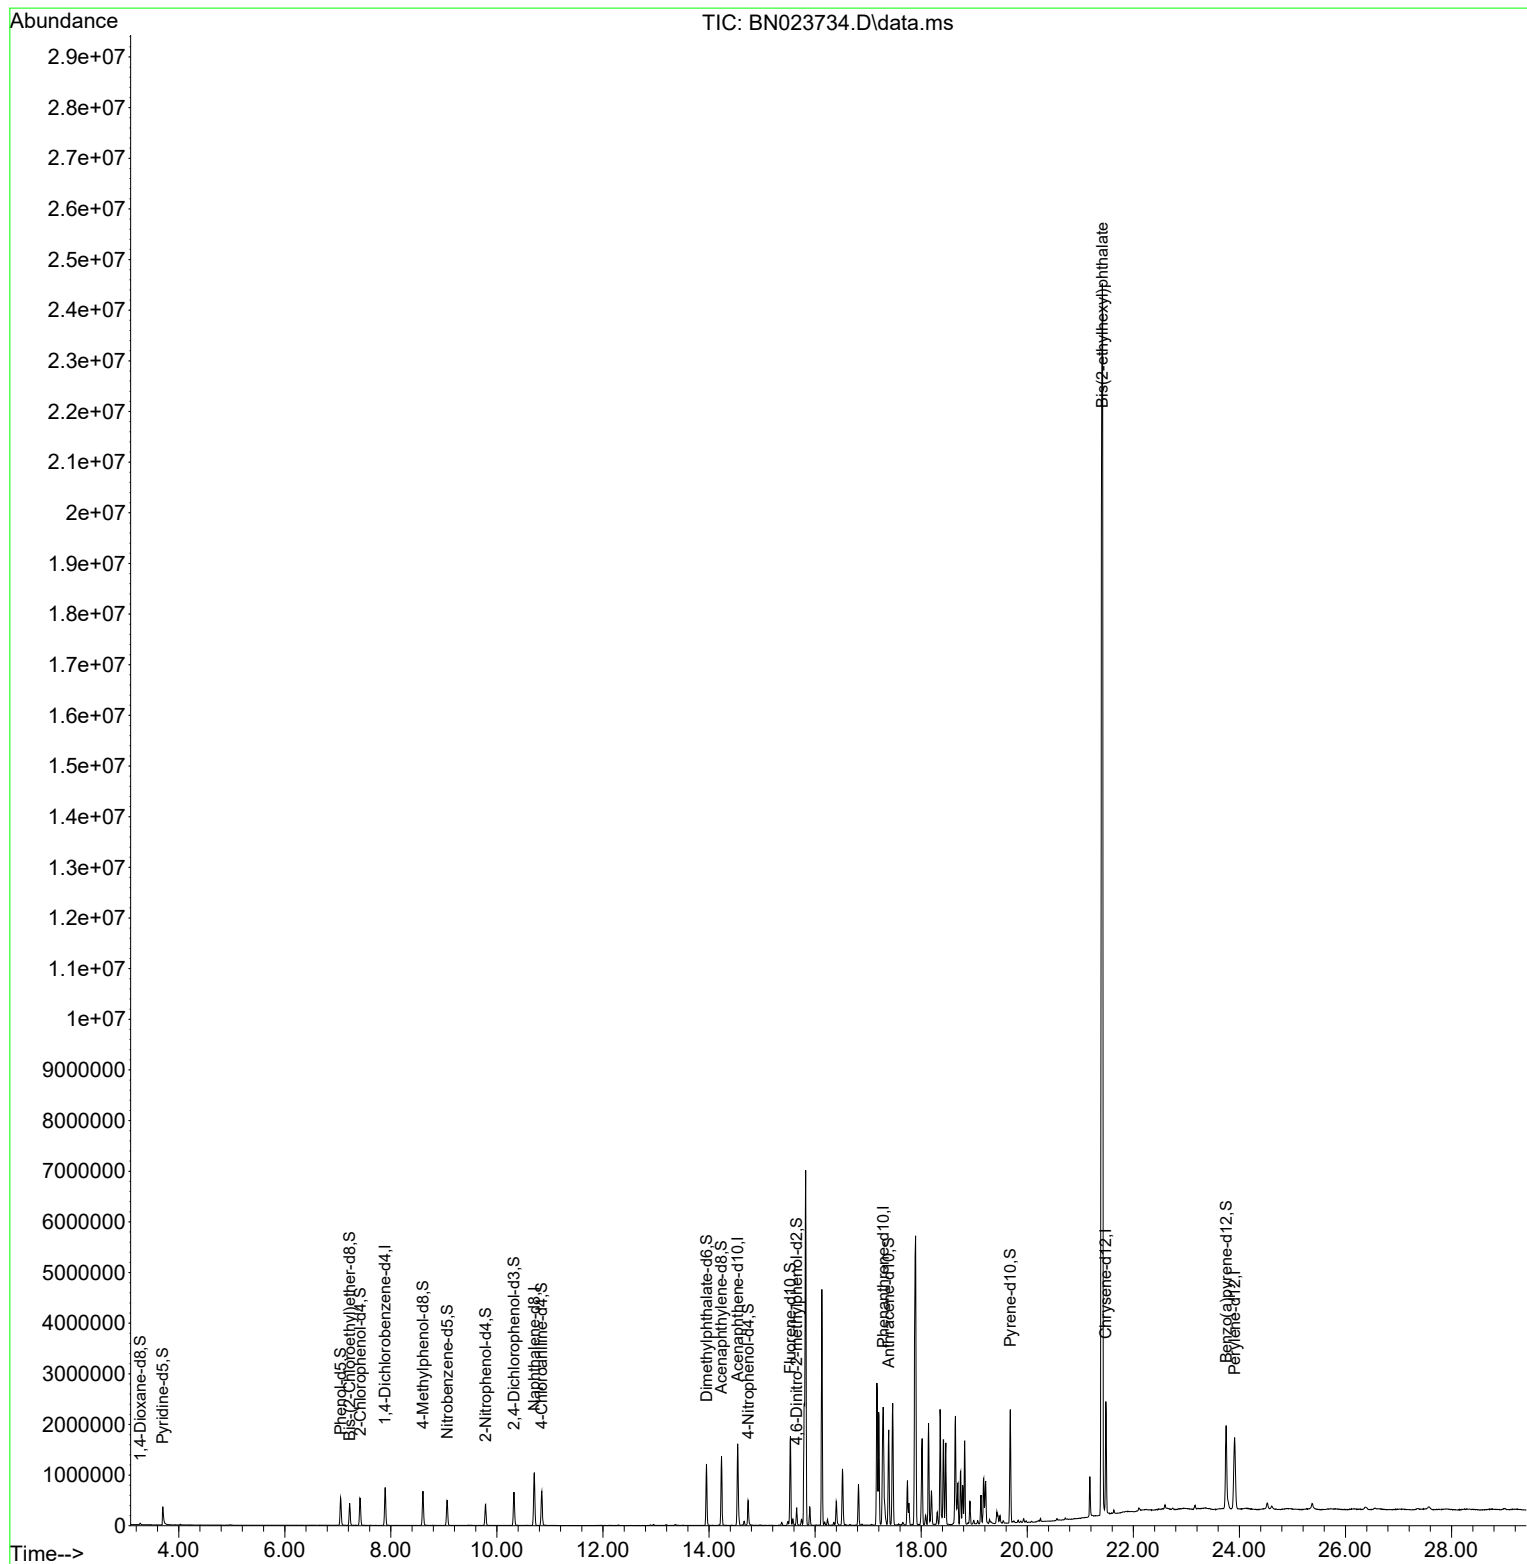

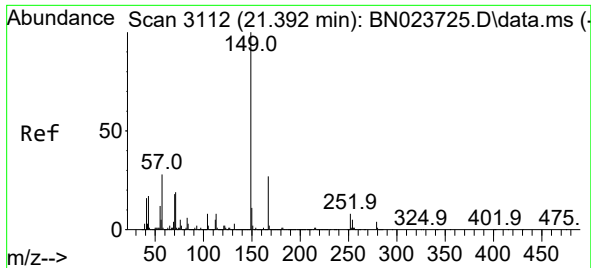

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 453.773 ng/ul
 RT: 21.416 min Scan# 3116
 Delta R.T. 0.025 min
 Lab File: BN023734.D
 Acq: 20 Jan 2023 19:21

Instrument :
 BNA_N
 ClientSampleId :
 A4462ME

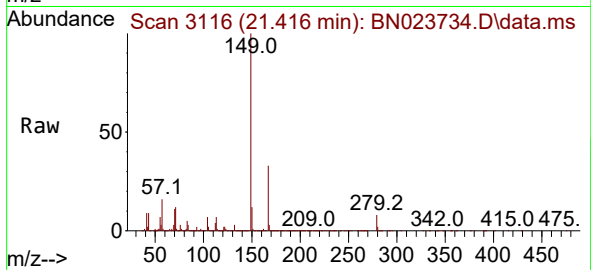

Tgt Ion:149 Resp:17157148
 Ion Ratio Lower Upper
 149 100
 167 32.6 22.0 33.0
 279 7.8 3.4 5.2#

