




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023729.D
 Acq On : 20 Jan 2023 16:16
 Operator : CG/JU
 Sample : 01146-02ME
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A43Y5ME

Manual IntegrationsAPPROVED

Quant Time: Jan 20 21:57:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 05 03:34:47 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/23/2023
 Supervised By :Yogesh Patel 01/24/2023

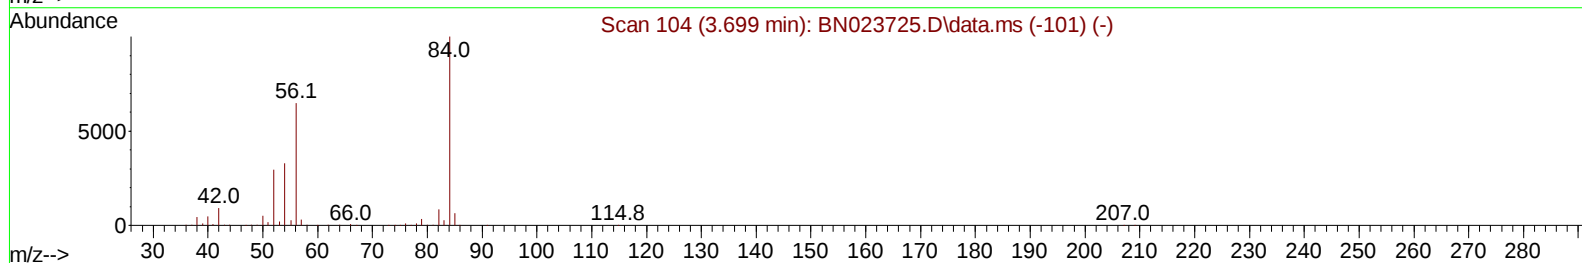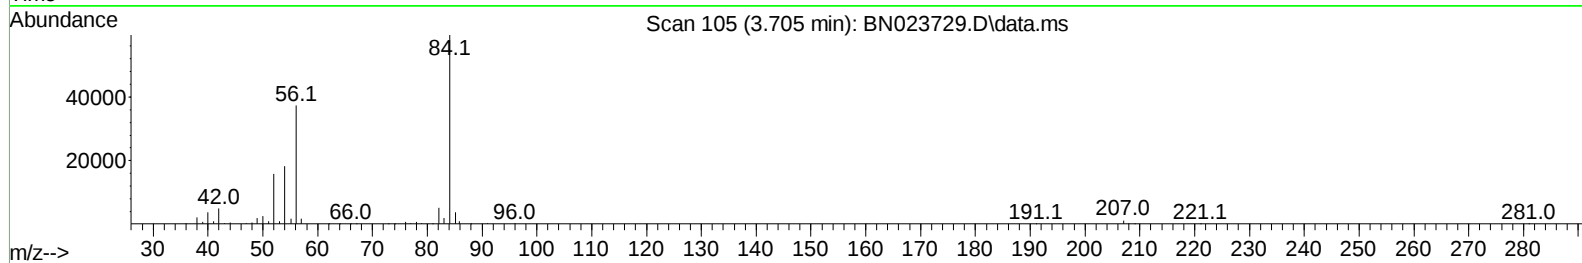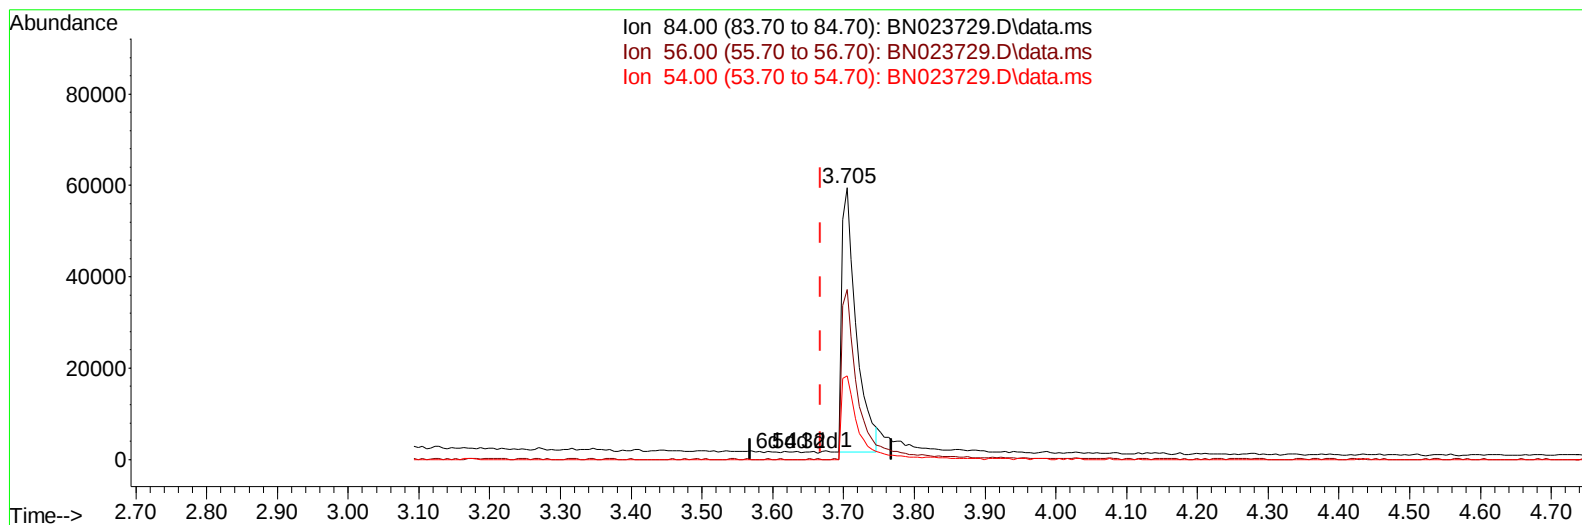

TIC: BN023729.D\data.ms

(4) Pyridine-d5 (S)

3.705min (+ 0.037) 6.08 ng/u1

response 81441

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	64.00	62.70
54.00	32.20	30.79
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023729.D
 Acq On : 20 Jan 2023 16:16
 Operator : CG/JU
 Sample : 01146-02ME
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A43Y5ME

Manual IntegrationsAPPROVED

Quant Time: Jan 20 21:57:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 05 03:34:47 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/23/2023
 Supervised By :Yogesh Patel 01/24/2023

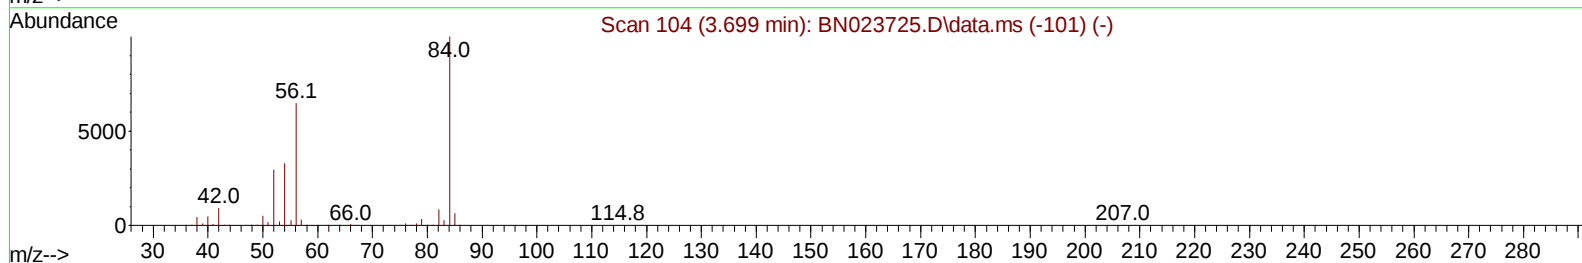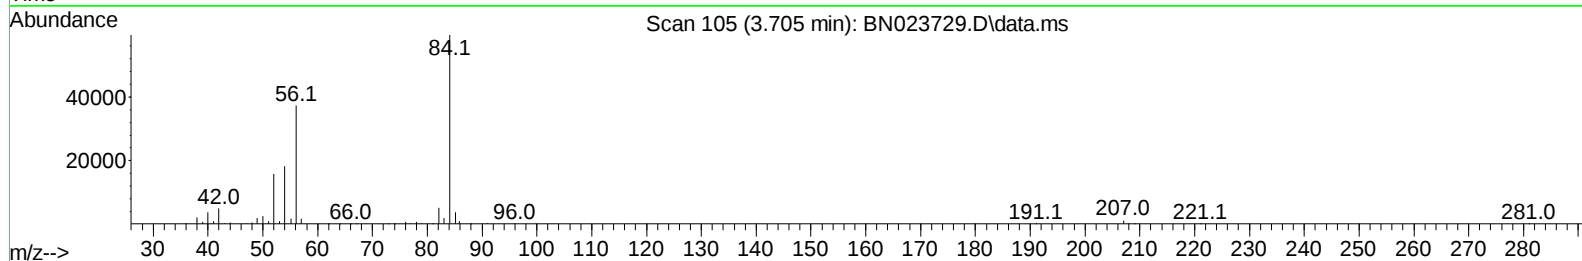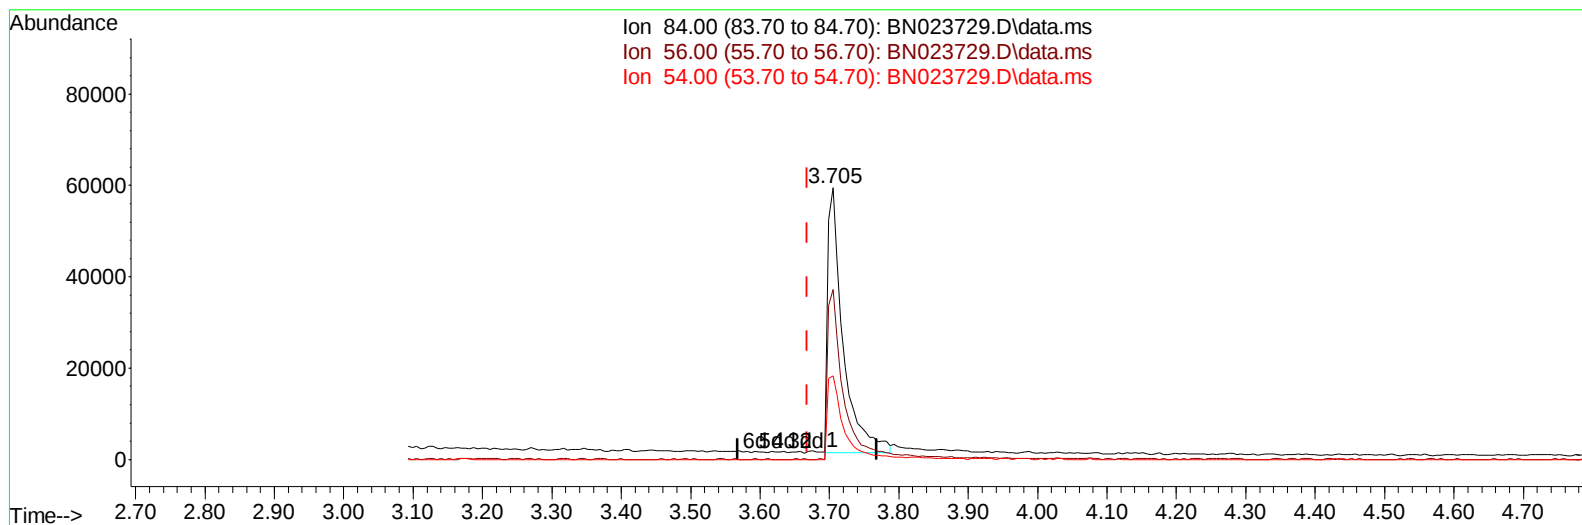

TIC: BN023729.D\data.ms

(4) Pyridine-d5 (S)

3.705min (+ 0.037) 6.62 ng/u1 m

response 88626

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	64.00	62.70
54.00	32.20	30.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023729.D
 Acq On : 20 Jan 2023 16:16
 Operator : CG/JU
 Sample : 01146-02ME
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A43Y5ME

Manual IntegrationsAPPROVED

Quant Time: Jan 20 21:57:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 05 03:34:47 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/23/2023
 Supervised By :Yogesh Patel 01/24/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	192051	20.000	ng/ul	0.00
20) Naphthalene-d8	10.705	136	804867	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.540	164	506026	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.287	188	1087813	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	957361	20.000	ng/ul	0.00
88) Perylene-d12	23.910	264	963624	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.276	96	21074	4.722	ng/uL	0.04
4) Pyridine-d5	3.705	84	88626m	6.619	ng/ul	0.04
7) Phenol-d5	7.052	99	393662	23.128	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	256149	24.531	ng/ul	0.00
11) 2-Chlorophenol-d4	7.422	132	328807	25.223	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	319456	23.514	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	158999	26.197	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	171707	26.725	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	306238	24.989	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	331189	17.181	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	971951	25.821	ng/ul	0.00
49) Acenaphthylene-d8	14.234	160	1083470	25.978	ng/ul	0.00
54) 4-Nitrophenol-d4	14.740	143	146080	19.062	ng/ul	0.00
60) Fluorene-d10	15.534	176	831574	25.853	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	87951	13.403	ng/ul	0.00
73) Anthracene-d10	17.387	188	1297467	26.654	ng/ul	0.00
81) Pyrene-d10	19.681	212	1512289	27.620	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.763	264	1219366	25.588	ng/ul	0.01
Target Compounds						
					Qvalue	
86) Bis(2-ethylhexyl)phtha...	21.416	149	16553864	425.745	ng/ul#	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023729.D
 Acq On : 20 Jan 2023 16:16
 Operator : CG/JU
 Sample : 01146-02ME
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A43Y5ME

Manual IntegrationsAPPROVED

Quant Time: Jan 20 21:57:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 05 03:34:47 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/23/2023
 Supervised By :Yogesh Patel 01/24/2023

