




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023741.D
 Acq On : 21 Jan 2023 00:18
 Operator : CG/JU
 Sample : 01146-02MEDL 30X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A43Y5MEDL

Manual IntegrationsAPPROVED

Quant Time: Jan 21 01:38:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 20 23:02:18 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/23/2023
 Supervised By :Yogesh Patel 01/24/2023

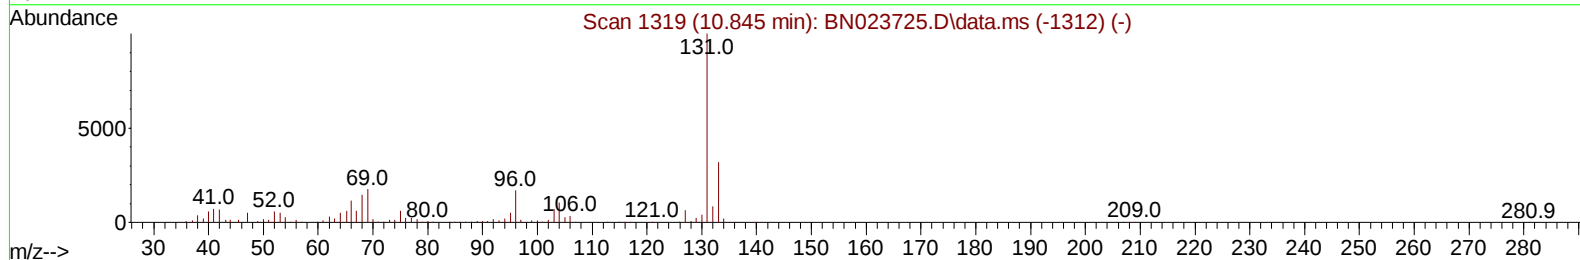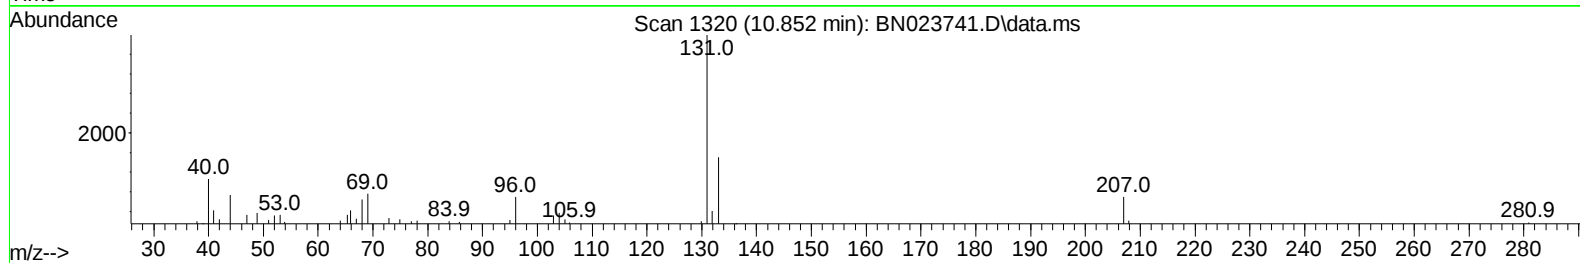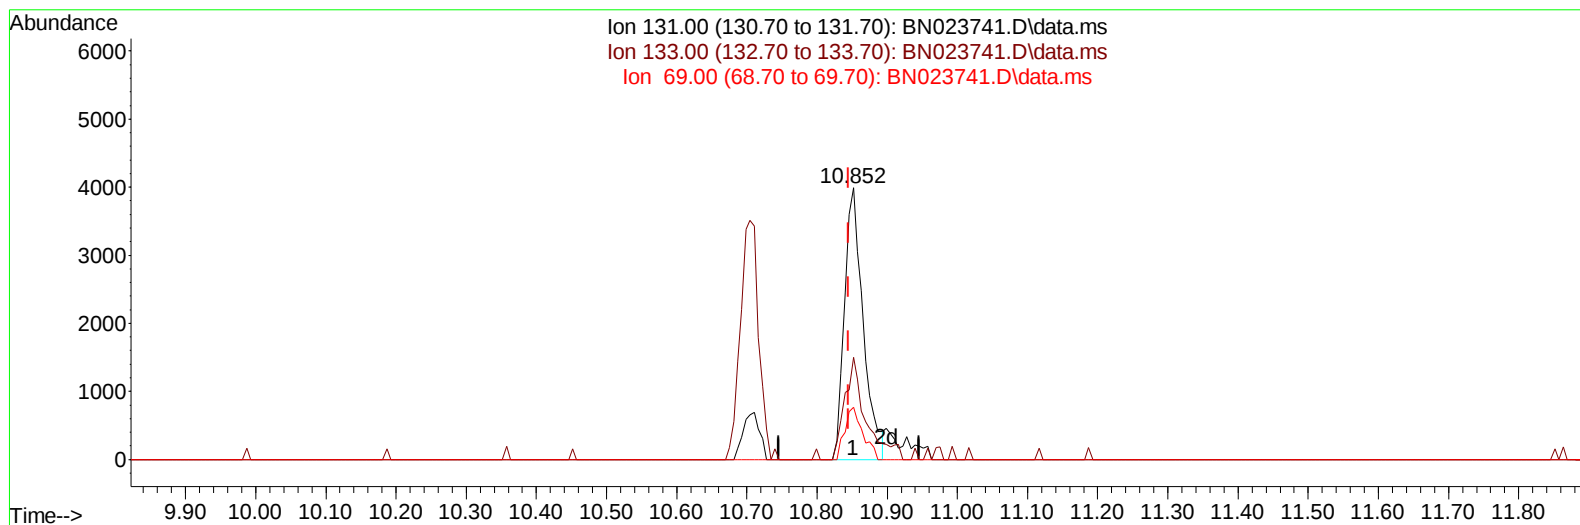

TIC: BN023741.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.852min (+ 0.006) 0.38 ng/ul

response 7398

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.40	37.65
69.00	17.20	19.30
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023741.D
Acq On : 21 Jan 2023 00:18
Operator : CG/JU
Sample : 01146-02MEDL 30X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A43Y5MEDL

Manual IntegrationsAPPROVED

Quant Time: Jan 21 01:38:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 20 23:02:18 2023
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/23/2023
Supervised By :Yogesh Patel 01/24/2023

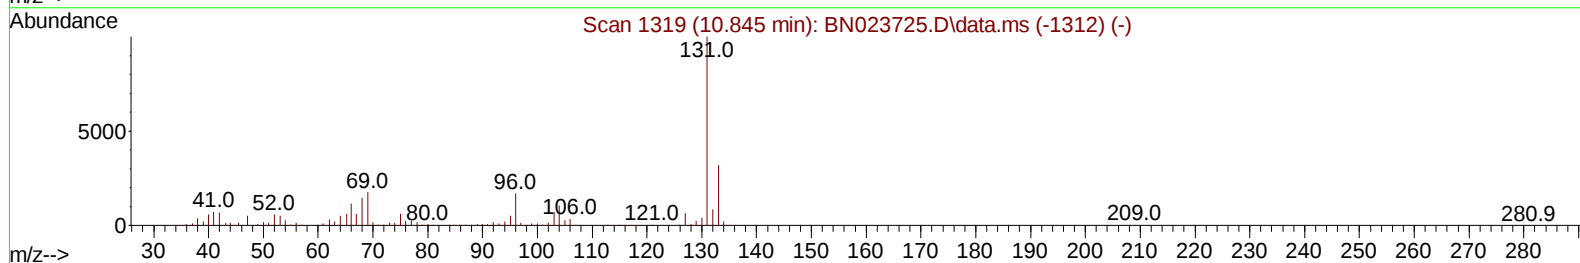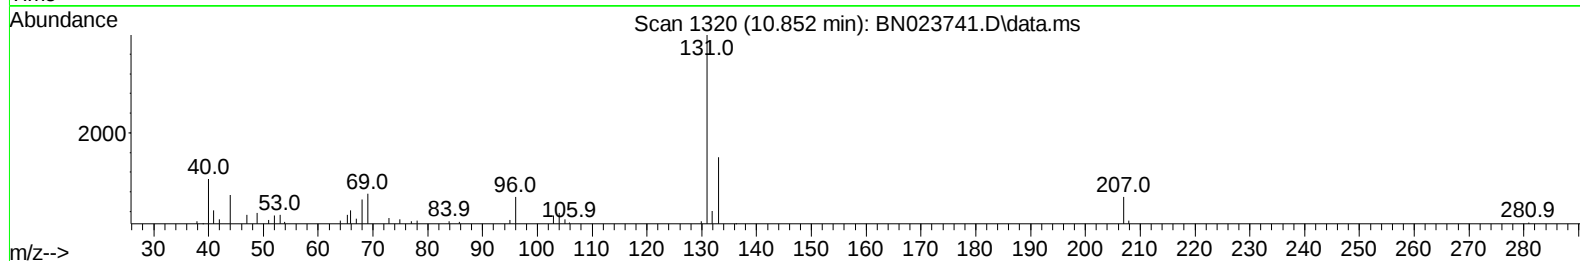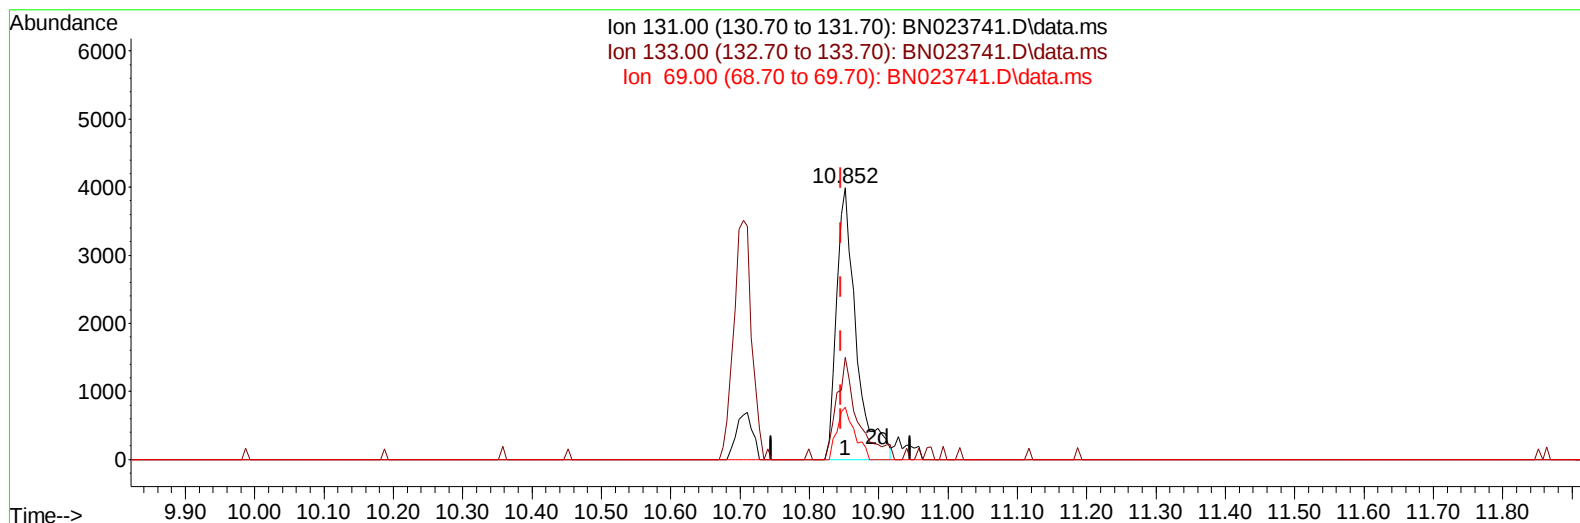

TIC: BN023741.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.852min (+ 0.006) 0.41 ng/ul m

response 7855

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.40	37.65
69.00	17.20	19.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023741.D
 Acq On : 21 Jan 2023 00:18
 Operator : CG/JU
 Sample : 01146-02MEDL 30X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A43Y5MEDL

Manual IntegrationsAPPROVED

Quant Time: Jan 21 01:38:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 20 23:02:18 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/23/2023
 Supervised By :Yogesh Patel 01/24/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	204994	20.000	ng/ul	0.00
20) Naphthalene-d8	10.705	136	802612	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.540	164	460511	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.287	188	986078	20.000	ng/ul	0.00
79) Chrysene-d12	21.469	240	802189	20.000	ng/ul	-0.02
88) Perylene-d12	23.886	264	806526	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.058	99	11476	0.632	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	9199	0.825	ng/ul	0.00
11) 2-Chlorophenol-d4	7.417	132	9155	0.658	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	7186	0.496	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	3690	0.610	ng/ul	0.00
24) 2-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
28) 2,4-Dichlorophenol-d3	10.322	165	6143	0.503	ng/ul	0.00
31) 4-Chloroaniline-d4	10.852	131	7855m	0.409	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	25173	0.735	ng/ul	0.00
49) Acenaphthylene-d8	14.234	160	23849	0.628	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.528	176	23973	0.819	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.381	188	32651	0.740	ng/ul	0.00
81) Pyrene-d10	19.675	212	36028	0.785	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.727	264	26780	0.671	ng/ul	-0.03
Target Compounds						
					Qvalue	
86) Bis(2-ethylhexyl)phtha...	21.380	149	826132	25.357	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023741.D
Acq On : 21 Jan 2023 00:18
Operator : CG/JU
Sample : 01146-02MEDL 30X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A43Y5MEDL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/23/2023
Supervised By :Yogesh Patel 01/24/2023

Quant Time: Jan 21 01:38:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 20 23:02:18 2023
Response via : Initial Calibration

