




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023743.D
Acq On : 21 Jan 2023 01:31
Operator : CG/JU
Sample : 01146-10MEDL 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4411MEDL

Manual IntegrationsAPPROVED

Quant Time: Jan 21 02:06:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 20 23:02:18 2023
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/23/2023
Supervised By :Yogesh Patel 01/24/2023

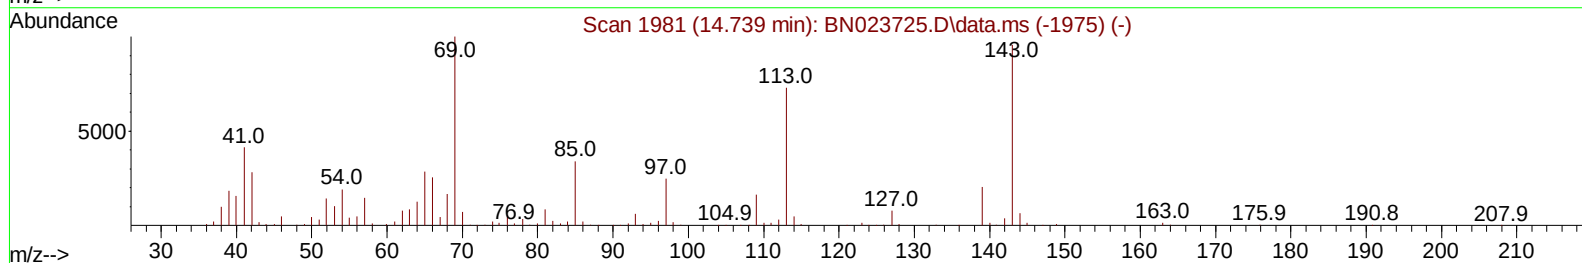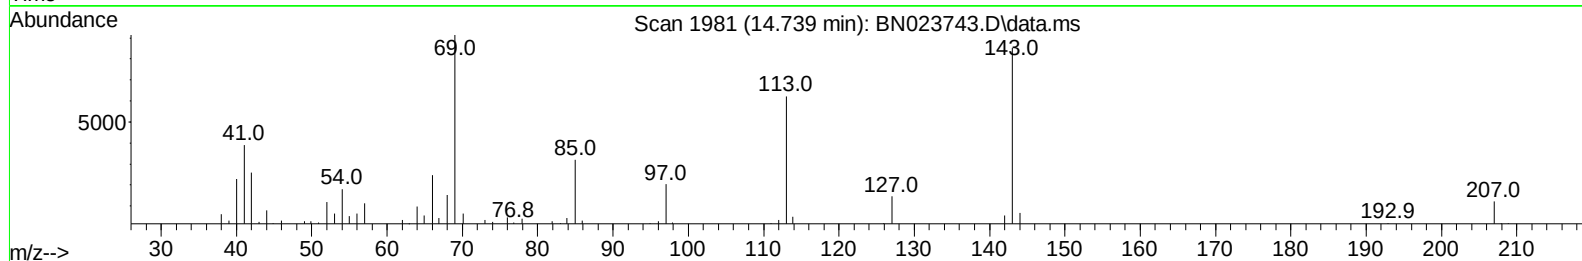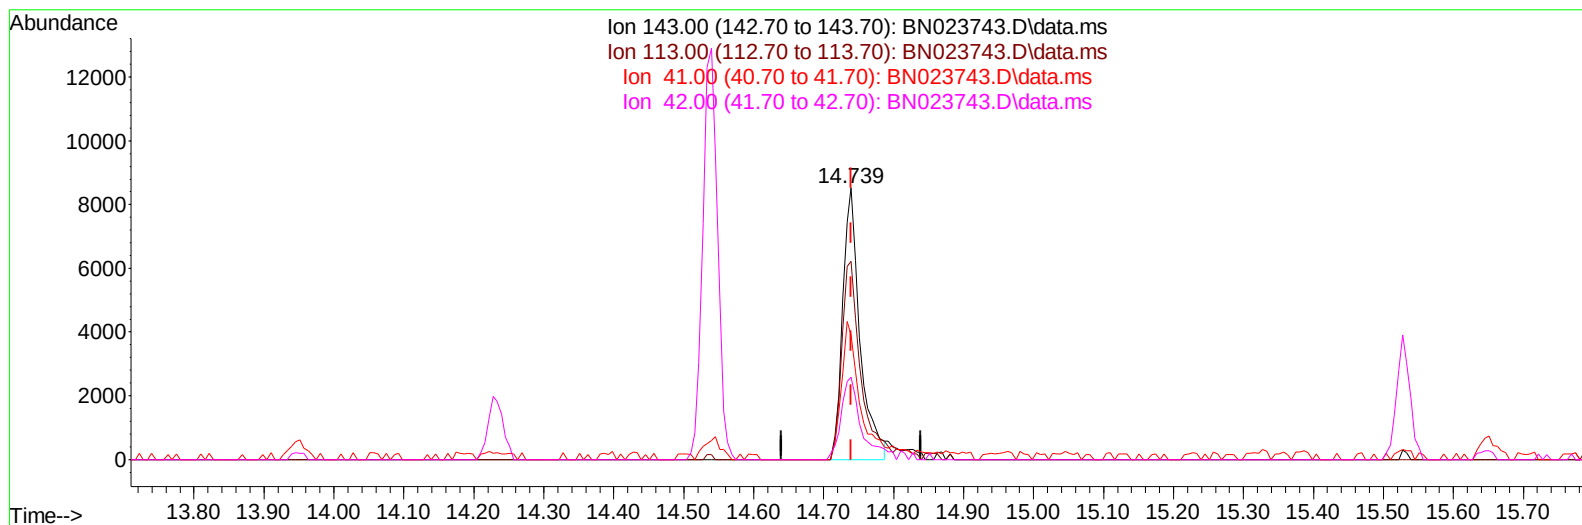

TIC: BN023743.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.739min (-0.000) 1.95 ng/u1

response 14543

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.00	73.05
41.00	40.90	45.82
42.00	27.80	30.26




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023743.D
Acq On : 21 Jan 2023 01:31
Operator : CG/JU
Sample : 01146-10MEDL 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4411MEDL

Manual IntegrationsAPPROVED

Quant Time: Jan 21 02:06:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 20 23:02:18 2023
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/23/2023
Supervised By :Yogesh Patel 01/24/2023

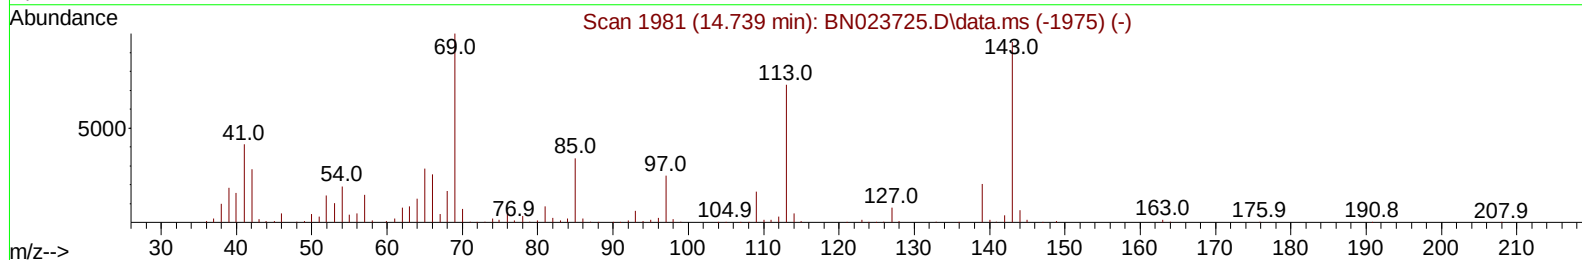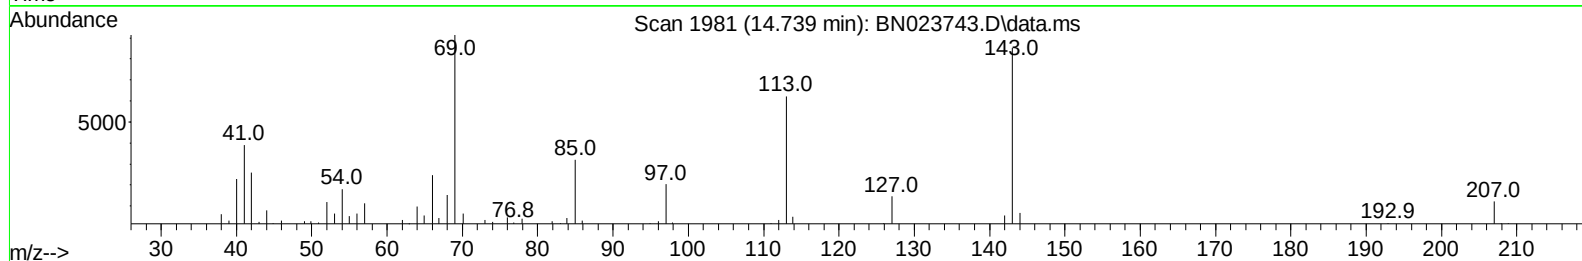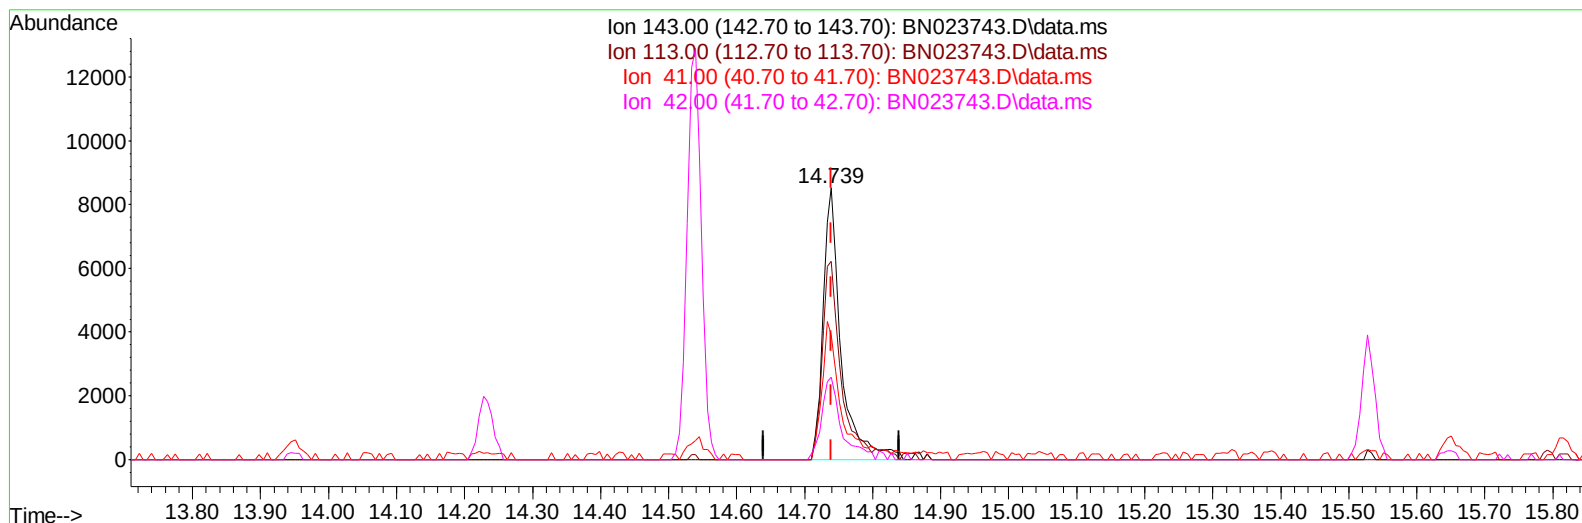

TIC: BN023743.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.739min (-0.000) 2.09 ng/ul m

response 15589

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.00	73.05
41.00	40.90	45.82
42.00	27.80	30.26

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023743.D
 Acq On : 21 Jan 2023 01:31
 Operator : CG/JU
 Sample : 01146-10MEDL 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4411MEDL

Manual IntegrationsAPPROVED

Quant Time: Jan 21 02:06:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 20 23:02:18 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/23/2023
 Supervised By :Yogesh Patel 01/24/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	196636	20.000	ng/ul	0.00
20) Naphthalene-d8	10.704	136	811956	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.539	164	493309	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.286	188	976170	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	1051832	20.000	ng/ul	0.00
88) Perylene-d12	23.898	264	1103224	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	5291	1.158	ng/uL	0.00
4) Pyridine-d5	3.710	84	46190	3.369	ng/ul	0.01
7) Phenol-d5	7.051	99	73041	4.191	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	51832	4.848	ng/ul	0.00
11) 2-Chlorophenol-d4	7.416	132	59343	4.446	ng/ul	0.00
15) 4-Methylphenol-d8	8.604	113	55163	3.966	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	26159	4.272	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	24295	3.748	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	49017	3.965	ng/ul	0.00
31) 4-Chloroaniline-d4	10.845	131	80441	4.137	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	179285	4.886	ng/ul	0.00
49) Acenaphthylene-d8	14.233	160	177819	4.373	ng/ul	0.00
54) 4-Nitrophenol-d4	14.739	143	15589m	2.087	ng/ul	0.00
60) Fluorene-d10	15.527	176	157585	5.026	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.380	188	228772	5.237	ng/ul	0.00
81) Pyrene-d10	19.674	212	278724	4.633	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.739	264	251244	4.605	ng/ul	-0.02
Target Compounds						
					Qvalue	
86) Bis(2-ethylhexyl)phtha...	21.386	149	1639574	38.380	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023743.D
Acq On : 21 Jan 2023 01:31
Operator : CG/JU
Sample : 01146-10MEDL 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4411MEDL

Manual IntegrationsAPPROVED

Quant Time: Jan 21 02:06:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 20 23:02:18 2023
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/23/2023
Supervised By :Yogesh Patel 01/24/2023

