

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023727.D
 Acq On : 20 Jan 2023 15:02
 Operator : CG/JU
 Sample : 01145-02ME
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A43S7ME

Quant Time: Jan 20 21:57:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 05 03:34:47 2023
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/23/2023
 Supervised By :Yogesh Patel 01/24/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	229141	20.000	ng/u1	0.00
20) Naphthalene-d8	10.705	136	953858	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.540	164	500177	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.287	188	1166211	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	821314	20.000	ng/u1	0.00
88) Perylene-d12	23.910	264	829591	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.276	96	33048	6.206	ng/uL	0.04
4) Pyridine-d5	3.699	84	429023	26.854	ng/u1	0.03
7) Phenol-d5	7.058	99	625727	30.812	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	396962	31.863	ng/u1	0.00
11) 2-Chlorophenol-d4	7.422	132	501378	32.236	ng/u1	0.00
15) 4-Methylphenol-d8	8.605	113	485043	29.924	ng/u1	0.00
21) Nitrobenzene-d5	9.063	128	238644	33.178	ng/u1	0.00
24) 2-Nitrophenol-d4	9.787	143	260190	34.172	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	458650	31.580	ng/u1	0.00
31) 4-Chloroaniline-d4	10.846	131	671699	29.403	ng/u1	0.00
46) Dimethylphthalate-d6	13.951	166	1170806	31.467	ng/u1	0.00
49) Acenaphthylene-d8	14.234	160	1374896	33.350	ng/u1	0.00
54) 4-Nitrophenol-d4	14.740	143	194961	25.739	ng/u1	0.00
60) Fluorene-d10	15.534	176	1163165	36.585	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	109021	15.497	ng/u1	0.00
73) Anthracene-d10	17.387	188	1661320	31.834	ng/u1	0.00
81) Pyrene-d10	19.681	212	1798193	38.282	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.745	264	1375753	33.534	ng/u1	0.00

Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.422	149	23996794m	719.399	ng/u1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023727.D
Acq On : 20 Jan 2023 15:02
Operator : CG/JU
Sample : 01145-02ME
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A43S7ME

Quant Time: Jan 20 21:57:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 05 03:34:47 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 01/23/2023
Supervised By :Yogesh Patel 01/24/2023

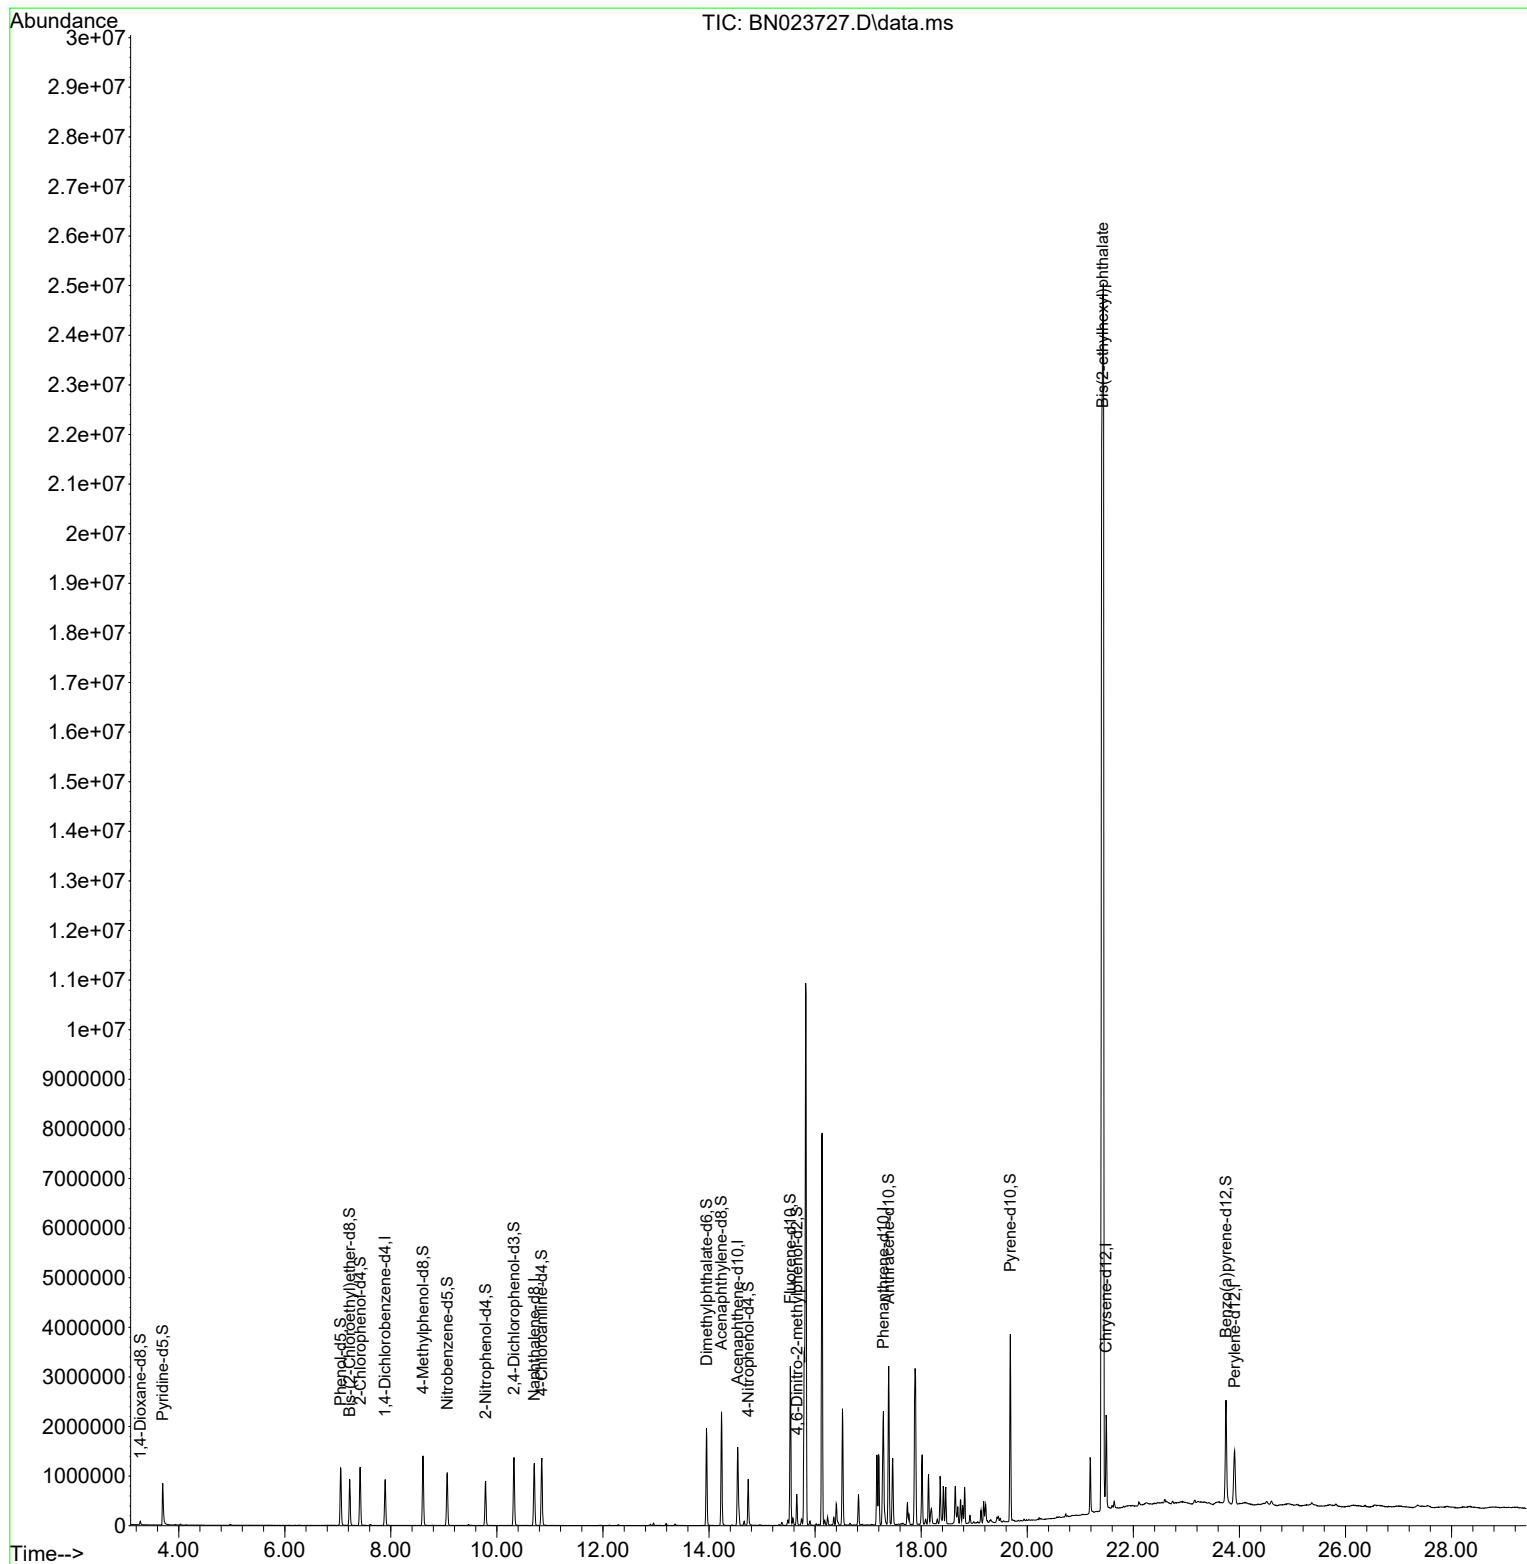

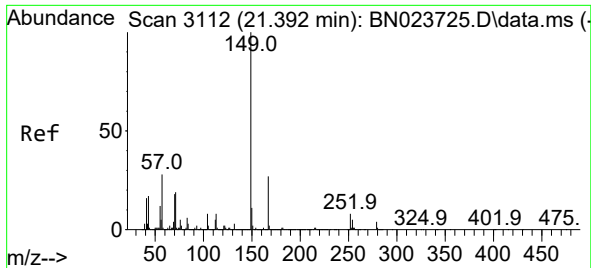

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 719.399 ng/ul m
 RT: 21.422 min Scan# 3117
 Delta R.T. 0.031 min
 Lab File: BN023727.D
 Acq: 20 Jan 2023 15:02

Instrument :
 BNA_N
 ClientSampleId :
 A43S7ME

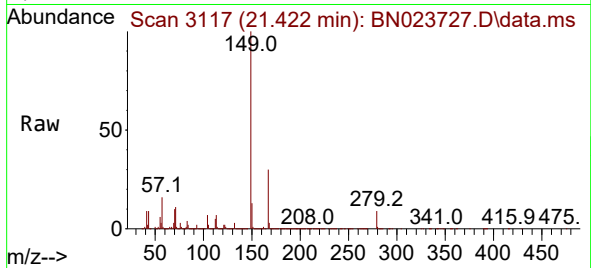

Tgt Ion:149 Resp:23996794
 Ion Ratio Lower Upper
 149 100
 167 30.4 22.0 33.0
 279 8.5 3.4 5.2

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/23/2023
 Supervised By :Yogesh Patel 01/24/2023

