

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023730.D
 Acq On : 20 Jan 2023 16:52
 Operator : CG/JU
 Sample : 01146-08ME
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4405ME

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/23/2023
 Supervised By :Yogesh Patel 01/24/2023

Quant Time: Jan 20 21:57:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 05 03:34:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	200717	20.000	ng/u1	0.00
20) Naphthalene-d8	10.704	136	861177	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.539	164	474403	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.286	188	868469	20.000	ng/u1	0.00
79) Chrysene-d12	21.492	240	638883	20.000	ng/u1	0.00
88) Perylene-d12	23.910	264	652905	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	22751	4.878	ng/uL	0.04
4) Pyridine-d5	3.699	84	301928	21.575	ng/u1	0.03
7) Phenol-d5	7.057	99	425709	23.931	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	267371	24.500	ng/u1	0.00
11) 2-Chlorophenol-d4	7.422	132	359291	26.372	ng/u1	0.00
15) 4-Methylphenol-d8	8.604	113	346146	24.379	ng/u1	0.00
21) Nitrobenzene-d5	9.063	128	154208	23.747	ng/u1	0.00
24) 2-Nitrophenol-d4	9.787	143	172715	25.124	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	312118	23.803	ng/u1	0.00
31) 4-Chloroaniline-d4	10.845	131	309607	15.011	ng/u1	0.00
46) Dimethylphthalate-d6	13.951	166	913399	25.883	ng/u1	0.00
49) Acenaphthylene-d8	14.234	160	1061300	27.142	ng/u1	0.00
54) 4-Nitrophenol-d4	14.739	143	128427	17.876	ng/u1	0.00
60) Fluorene-d10	15.533	176	767835	25.463	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	77817	14.853	ng/u1	0.00
73) Anthracene-d10	17.386	188	1012331	26.049	ng/u1	0.00
81) Pyrene-d10	19.680	212	1136568	31.106	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.762	264	829252	25.683	ng/u1	0.01

Target Compounds Qvalue
 86) Bis(2-ethylhexyl)phtha... 21.421 149 33965847m 1309.022 ng/u1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023730.D
Acq On : 20 Jan 2023 16:52
Operator : CG/JU
Sample : 01146-08ME
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A4405ME

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 01/23/2023
Supervised By :Yogesh Patel 01/24/2023

Quant Time: Jan 20 21:57:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 05 03:34:47 2023
Response via : Initial Calibration

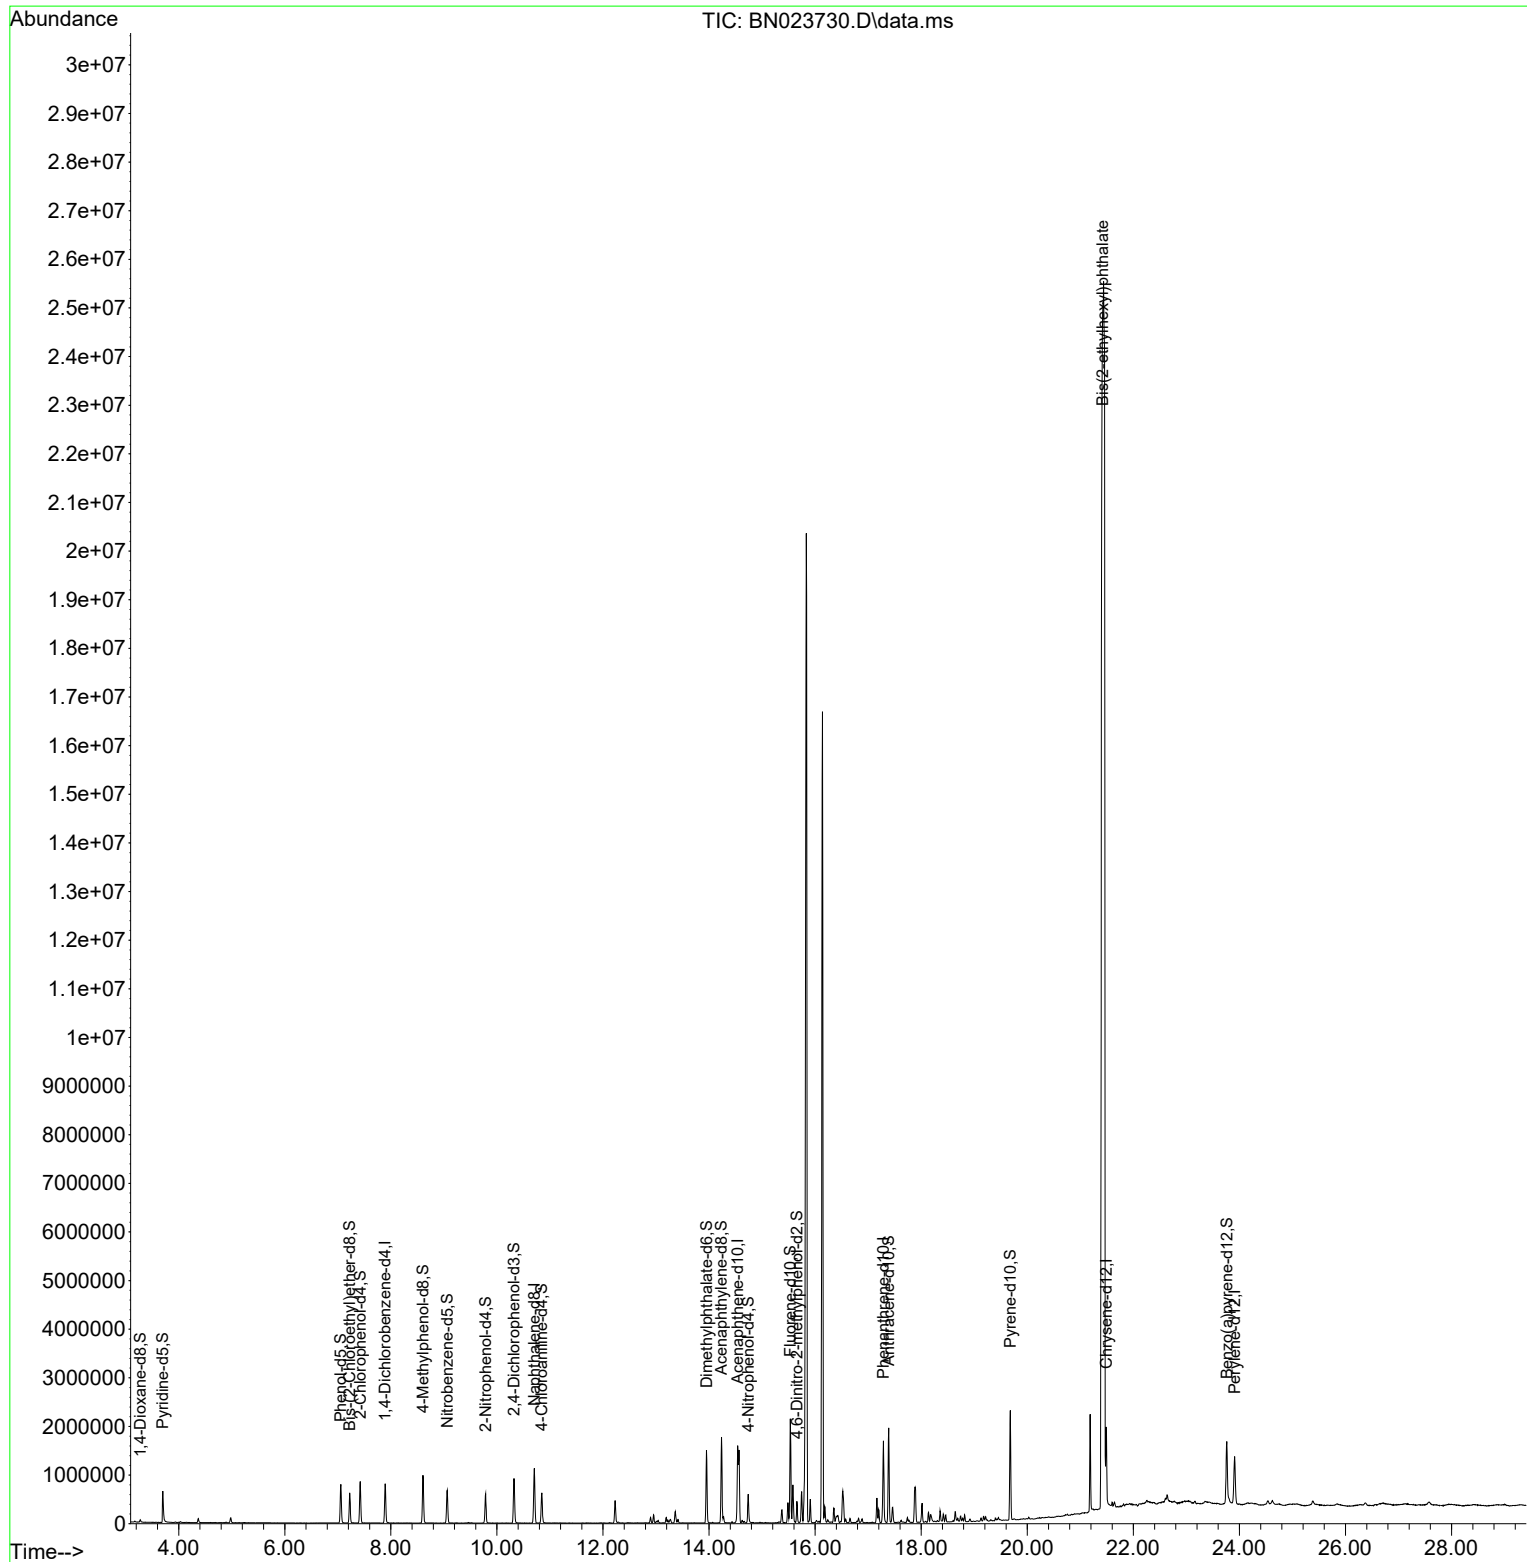

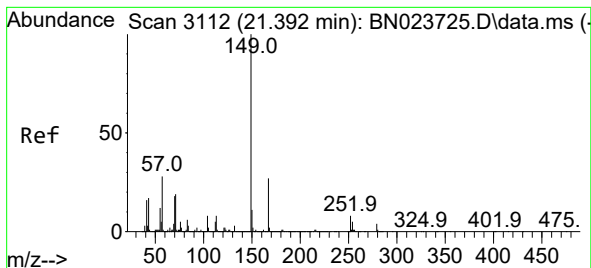

#86

Bis(2-ethylhexyl)phthalate

Concen: 1309.022 ng/ul m

RT: 21.421 min Scan# 3117

Delta R.T. 0.030 min

Lab File: BN023730.D


Acq: 20 Jan 2023 16:52

Instrument :

BNA_N

ClientSampleId :

A4405ME

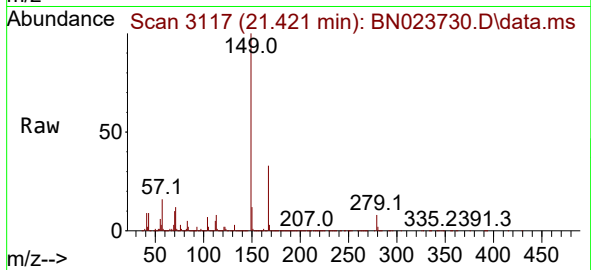

Tgt Ion:149 Resp:3396584

Ion Ratio Lower Upper

149 100

167 32.6 22.0 33.0

279 7.9 3.4 5.2

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 01/23/2023

Supervised By :Yogesh Patel 01/24/2023

