

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023731.D
 Acq On : 20 Jan 2023 17:30
 Operator : CG/JU
 Sample : 01146-10ME
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4411ME

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/23/2023
 Supervised By :Yogesh Patel 01/24/2023

Quant Time: Jan 20 23:40:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 20 23:02:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	211280	20.000	ng/u1	0.00
20) Naphthalene-d8	10.704	136	761873	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.539	164	516680	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.286	188	1116049	20.000	ng/u1	0.00
79) Chrysene-d12	21.480	240	1007179	20.000	ng/u1	0.00
88) Perylene-d12	23.904	264	1102799	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	23032	4.691	ng/uL	0.00
4) Pyridine-d5	3.699	84	284262	19.297	ng/u1	0.00
7) Phenol-d5	7.058	99	415016	22.164	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	266849	23.230	ng/u1	0.00
11) 2-Chlorophenol-d4	7.422	132	337377	23.525	ng/u1	0.00
15) 4-Methylphenol-d8	8.604	113	324801	21.732	ng/u1	0.00
21) Nitrobenzene-d5	9.063	128	153932	26.794	ng/u1	0.00
24) 2-Nitrophenol-d4	9.787	143	165111	27.149	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	266709	22.992	ng/u1	0.00
31) 4-Chloroaniline-d4	10.846	131	409998	22.470	ng/u1	0.00
46) Dimethylphthalate-d6	13.951	166	952341	24.778	ng/u1	0.00
49) Acenaphthylene-d8	14.234	160	1061802	24.933	ng/u1	0.00
54) 4-Nitrophenol-d4	14.739	143	147621	18.866	ng/u1	0.00
60) Fluorene-d10	15.534	176	823071	25.061	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	85964	12.768	ng/u1	0.00
73) Anthracene-d10	17.386	188	1265856	25.347	ng/u1	0.00
81) Pyrene-d10	19.680	212	1476033	25.625	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.751	264	1382378	25.348	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.398	149	6613043	161.667	ng/u1	Qvalue 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023731.D
Acq On : 20 Jan 2023 17:30
Operator : CG/JU
Sample : 01146-10ME
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A4411ME

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 01/23/2023
Supervised By :Yogesh Patel 01/24/2023


Quant Time: Jan 20 23:40:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 20 23:02:18 2023
Response via : Initial Calibration

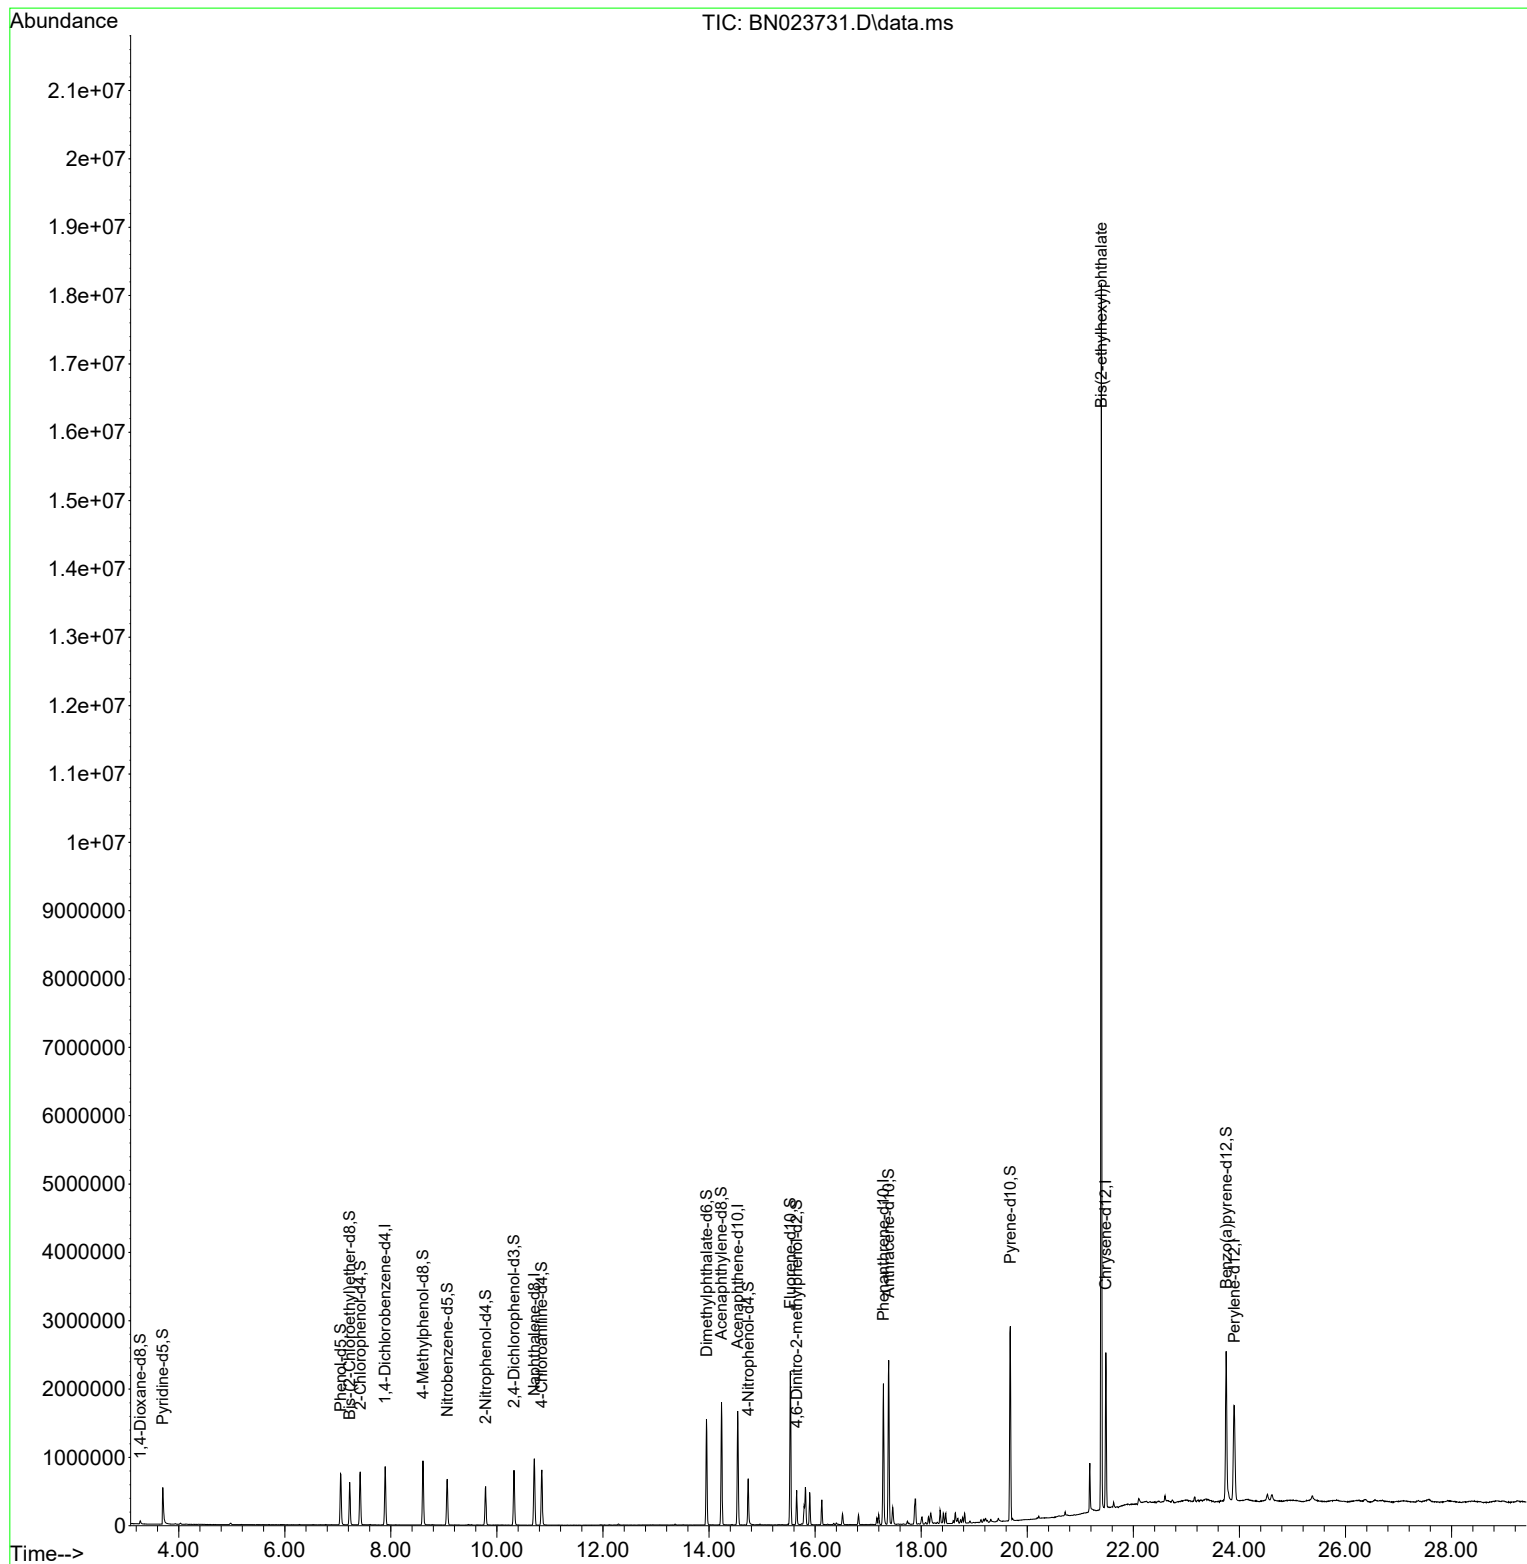

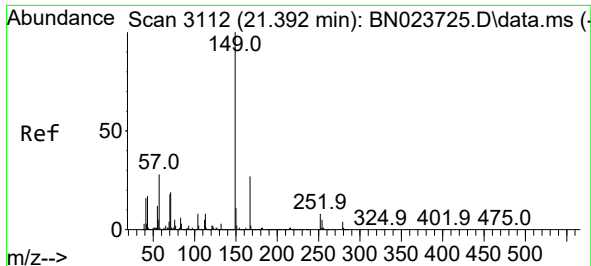

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 161.667 ng/ul
 RT: 21.398 min Scan# 3113
 Delta R.T. 0.006 min
 Lab File: BN023731.D
 Acq: 20 Jan 2023 17:30

Instrument :
 BNA_N
 ClientSampleId :
 A4411ME

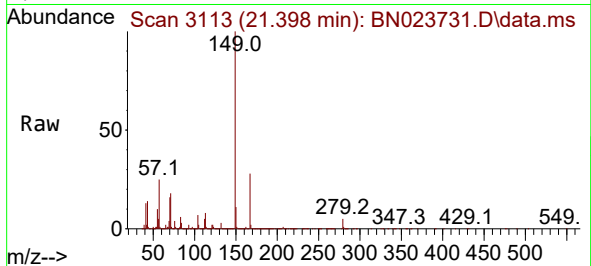

Tgt Ion:149 Resp: 661304
 Ion Ratio Lower Upper
 149 100
 167 27.6 22.0 33.0
 279 5.0 3.4 5.2

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/23/2023
 Supervised By :Yogesh Patel 01/24/2023

