

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023732.D
 Acq On : 20 Jan 2023 18:07
 Operator : CG/JU
 Sample : 01146-11ME
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4412ME

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/23/2023
 Supervised By :Yogesh Patel 01/24/2023

Quant Time: Jan 20 23:38:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 20 23:02:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	232118	20.000	ng/u1	0.00
20) Naphthalene-d8	10.704	136	874381	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.540	164	586241	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.286	188	1248152	20.000	ng/u1	0.00
79) Chrysene-d12	21.486	240	995806	20.000	ng/u1	0.00
88) Perylene-d12	23.910	264	1034812	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	25027	4.640	ng/uL	0.00
4) Pyridine-d5	3.699	84	313074	19.345	ng/u1	0.00
7) Phenol-d5	7.058	99	436850	21.235	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	279941	22.182	ng/u1	0.00
11) 2-Chlorophenol-d4	7.422	132	354061	22.472	ng/u1	0.00
15) 4-Methylphenol-d8	8.605	113	345203	21.023	ng/u1	0.00
21) Nitrobenzene-d5	9.063	128	167891	25.463	ng/u1	0.00
24) 2-Nitrophenol-d4	9.787	143	172903	24.772	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	276581	20.775	ng/u1	0.00
31) 4-Chloroaniline-d4	10.846	131	457505	21.847	ng/u1	0.00
46) Dimethylphthalate-d6	13.951	166	993457	22.781	ng/u1	0.00
49) Acenaphthylene-d8	14.234	160	1124490	23.272	ng/u1	0.00
54) 4-Nitrophenol-d4	14.740	143	151512	17.066	ng/u1	0.00
60) Fluorene-d10	15.534	176	854119	22.921	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	90328	11.997	ng/u1	0.00
73) Anthracene-d10	17.386	188	1322362	23.676	ng/u1	0.00
81) Pyrene-d10	19.680	212	1493783	26.229	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.757	264	1177072	23.001	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.404	149	7604506	188.028	ng/u1	Qvalue 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023732.D
Acq On : 20 Jan 2023 18:07
Operator : CG/JU
Sample : 01146-11ME
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A4412ME

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 01/23/2023
Supervised By :Yogesh Patel 01/24/2023


Quant Time: Jan 20 23:38:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 20 23:02:18 2023
Response via : Initial Calibration

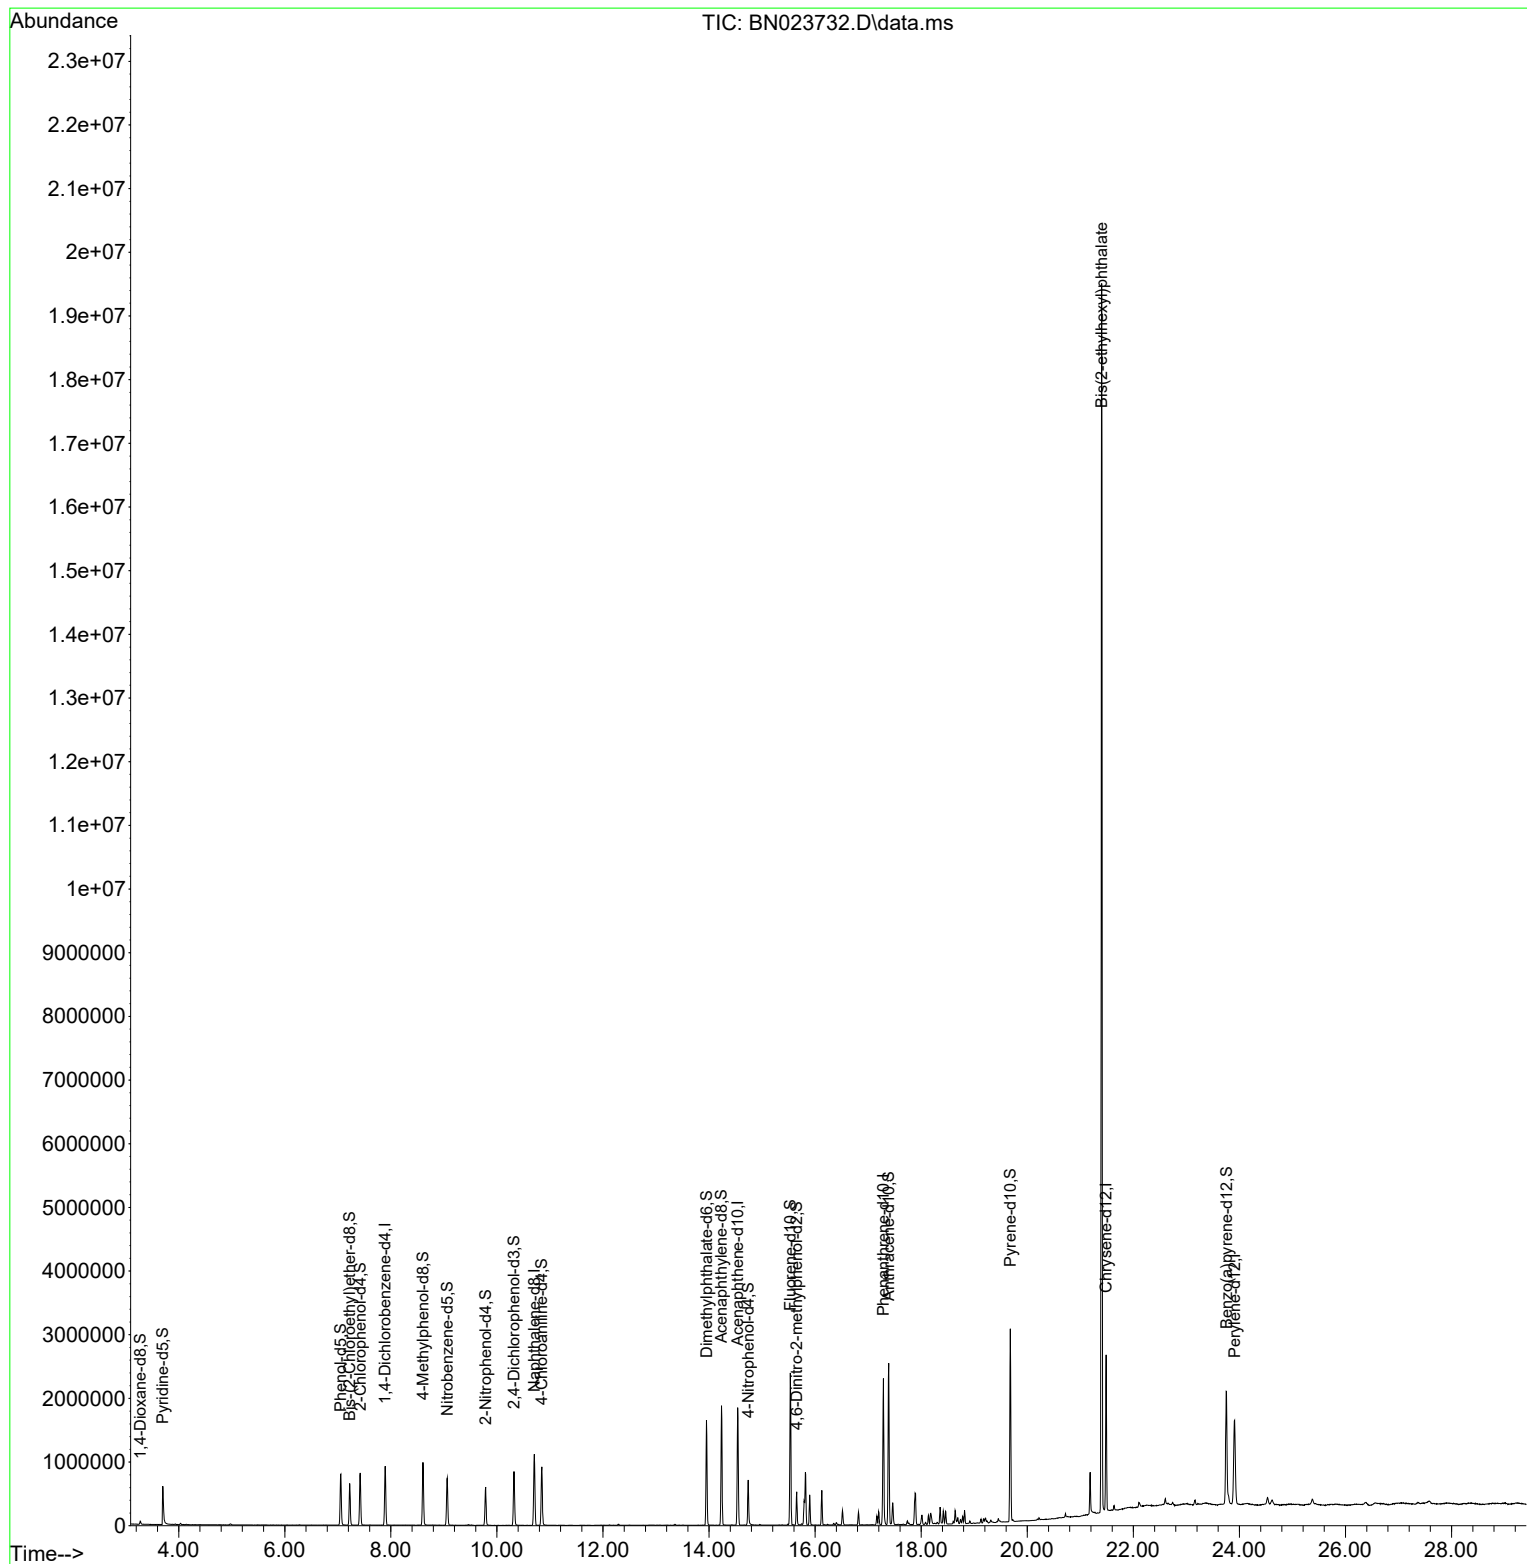

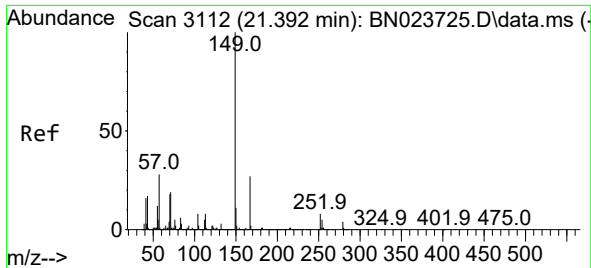

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 188.028 ng/ul
 RT: 21.404 min Scan# 3114
 Delta R.T. 0.012 min
 Lab File: BN023732.D
 Acq: 20 Jan 2023 18:07

Instrument :
 BNA_N
 ClientSampleId :
 A4412ME

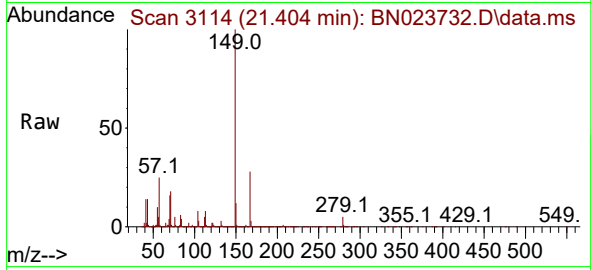

Tgt Ion:149 Resp: 7604500
 Ion Ratio Lower Upper
 149 100
 167 27.5 22.0 33.0
 279 5.1 3.4 5.2

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/23/2023
 Supervised By :Yogesh Patel 01/24/2023

