

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023733.D
 Acq On : 20 Jan 2023 18:44
 Operator : CG/JU
 Sample : 01146-12ME
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4418ME

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/23/2023
 Supervised By :Yogesh Patel 01/24/2023

Quant Time: Jan 20 23:04:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 20 23:02:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	201248	20.000	ng/u1	0.00
20) Naphthalene-d8	10.704	136	817380	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.539	164	490980	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.286	188	1072021	20.000	ng/u1	0.00
79) Chrysene-d12	21.480	240	971960	20.000	ng/u1	0.00
88) Perylene-d12	23.915	264	1012137	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	25602	5.474	ng/uL	0.00
4) Pyridine-d5	3.699	84	331837	23.649	ng/u1	0.00
7) Phenol-d5	7.058	99	486981	27.303	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	304953	27.870	ng/u1	0.00
11) 2-Chlorophenol-d4	7.422	132	390432	28.582	ng/u1	0.00
15) 4-Methylphenol-d8	8.604	113	384381	27.000	ng/u1	0.00
21) Nitrobenzene-d5	9.063	128	184341	29.908	ng/u1	0.00
24) 2-Nitrophenol-d4	9.787	143	201533	30.887	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	358714	28.823	ng/u1	0.00
31) 4-Chloroaniline-d4	10.846	131	524938	26.815	ng/u1	0.00
46) Dimethylphthalate-d6	13.951	166	1058903	28.993	ng/u1	0.00
49) Acenaphthylene-d8	14.234	160	1232019	30.444	ng/u1	0.00
54) 4-Nitrophenol-d4	14.739	143	176356	23.718	ng/u1	0.00
60) Fluorene-d10	15.534	176	920234	29.487	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	108668	16.804	ng/u1	0.00
73) Anthracene-d10	17.386	188	1414846	29.493	ng/u1	0.00
81) Pyrene-d10	19.680	212	1673729	30.110	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.745	264	1500022	29.969	ng/u1	-0.01

Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.421	149	27170372m	688.292	ng/u1

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023733.D
Acq On : 20 Jan 2023 18:44
Operator : CG/JU
Sample : 01146-12ME
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A4418ME

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 01/23/2023
Supervised By :Yogesh Patel 01/24/2023


Quant Time: Jan 20 23:04:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 20 23:02:18 2023
Response via : Initial Calibration

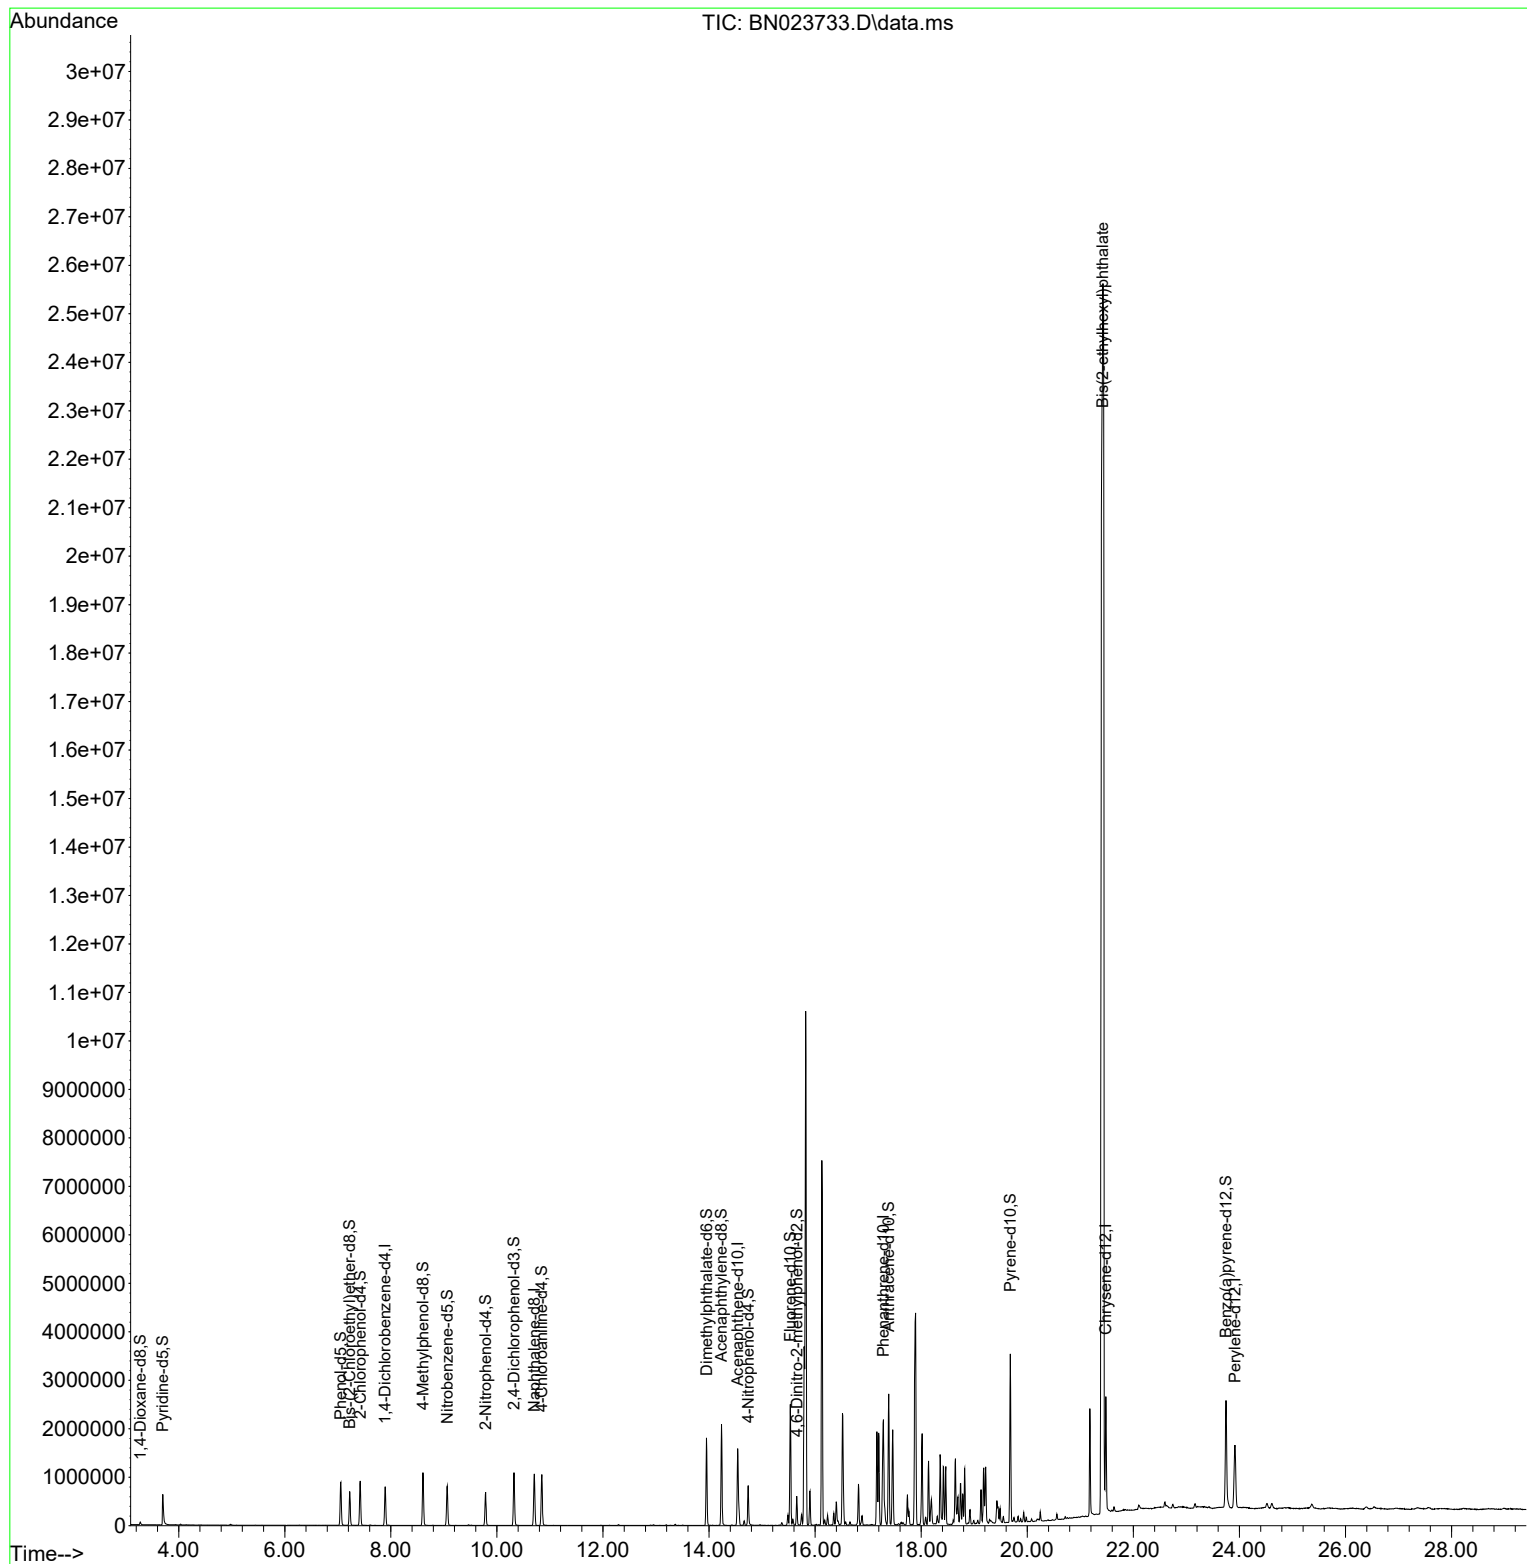

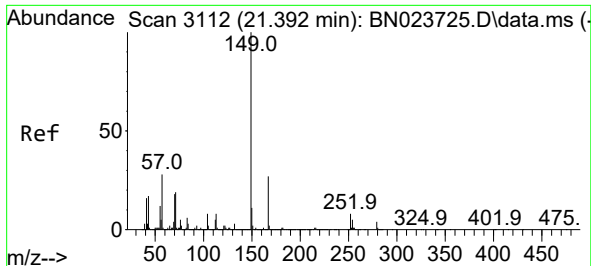

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 688.292 ng/ul m
 RT: 21.421 min Scan# 3117
 Delta R.T. 0.030 min
 Lab File: BN023733.D
 Acq: 20 Jan 2023 18:44

Instrument :
 BNA_N
 ClientSampleId :
 A4418ME

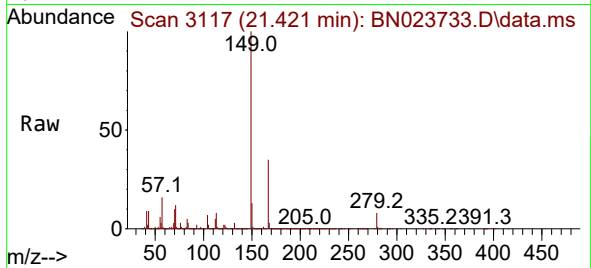

Tgt Ion:149 Resp:27170372
 Ion Ratio Lower Upper
 149 100
 167 35.2 22.0 33.0
 279 7.7 3.4 5.2

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 01/23/2023
 Supervised By :Yogesh Patel 01/24/2023

