

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023735.D
 Acq On : 20 Jan 2023 19:59
 Operator : CG/JU
 Sample : 01146-16ME
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4470ME

Quant Time: Jan 20 23:18:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 20 23:02:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	190769	20.000	ng/ul	0.00
20) Naphthalene-d8	10.704	136	797243	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.539	164	488657	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.286	188	1092063	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	867967	20.000	ng/ul	0.00
88) Perylene-d12	23.915	264	838426	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	22239	5.017	ng/uL	0.00
4) Pyridine-d5	3.699	84	282290	21.223	ng/ul	0.00
7) Phenol-d5	7.058	99	381464	22.562	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	246220	23.739	ng/ul	0.00
11) 2-Chlorophenol-d4	7.422	132	305903	23.624	ng/ul	0.00
15) 4-Methylphenol-d8	8.604	113	308619	22.869	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	151238	25.157	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	154065	24.209	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	269874	22.232	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	433420	22.699	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	938566	25.820	ng/ul	0.00
49) Acenaphthylene-d8	14.234	160	1054567	26.183	ng/ul	0.00
54) 4-Nitrophenol-d4	14.739	143	72770	9.834	ng/ul	0.00
60) Fluorene-d10	15.534	176	806412	25.962	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	38524	5.848	ng/ul	0.00
73) Anthracene-d10	17.386	188	1208028	24.720	ng/ul	0.00
81) Pyrene-d10	19.680	212	1388026	27.962	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.745	264	1097524	26.470	ng/ul	-0.01


Target Compounds					Qvalue	
86) Bis(2-ethylhexyl)phtha...	21.398	149	7947994	225.465	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023735.D
Acq On : 20 Jan 2023 19:59
Operator : CG/JU
Sample : 01146-16ME
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4470ME

Quant Time: Jan 20 23:18:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 20 23:02:18 2023
Response via : Initial Calibration

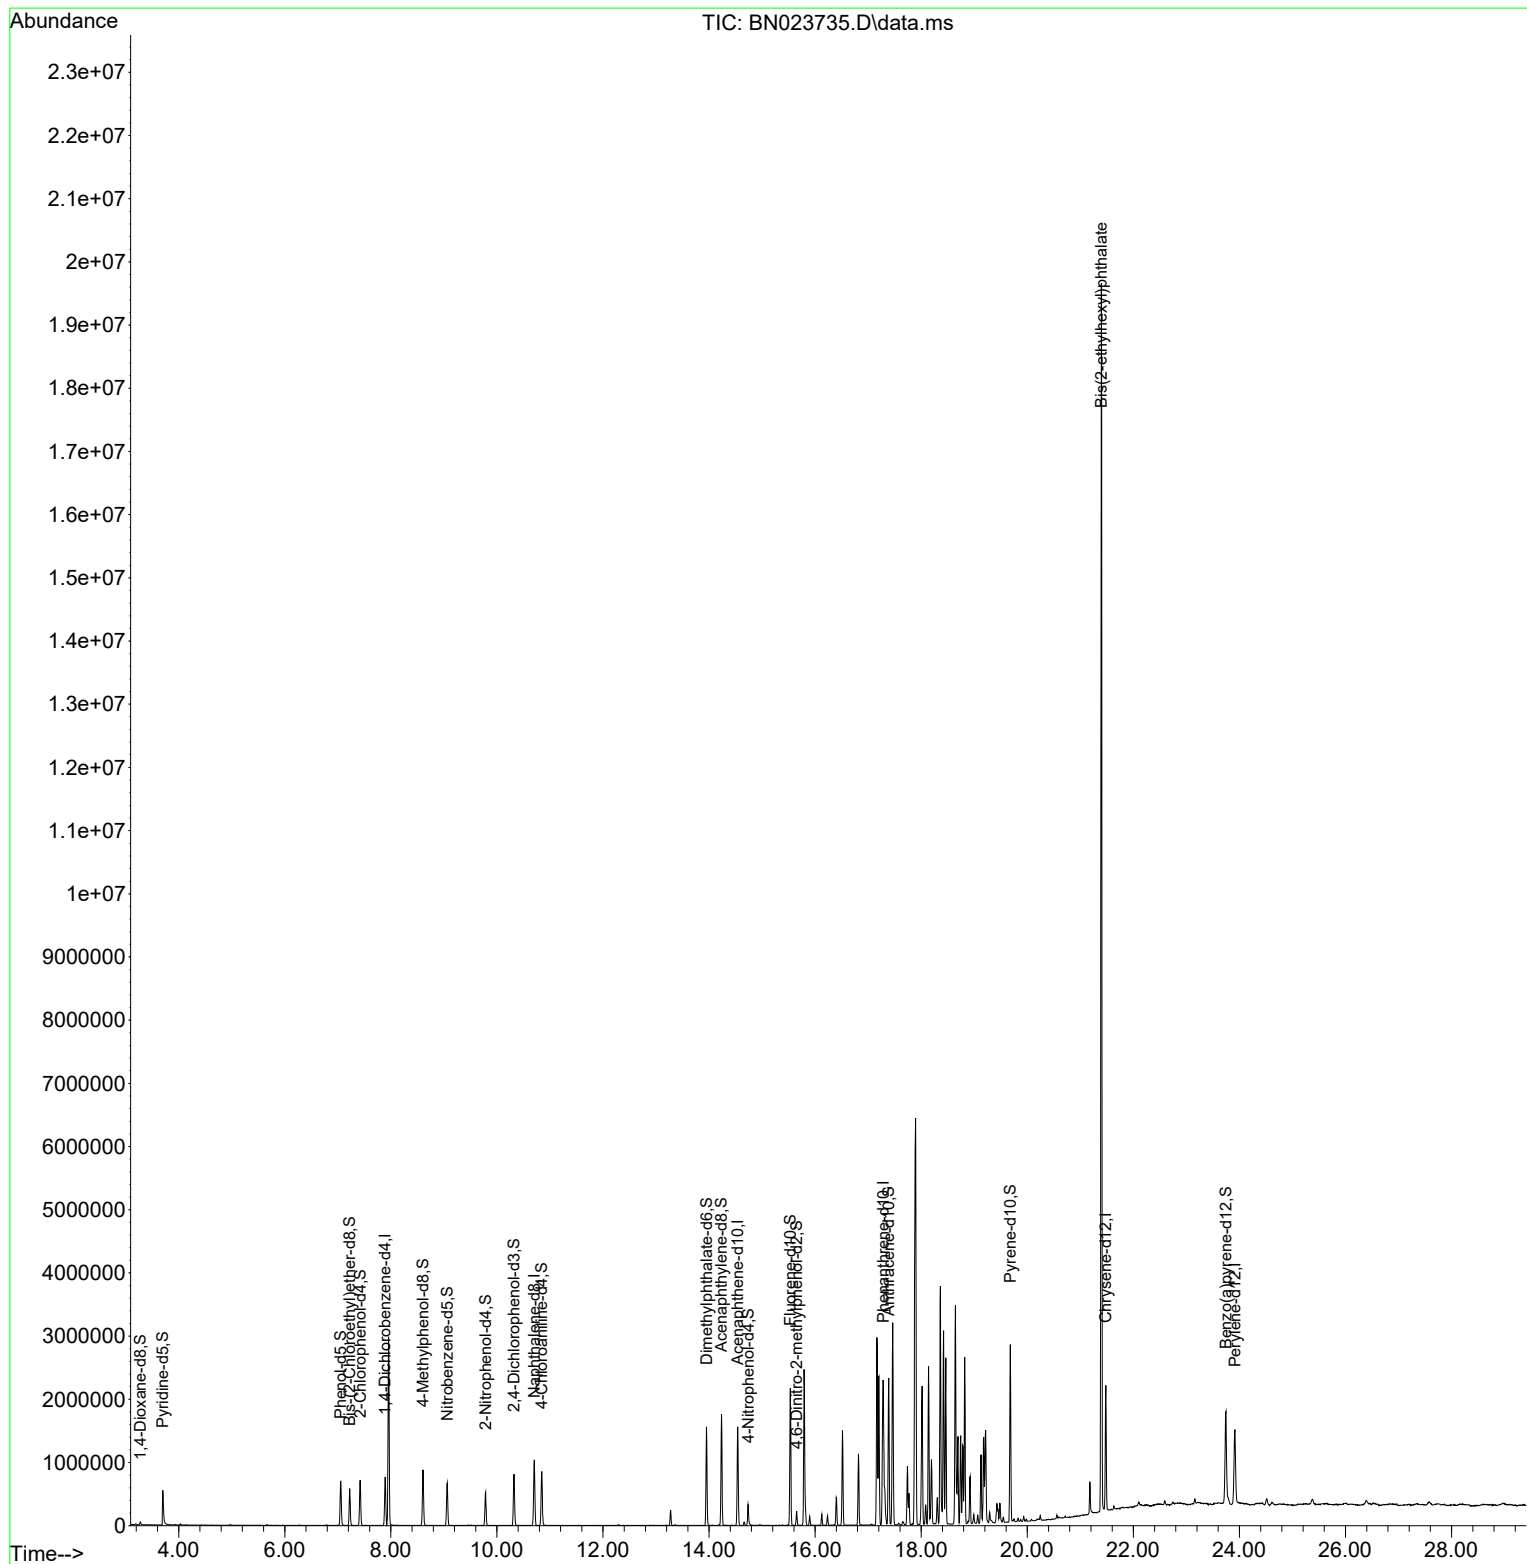

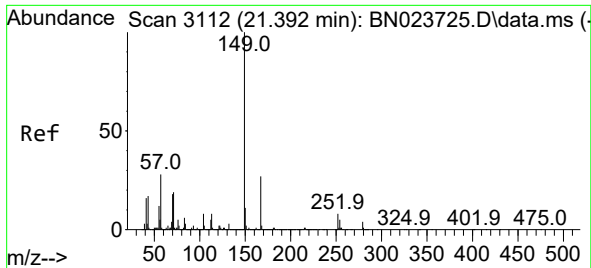

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 225.465 ng/ul
 RT: 21.398 min Scan# 3113
 Delta R.T. 0.006 min
 Lab File: BN023735.D
 Acq: 20 Jan 2023 19:59

Instrument :
 BNA_N
 ClientSampleId :
 A4470ME

Tgt Ion:149 Resp: 7947994
 Ion Ratio Lower Upper
 149 100
 167 29.4 22.0 33.0
 279 5.3 3.4 5.2#

