

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN012023\  
 Data File : BN023739.D  
 Acq On : 20 Jan 2023 23:04  
 Operator : CG/JU  
 Sample : 01145-02MEDL 50X  
 Misc :  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 A43S7MEDL

Quant Time: Jan 20 23:34:38 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN010523.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Fri Jan 20 23:02:18 2023  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|-------------------------------|--------|------|----------|--------|-------|----------|
| Internal Standards            |        |      |          |        |       |          |
| 1) 1,4-Dichlorobenzene-d4     | 7.893  | 152  | 214712   | 20.000 | ng/ul | 0.00     |
| 20) Naphthalene-d8            | 10.699 | 136  | 734012   | 20.000 | ng/ul | 0.00     |
| 38) Acenaphthene-d10          | 14.540 | 164  | 510585   | 20.000 | ng/ul | 0.00     |
| 64) Phenanthrene-d10          | 17.287 | 188  | 1078564  | 20.000 | ng/ul | 0.00     |
| 79) Chrysene-d12              | 21.475 | 240  | 864793   | 20.000 | ng/ul | -0.01    |
| 88) Perylene-d12              | 23.892 | 264  | 818079   | 20.000 | ng/ul | -0.02    |
| System Monitoring Compounds   |        |      |          |        |       |          |
| 3) 1,4-Dioxane-d8             | 0.000  | 96   | 0d       | 0.000  | ng/uL |          |
| 4) Pyridine-d5                | 0.000  | 84   | 0d       | 0.000  | ng/ul |          |
| 7) Phenol-d5                  | 7.052  | 99   | 9679     | 0.509  | ng/ul | 0.00     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.222  | 67   | 7804     | 0.668  | ng/ul | 0.00     |
| 11) 2-Chlorophenol-d4         | 7.417  | 132  | 8039     | 0.552  | ng/ul | 0.00     |
| 15) 4-Methylphenol-d8         | 8.605  | 113  | 6948     | 0.457  | ng/ul | 0.00     |
| 21) Nitrobenzene-d5           | 9.063  | 128  | 3370     | 0.609  | ng/ul | 0.00     |
| 24) 2-Nitrophenol-d4          | 9.787  | 143  | 2748     | 0.469  | ng/ul | 0.00     |
| 28) 2,4-Dichlorophenol-d3     | 10.322 | 165  | 4996     | 0.447  | ng/ul | 0.00     |
| 31) 4-Chloroaniline-d4        | 10.846 | 131  | 8798     | 0.500  | ng/ul | 0.00     |
| 46) Dimethylphthalate-d6      | 13.951 | 166  | 25286    | 0.666  | ng/ul | 0.00     |
| 49) Acenaphthylene-d8         | 14.234 | 160  | 23100    | 0.549  | ng/ul | 0.00     |
| 54) 4-Nitrophenol-d4          | 0.000  | 143  | 0d       | 0.000  | ng/ul |          |
| 60) Fluorene-d10              | 15.534 | 176  | 22058    | 0.680  | ng/ul | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 0.000  | 200  | 0d       | 0.000  | ng/ul |          |
| 73) Anthracene-d10            | 17.381 | 188  | 30240    | 0.627  | ng/ul | 0.00     |
| 81) Pyrene-d10                | 19.675 | 212  | 33851    | 0.684  | ng/ul | 0.00     |
| 92) Benzo(a)pyrene-d12        | 23.733 | 264  | 22702    | 0.561  | ng/ul | -0.02    |
| Target Compounds              |        |      |          |        |       |          |
| 86) Bis(2-ethylhexyl)phtha... | 21.386 | 149  | 1692843  | 48.198 | ng/ul | 98       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN012023\  
Data File : BN023739.D  
Acq On : 20 Jan 2023 23:04  
Operator : CG/JU  
Sample : 01145-02MEDL 50X  
Misc :  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
A43S7MEDL

Quant Time: Jan 20 23:34:38 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN010523.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Fri Jan 20 23:02:18 2023  
Response via : Initial Calibration

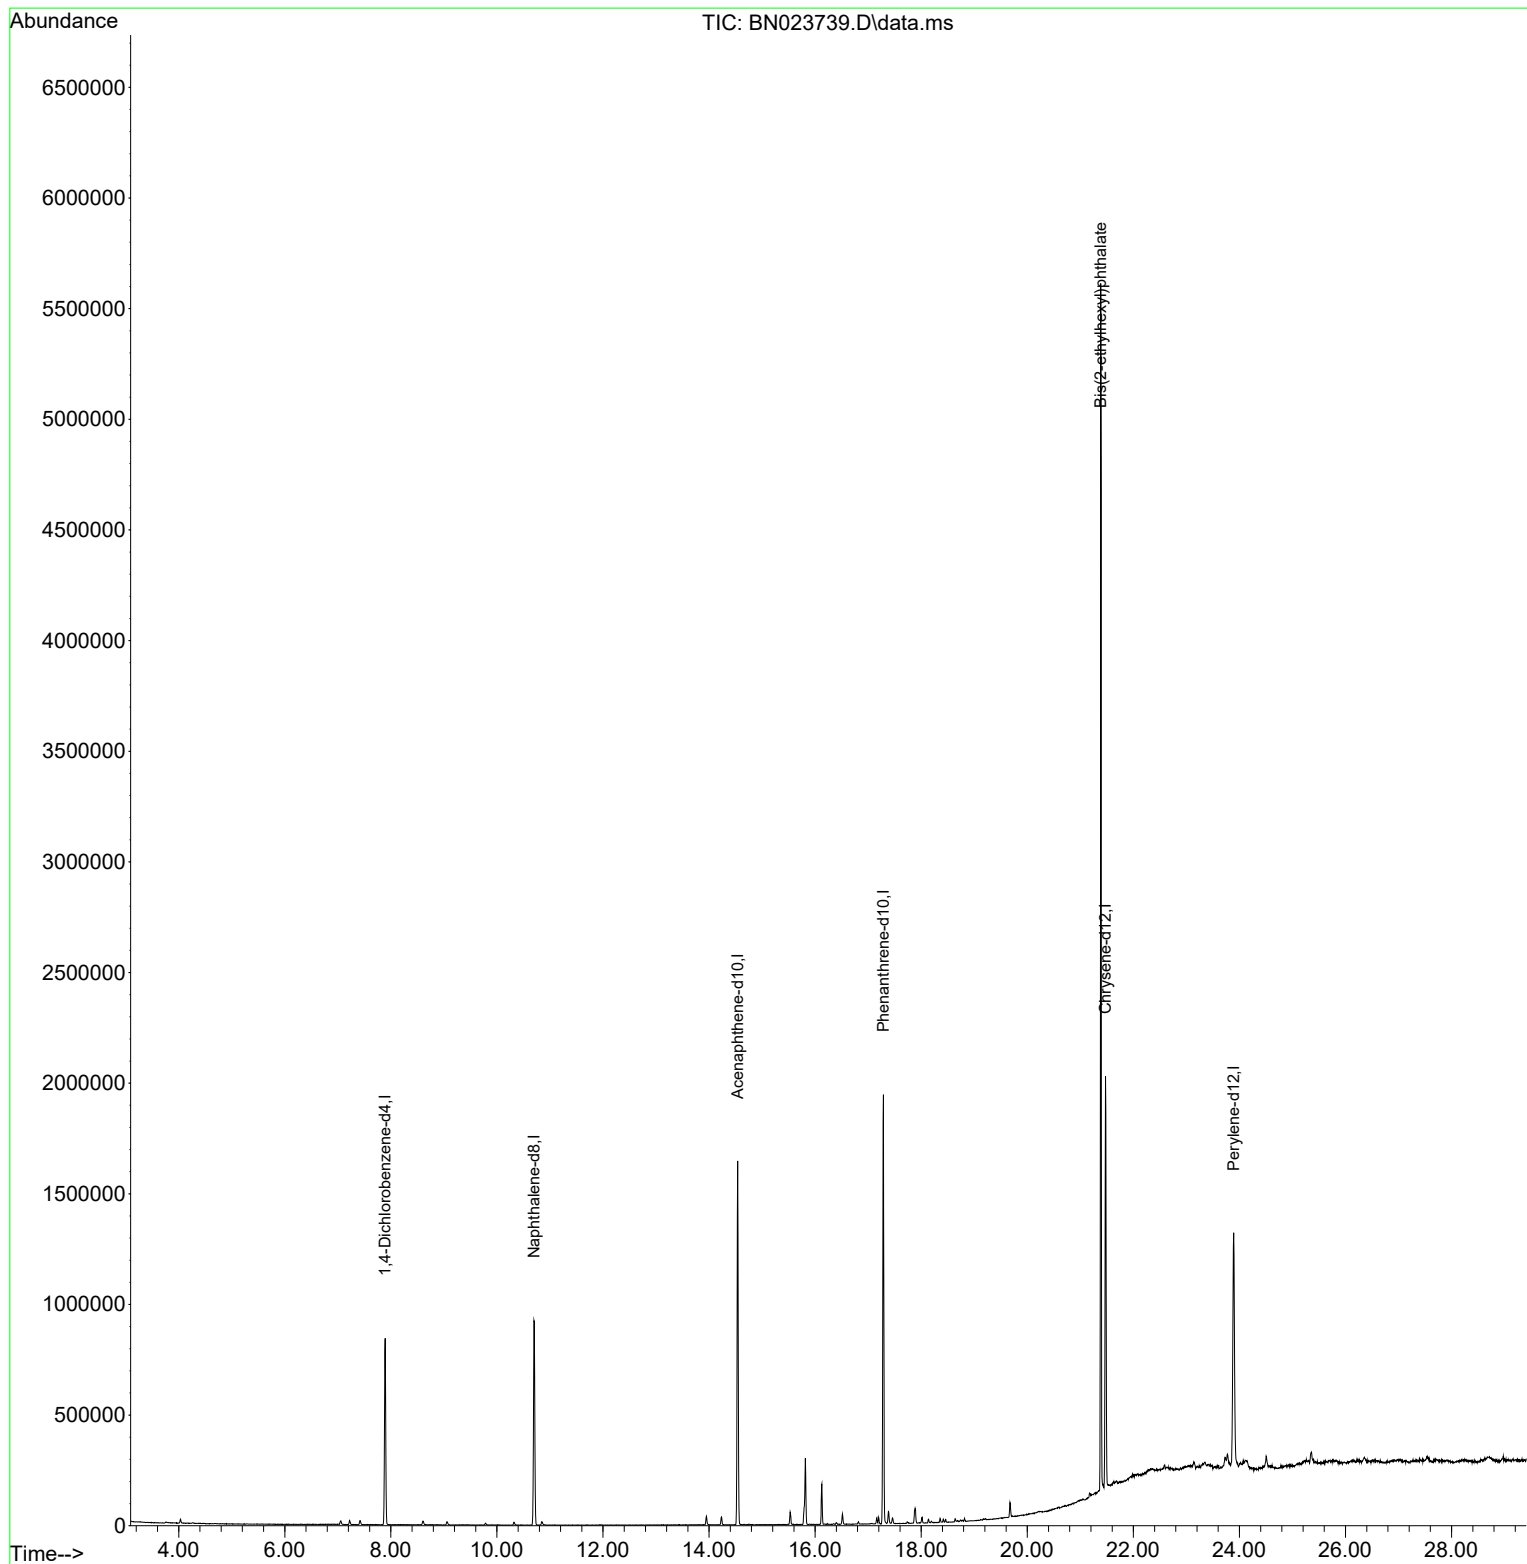

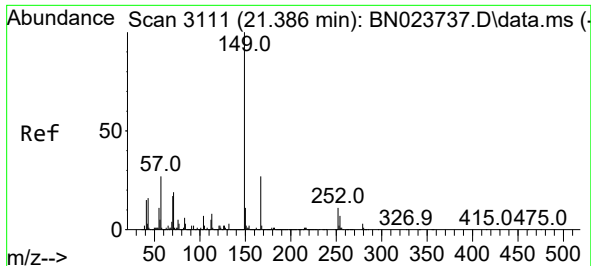

#86  
 Bis(2-ethylhexyl)phthalate  
 Concen: 48.198 ng/ul  
 RT: 21.386 min Scan# 3111  
 Delta R.T. -0.006 min  
 Lab File: BN023739.D  
 Acq: 20 Jan 2023 23:04

Instrument :  
 BNA\_N  
 ClientSampleId :  
 A43S7MEDL

Tgt Ion:149 Resp: 1692843  
 Ion Ratio Lower Upper  
 149 100  
 167 26.6 22.0 33.0  
 279 3.8 3.4 5.2

