

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023740.D
 Acq On : 20 Jan 2023 23:41
 Operator : CG/JU
 Sample : 01145-11MEDL 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A43X9MEDL

Quant Time: Jan 21 01:38:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 20 23:02:18 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	191114	20.000	ng/ul	0.00
20) Naphthalene-d8	10.699	136	769274	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.540	164	437924	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.286	188	1036488	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	952884	20.000	ng/ul	0.00
88) Perylene-d12	23.898	264	1115666	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	6852	1.543	ng/uL	0.00
4) Pyridine-d5	3.705	84	69519	5.217	ng/ul	0.00
7) Phenol-d5	7.052	99	100305	5.922	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	70252	6.761	ng/ul	0.00
11) 2-Chlorophenol-d4	7.416	132	82173	6.335	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	76323	5.645	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	35971	6.201	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	34816	5.670	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	68984	5.890	ng/ul	0.00
31) 4-Chloroaniline-d4	10.840	131	110808	6.014	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	217945	6.690	ng/ul	0.00
49) Acenaphthylene-d8	14.234	160	230194	6.377	ng/ul	0.00
54) 4-Nitrophenol-d4	14.740	143	24868	3.750	ng/ul	0.00
60) Fluorene-d10	15.528	176	214116	7.692	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.381	188	327180	7.054	ng/ul	0.00
81) Pyrene-d10	19.675	212	385718	7.078	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.739	264	388343	7.039	ng/ul	-0.02
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.392	149	2054996	53.100	ng/ul	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023740.D
Acq On : 20 Jan 2023 23:41
Operator : CG/JU
Sample : 01145-11MEDL 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A43X9MEDL

Quant Time: Jan 21 01:38:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 20 23:02:18 2023
Response via : Initial Calibration

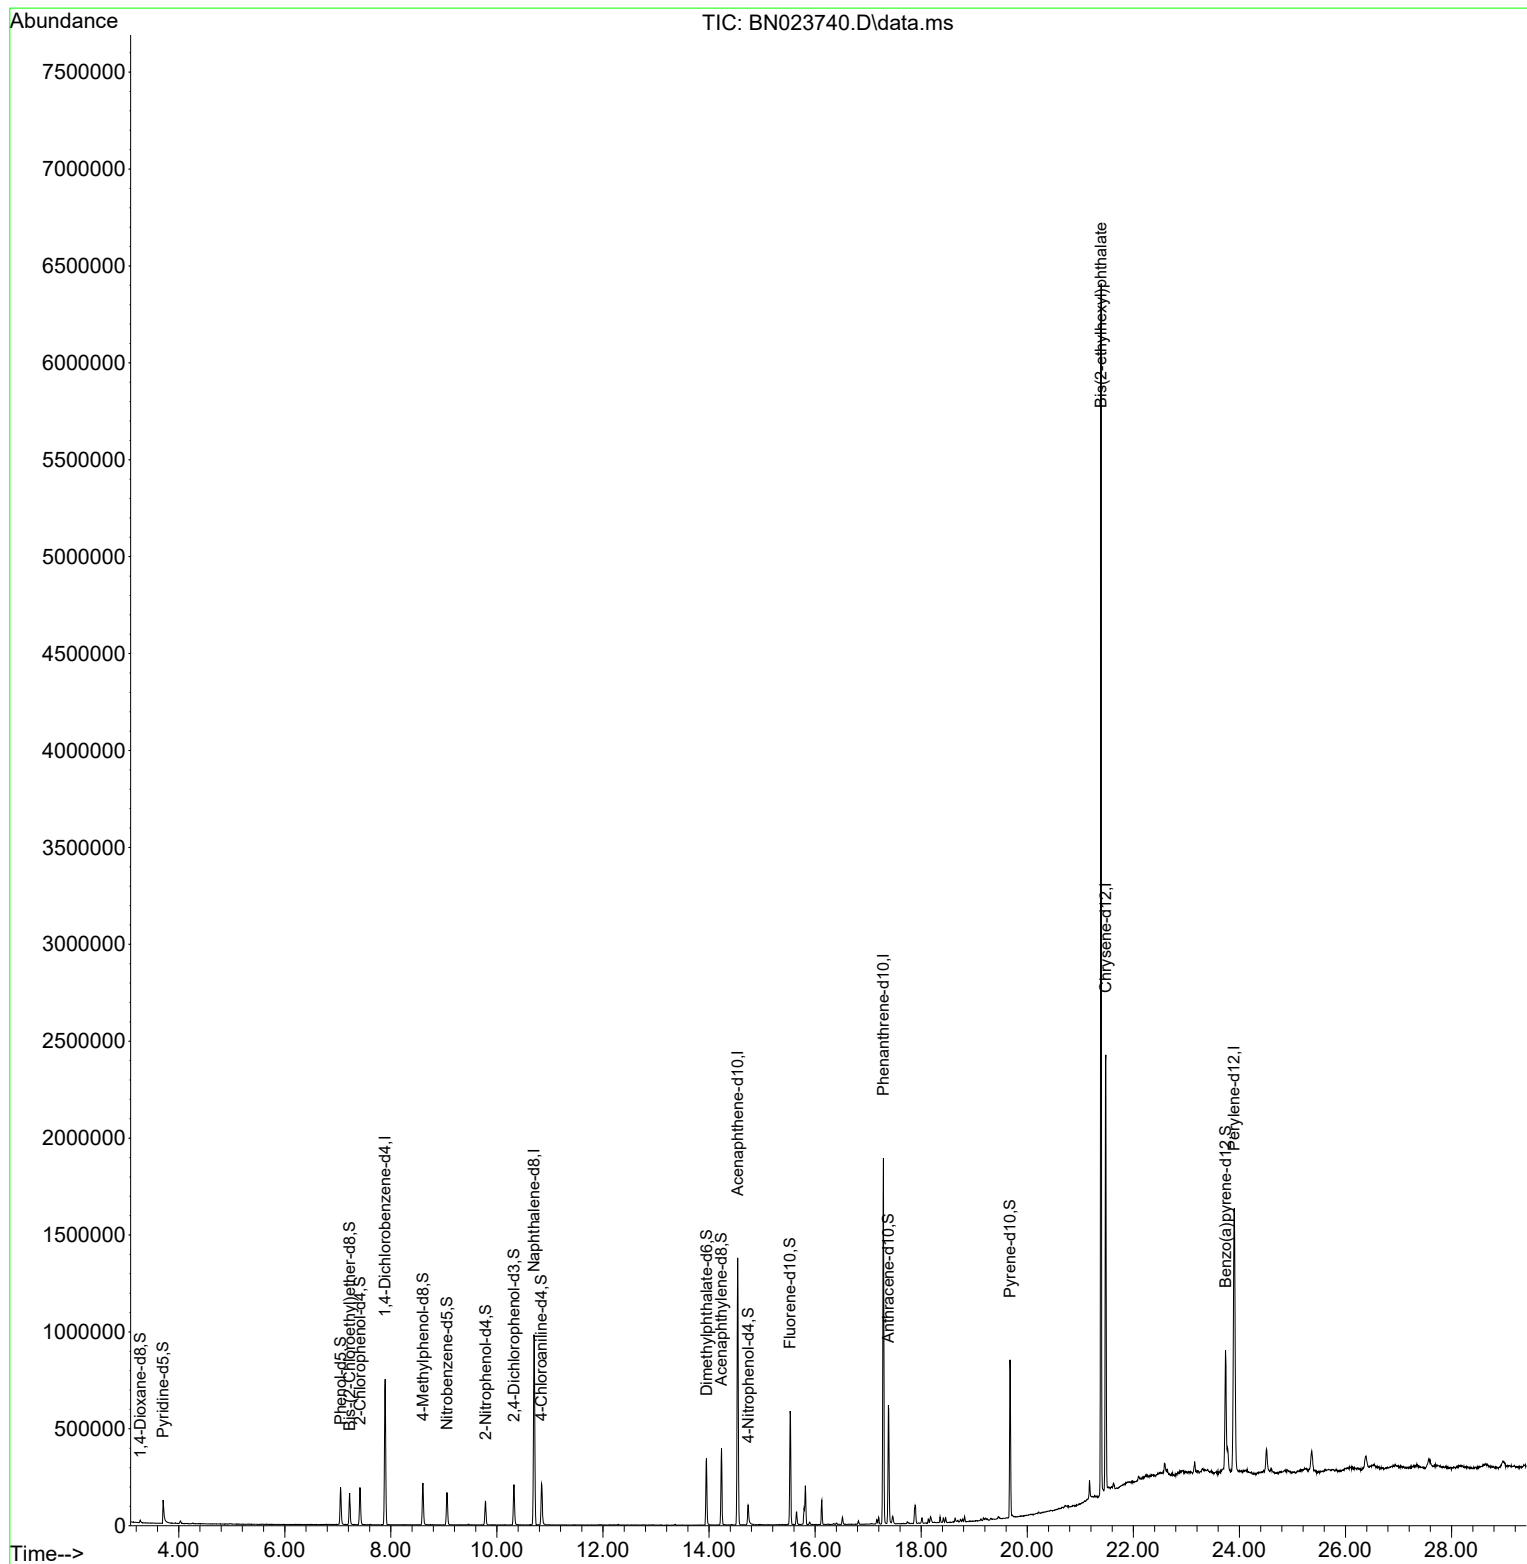

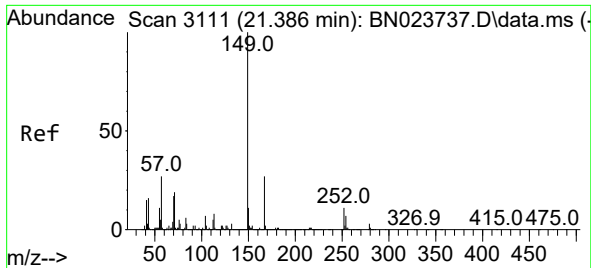

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 53.100 ng/ul
 RT: 21.392 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: BN023740.D
 Acq: 20 Jan 2023 23:41

Instrument :
 BNA_N
 ClientSampleId :
 A43X9MEDL

Tgt Ion:149 Resp: 2054996
 Ion Ratio Lower Upper
 149 100
 167 27.3 22.0 33.0
 279 4.3 3.4 5.2

