

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023742.D
 Acq On : 21 Jan 2023 00:54
 Operator : CG/JU
 Sample : 01146-08MEDL 100X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4405MEDL

Quant Time: Jan 21 01:39:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 20 23:02:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	181904	20.000	ng/ul	0.00
20) Naphthalene-d8	10.699	136	712833	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.540	164	423565	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.287	188	890009	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	924576	20.000	ng/ul	0.00
88) Perylene-d12	23.898	264	984490	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.058	99	2160	0.134	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.228	67	2191	0.222	ng/ul	0.00
11) 2-Chlorophenol-d4	7.422	132	1985	0.161	ng/ul	0.00
15) 4-Methylphenol-d8	0.000	113	0d	0.000	ng/ul	
21) Nitrobenzene-d5	9.063	128	849	0.158	ng/ul	0.00
24) 2-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
28) 2,4-Dichlorophenol-d3	0.000	165	0d	0.000	ng/ul	
31) 4-Chloroaniline-d4	0.000	131	0d	0.000	ng/ul	
46) Dimethylphthalate-d6	13.951	166	6163	0.196	ng/ul	0.00
49) Acenaphthylene-d8	14.234	160	6047	0.173	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0	0.000	ng/ul	
60) Fluorene-d10	15.534	176	5749	0.214	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0	0.000	ng/ul	
73) Anthracene-d10	17.381	188	9343	0.235	ng/ul	0.00
81) Pyrene-d10	19.675	212	9283	0.176	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.739	264	7760	0.159	ng/ul	-0.02


Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.392	149	1865869	49.689 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023742.D
Acq On : 21 Jan 2023 00:54
Operator : CG/JU
Sample : 01146-08MEDL 100X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4405MEDL

Quant Time: Jan 21 01:39:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 20 23:02:18 2023
Response via : Initial Calibration

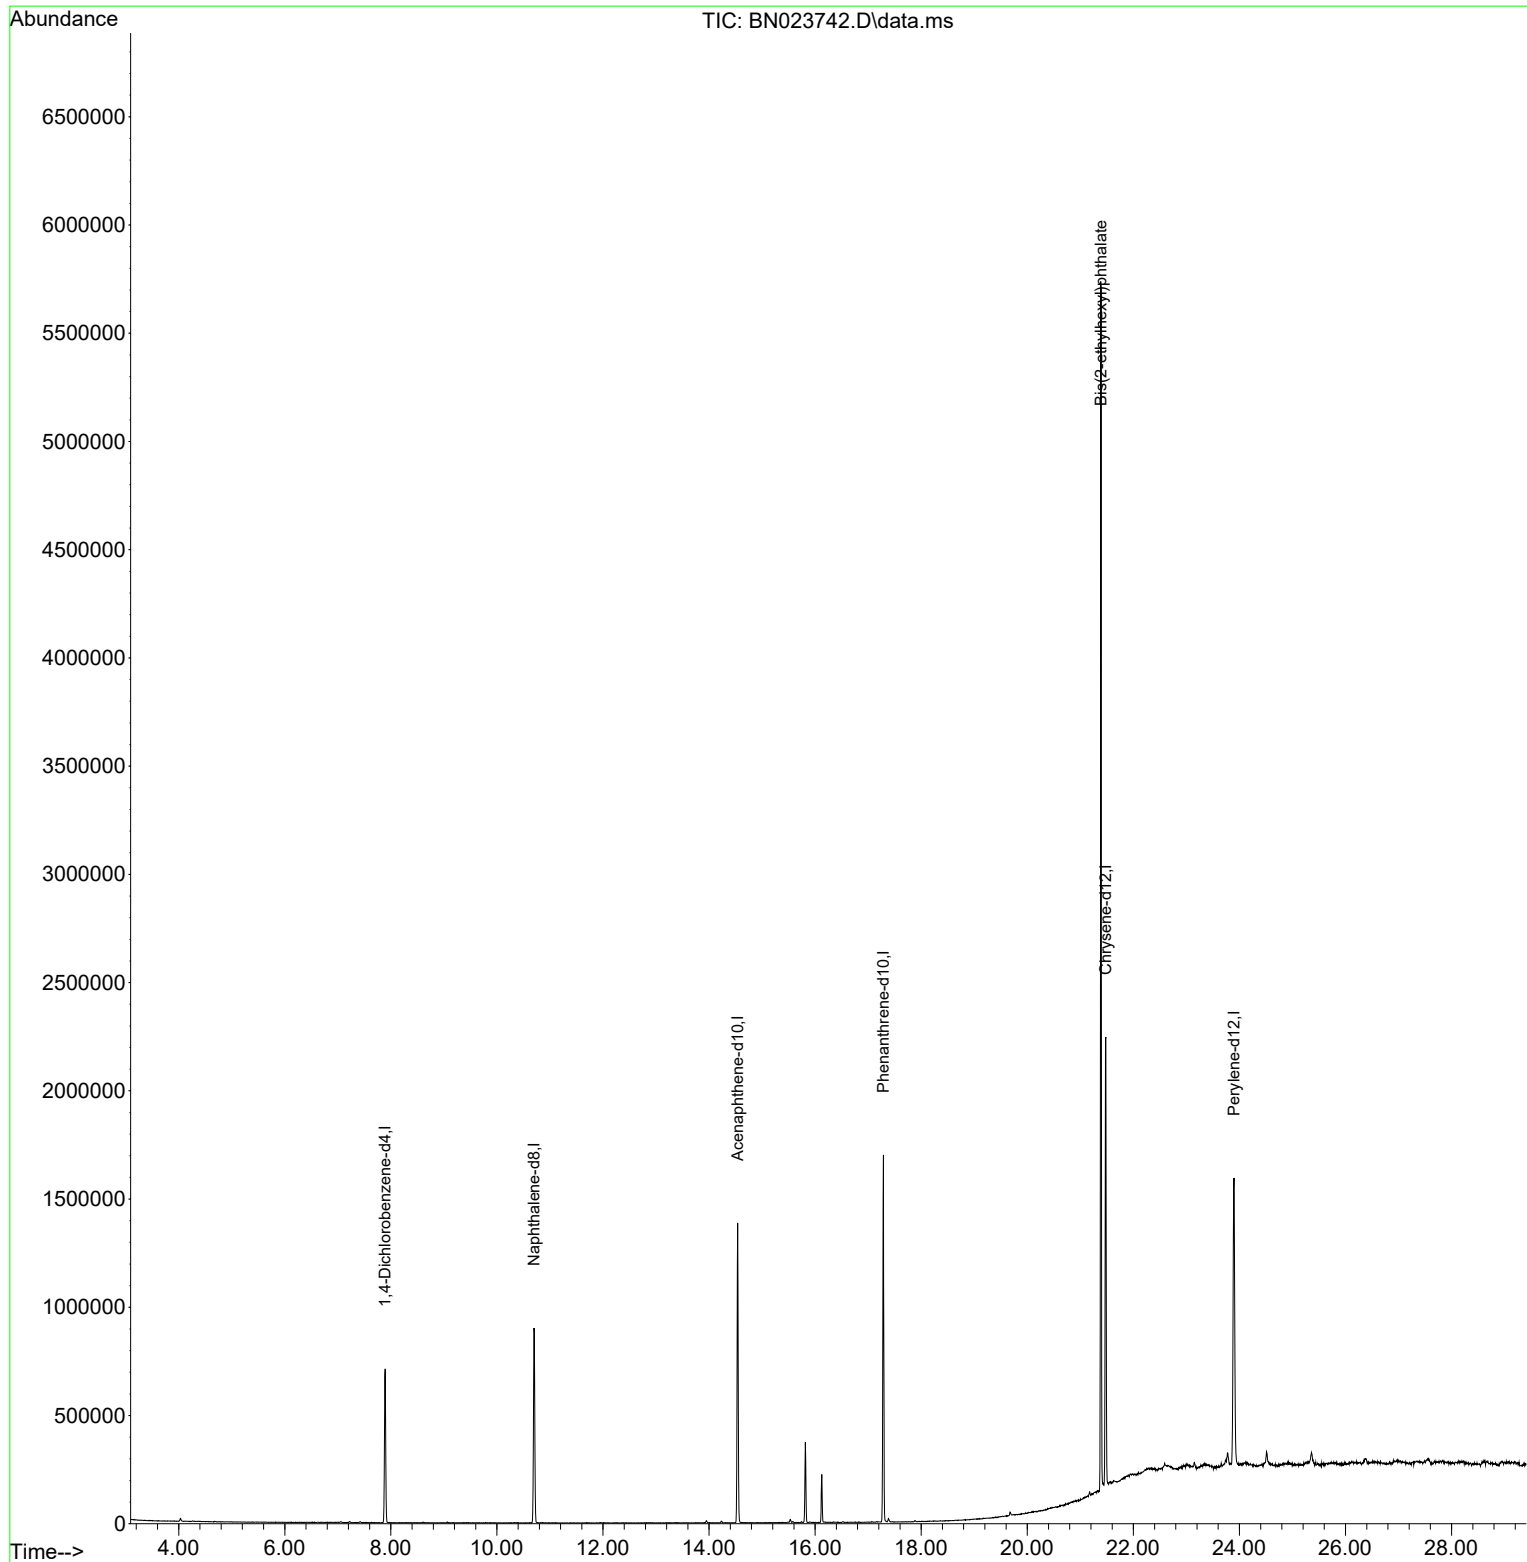

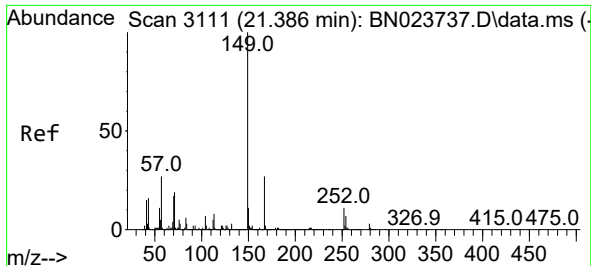

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 49.689 ng/ul
 RT: 21.392 min Scan# 3112
 Delta R.T. 0.000 min
 Lab File: BN023742.D
 Acq: 21 Jan 2023 00:54

Instrument :
 BNA_N
 ClientSampleId :
 A4405MEDL

Tgt Ion:149 Resp: 1865869

Ion	Ratio	Lower	Upper
149	100		
167	28.1	22.0	33.0
279	4.4	3.4	5.2

