

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023744.D
 Acq On : 21 Jan 2023 02:08
 Operator : CG/JU
 Sample : 01146-11MEDL 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4412MEDL

Quant Time: Jan 21 02:55:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 20 23:02:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.893	152	209030	20.000	ng/ul	0.00
20) Naphthalene-d8	10.699	136	927100	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.540	164	494424	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.287	188	1107081	20.000	ng/ul	0.00
79) Chrysene-d12	21.475	240	1024840	20.000	ng/ul	-0.01
88) Perylene-d12	23.898	264	1033269	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.276	96	5228	1.076	ng/uL	0.00
4) Pyridine-d5	3.705	84	50665	3.476	ng/ul	0.00
7) Phenol-d5	7.052	99	75347	4.067	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.222	67	53361	4.695	ng/ul	0.00
11) 2-Chlorophenol-d4	7.417	132	64460	4.543	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	56664	3.832	ng/ul	0.00
21) Nitrobenzene-d5	9.058	128	29092	4.161	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	27453	3.710	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.322	165	53420	3.784	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131	86717	3.905	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	173134	4.707	ng/ul	0.00
49) Acenaphthylene-d8	14.234	160	172387	4.230	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	0.00
60) Fluorene-d10	15.528	176	149917	4.770	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	0.00
73) Anthracene-d10	17.381	188	225628	4.554	ng/ul	0.00
81) Pyrene-d10	19.675	212	276224	4.713	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.733	264	209519	4.100	ng/ul	-0.02
Target Compounds						Qvalue
86) Bis(2-ethylhexyl)phtha...	21.386	149	1927557	46.310	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023744.D
Acq On : 21 Jan 2023 02:08
Operator : CG/JU
Sample : 01146-11MEDL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4412MEDL

Quant Time: Jan 21 02:55:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 20 23:02:18 2023
Response via : Initial Calibration

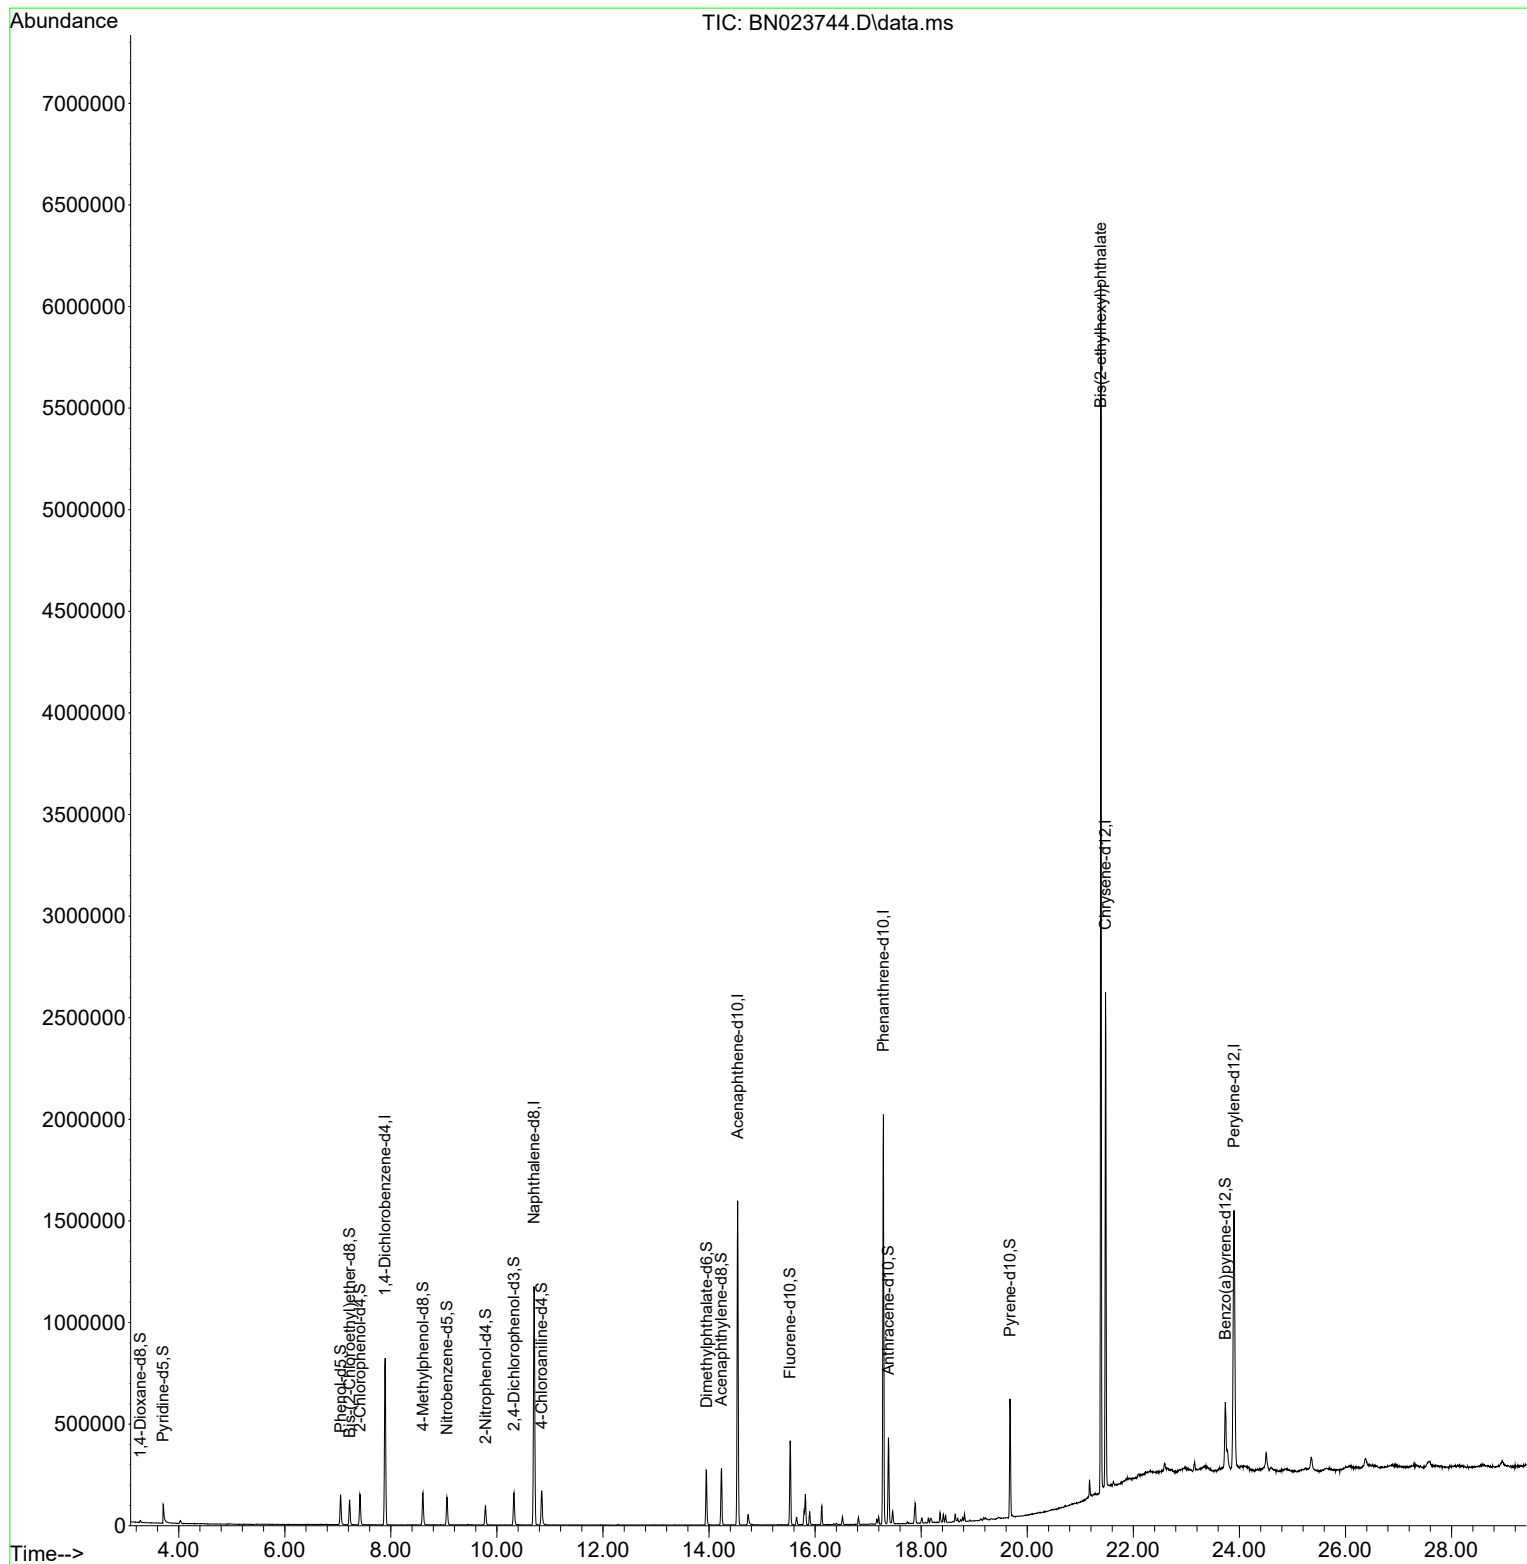

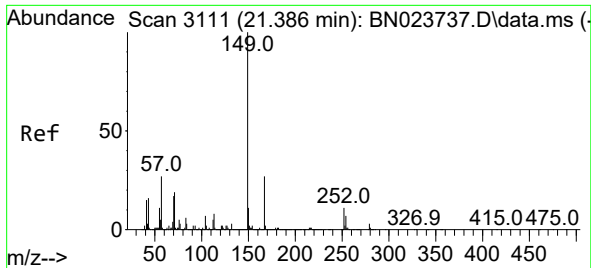

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 46.310 ng/ul
 RT: 21.386 min Scan# 3111
 Delta R.T. -0.006 min
 Lab File: BN023744.D
 Acq: 21 Jan 2023 02:08

Instrument :
 BNA_N
 ClientSampleId :
 A4412MEDL

Tgt Ion:149 Resp: 1927557
 Ion Ratio Lower Upper
 149 100
 167 27.2 22.0 33.0
 279 3.9 3.4 5.2

