

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023738.D
 Acq On : 20 Jan 2023 22:27
 Operator : CG/JU
 Sample : PB150349BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK349

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023738.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	39	rBV	62672	83529	1.95%	0.183%
2	3.699	101	104	126	rBV	776575	1127578	26.38%	2.476%
3	4.034	157	161	166	rVB	14393	20099	0.47%	0.044%
4	7.052	667	674	687	rBV	902520	1410155	32.99%	3.097%
5	7.222	697	703	716	rVB	749182	1135306	26.56%	2.493%
6	7.422	729	737	751	rBV	929097	1468662	34.36%	3.225%
7	7.893	810	817	825	rBV	691382	1067739	24.98%	2.345%
8	8.604	931	938	952	rBV	997888	1539690	36.02%	3.381%
9	9.057	1008	1015	1026	rBV	740955	1195165	27.96%	2.625%
10	9.787	1130	1139	1151	rBV	615804	987069	23.09%	2.168%
11	10.322	1222	1230	1244	rBV	913416	1486253	34.77%	3.264%
12	10.704	1287	1295	1302	rBV	787707	1294377	30.28%	2.842%
13	10.846	1312	1319	1334	rBV	911293	1549901	36.26%	3.404%
14	12.292	1560	1565	1572	rBV2	14881	23549	0.55%	0.052%
15	13.951	1841	1847	1856	rBV	1822580	2413928	56.47%	5.301%
16	14.234	1888	1895	1908	rBV	2007352	2850193	66.68%	6.259%
17	14.539	1940	1947	1956	rVB	1326372	1884689	44.09%	4.139%
18	14.734	1974	1980	1999	rBV	812944	1178728	27.58%	2.589%
19	15.533	2109	2116	2124	rBV	2466109	3492957	81.71%	7.671%
20	15.651	2129	2136	2149	rBV	648982	864953	20.23%	1.899%
21	15.769	2152	2156	2161	rVB2	11859	17022	0.40%	0.037%
22	17.286	2407	2414	2424	rBV	1526656	2175788	50.90%	4.778%
23	17.386	2424	2431	2445	rBV	2620727	3743795	87.58%	8.221%
24	17.663	2475	2478	2483	rVB5	3007	5237	0.12%	0.012%
25	19.239	2742	2746	2752	rBV2	30711	38968	0.91%	0.086%
26	19.310	2754	2758	2763	rBV	29728	38966	0.91%	0.086%
27	19.680	2815	2821	2826	rBV	3175560	4274606	100.00%	9.387%
28	21.480	3121	3127	3135	rBV	1830924	2332158	54.56%	5.121%
29	23.733	3503	3510	3526	rVB2	1876860	3849283	90.05%	8.453%
30	23.898	3532	3538	3548	rVB2	1063094	1986522	46.47%	4.362%




Sum of corrected areas: 45536865

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023738.D
Acq On : 20 Jan 2023 22:27
Operator : CG/JU
Sample : PB150349BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK349

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

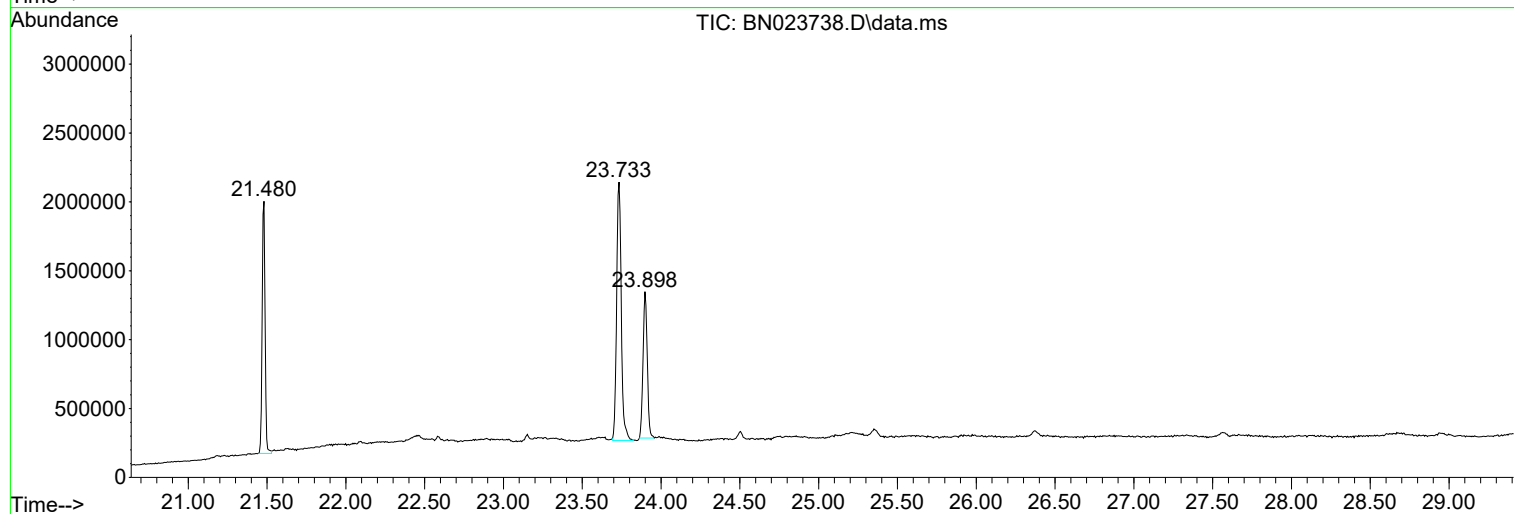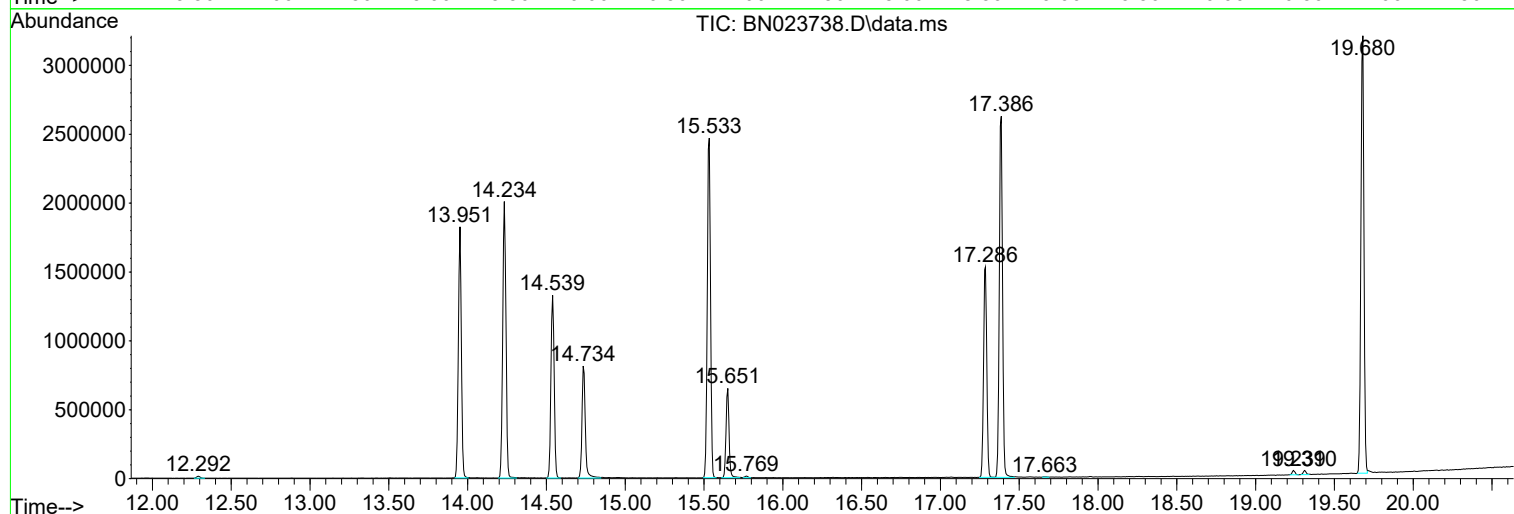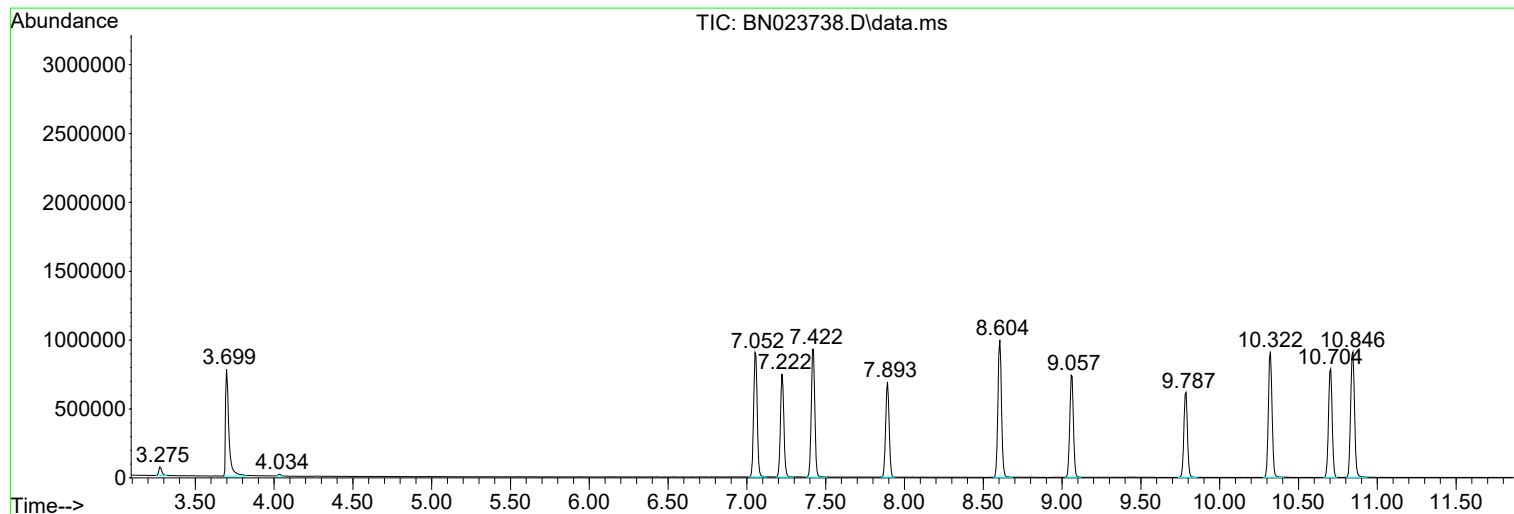

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023738.D
Acq On : 20 Jan 2023 22:27
Operator : CG/JU
Sample : PB150349BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK349

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023738.D
Acq On : 20 Jan 2023 22:27
Operator : CG/JU
Sample : PB150349BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK349

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc