

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023741.D
 Acq On : 21 Jan 2023 00:18
 Operator : CG/JU
 Sample : 01146-02MEDL 30X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A43Y5MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023741.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.034	156	161	166	rVB	15836	24110	0.84%	0.149%
2	4.264	196	200	206	rBV5	8678	12806	0.44%	0.079%
3	4.681	267	271	275	rVB2	4990	6747	0.23%	0.042%
4	7.011	661	667	668	rBV4	1794	3247	0.11%	0.020%
5	7.052	668	674	681	rVV	18838	31424	1.09%	0.194%
6	7.222	696	703	710	rVB	19903	33664	1.17%	0.208%
7	7.422	730	737	742	rBV	20900	34146	1.19%	0.211%
8	7.893	810	817	829	rVB	799950	1252073	43.48%	7.747%
9	8.605	934	938	945	rVB2	18659	31374	1.09%	0.194%
10	9.058	1009	1015	1021	rBV	17387	29204	1.01%	0.181%
11	9.787	1133	1139	1146	rVB2	10397	18735	0.65%	0.116%
12	10.322	1224	1230	1238	rBV2	16114	29631	1.03%	0.183%
13	10.705	1287	1295	1305	rBV	1003910	1685284	58.52%	10.428%
14	10.852	1313	1320	1326	rBV2	13682	24397	0.85%	0.151%
15	13.951	1841	1847	1853	rBV	39878	58031	2.02%	0.359%
16	14.234	1889	1895	1900	rBV	35967	53549	1.86%	0.331%
17	14.540	1940	1947	1956	rBV	1502275	2098318	72.87%	12.983%
18	14.757	1978	1984	1990	rBV7	2859	6528	0.23%	0.040%
19	15.528	2110	2115	2122	rVB	62711	89639	3.11%	0.555%
20	15.651	2132	2136	2138	rBV4	2843	3268	0.11%	0.020%
21	15.816	2155	2164	2170	rBV2	100109	176402	6.13%	1.091%
22	15.898	2174	2178	2182	rVV	8915	13045	0.45%	0.081%
23	16.122	2212	2216	2221	rVB	60776	79532	2.76%	0.492%
24	16.398	2261	2263	2267	rBV4	3623	3851	0.13%	0.024%
25	16.516	2278	2283	2289	rVB	19908	25605	0.89%	0.158%
26	16.816	2330	2334	2338	rVB5	6167	8077	0.28%	0.050%
27	17.069	2374	2377	2381	rVB4	3297	4127	0.14%	0.026%
28	17.163	2388	2393	2396	rBV3	7775	10691	0.37%	0.066%
29	17.198	2396	2399	2404	rVB3	14187	16671	0.58%	0.103%
30	17.287	2407	2414	2425	rVV	1806627	2496645	86.70%	15.448%
31	17.381	2425	2430	2438	rVV2	57659	90570	3.15%	0.560%
32	17.463	2440	2444	2448	rVB3	11808	18166	0.63%	0.112%
33	17.740	2488	2491	2495	rBV5	2886	4753	0.17%	0.029%
34	17.887	2510	2516	2522	rVB2	31720	58749	2.04%	0.364%
35	18.016	2532	2538	2543	rBV4	9025	14627	0.51%	0.091%
36	18.139	2556	2559	2562	rBV2	6843	7211	0.25%	0.045%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023741.D
 Acq On : 21 Jan 2023 00:18
 Operator : CG/JU
 Sample : 01146-02MEDL 30X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A43Y5MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

37	18.187	2564	2567	2569	rVV4	3307	3159	0.11%	0.020%
38	18.357	2593	2596	2599	rVB5	6897	6910	0.24%	0.043%
39	18.416	2603	2606	2609	rVV3	6910	7495	0.26%	0.046%
40	18.457	2611	2613	2618	rVB5	6841	8402	0.29%	0.052%
41	18.639	2642	2644	2647	rBV3	5594	5815	0.20%	0.036%
42	18.739	2659	2661	2665	rBV4	3137	5169	0.18%	0.032%
43	18.816	2671	2674	2679	rVB6	6595	9168	0.32%	0.057%
44	19.675	2816	2820	2827	rBV	74438	109368	3.80%	0.677%
45	21.380	3105	3110	3116	rBV	2706330	2879655	100.00%	17.818%
46	21.469	3120	3125	3131	rBV	1855623	2342510	81.35%	14.494%
47	23.886	3529	3536	3547	rVB	1038589	2229223	77.41%	13.793%




Sum of corrected areas: 16161771

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023741.D
Acq On : 21 Jan 2023 00:18
Operator : CG/JU
Sample : 01146-02MEDL 30X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A43Y5MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

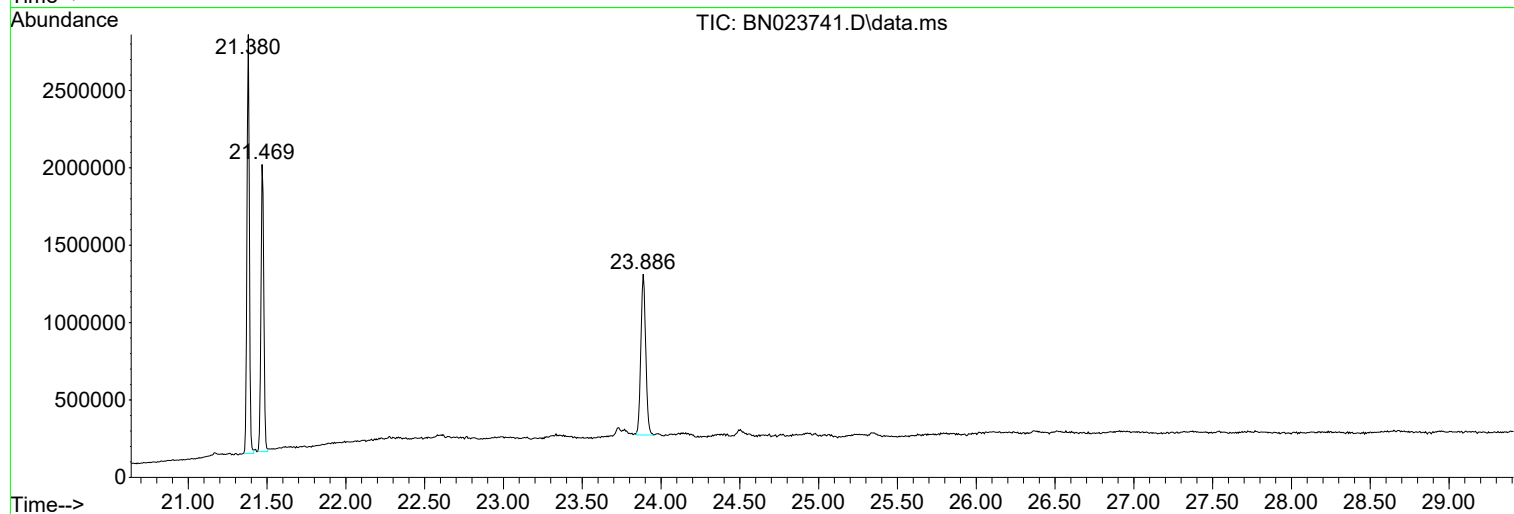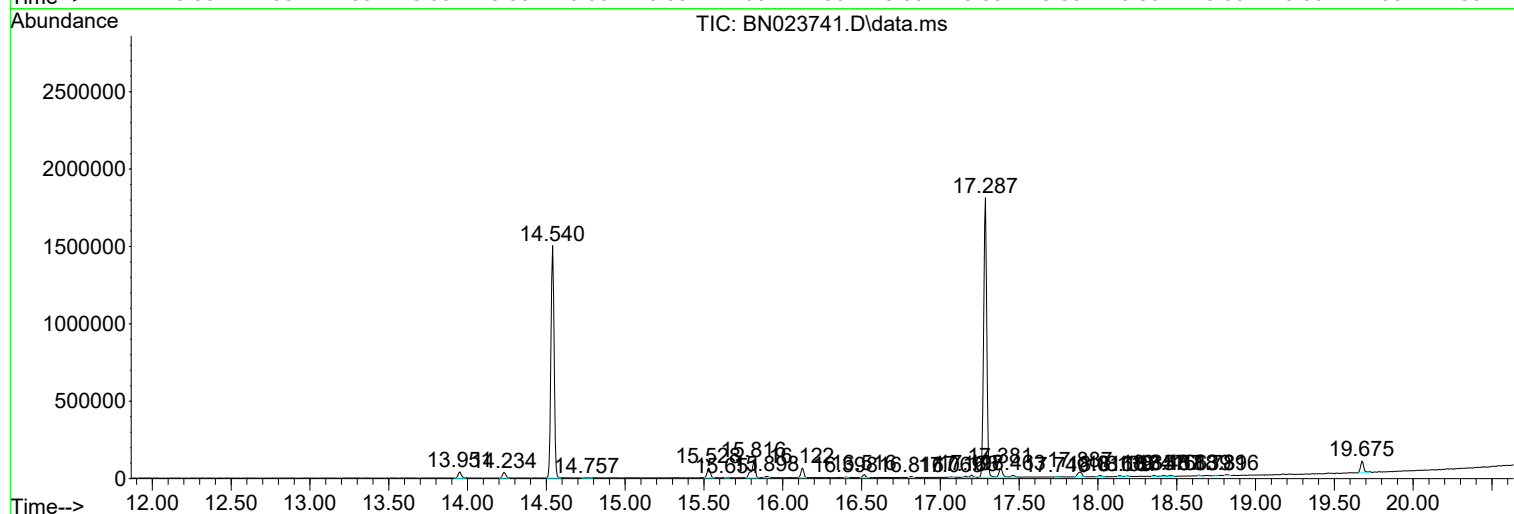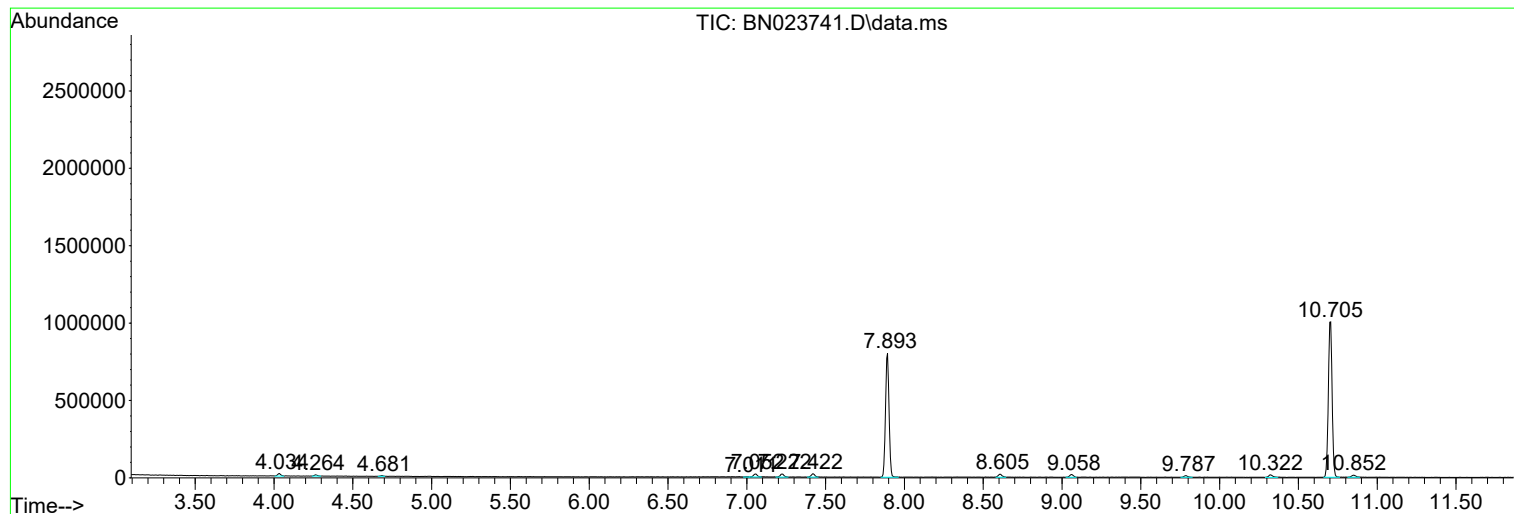

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023741.D
Acq On : 21 Jan 2023 00:18
Operator : CG/JU
Sample : 01146-02MEDL 30X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A43Y5MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023741.D
Acq On : 21 Jan 2023 00:18
Operator : CG/JU
Sample : 01146-02MEDL 30X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A43Y5MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc