

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023743.D
 Acq On : 21 Jan 2023 01:31
 Operator : CG/JU
 Sample : 01146-10MEDL 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4411MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023743.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	29	32	38	rVB2	10432	12279	0.22%	0.047%
2	3.705	103	105	122	rBV	76560	137773	2.46%	0.527%
3	4.028	156	160	166	rBV	14705	20600	0.37%	0.079%
4	7.051	667	674	682	rBV	140647	210675	3.76%	0.805%
5	7.222	696	703	711	rBV	121774	188004	3.36%	0.719%
6	7.416	730	736	743	rBV	138299	217264	3.88%	0.830%
7	7.893	809	817	825	rBV	775827	1214502	21.68%	4.642%
8	8.604	932	938	951	rBV	155796	256097	4.57%	0.979%
9	9.057	1007	1015	1024	rBV	123870	203631	3.64%	0.778%
10	9.781	1133	1138	1150	rVB	84337	143401	2.56%	0.548%
11	10.322	1224	1230	1238	rBV	147043	237507	4.24%	0.908%
12	10.704	1287	1295	1303	rBV	1018377	1709166	30.51%	6.533%
13	10.845	1313	1319	1327	rBV	157109	270708	4.83%	1.035%
14	13.951	1840	1847	1861	rBV	284814	401290	7.16%	1.534%
15	14.233	1888	1895	1904	rBV	293043	416356	7.43%	1.591%
16	14.539	1939	1947	1957	rBV	1569502	2235656	39.91%	8.545%
17	14.739	1975	1981	1993	rBV	58785	111976	2.00%	0.428%
18	15.527	2109	2115	2122	rVB	444781	609317	10.88%	2.329%
19	15.645	2131	2135	2142	rBV	38583	58102	1.04%	0.222%
20	15.816	2155	2164	2171	rVB2	108875	202412	3.61%	0.774%
21	15.898	2171	2178	2186	rBV	70927	96224	1.72%	0.368%
22	16.127	2212	2217	2221	rBV	68207	87238	1.56%	0.333%
23	16.398	2260	2263	2269	rBV5	4342	5777	0.10%	0.022%
24	16.516	2278	2283	2287	rBV	29739	39239	0.70%	0.150%
25	16.816	2330	2334	2340	rVB2	22835	29830	0.53%	0.114%
26	17.163	2388	2393	2396	rBV2	18737	24150	0.43%	0.092%
27	17.198	2396	2399	2404	rVB2	24853	31241	0.56%	0.119%
28	17.286	2407	2414	2424	rBV	1805574	2492056	44.49%	9.525%
29	17.380	2424	2430	2439	rVV	431991	608803	10.87%	2.327%
30	17.463	2439	2444	2450	rVB	46659	71855	1.28%	0.275%
31	17.739	2485	2491	2494	rBV5	7125	10694	0.19%	0.041%
32	17.886	2509	2516	2522	rBV2	70359	128820	2.30%	0.492%
33	18.010	2533	2537	2545	rVB4	17381	27608	0.49%	0.106%
34	18.133	2555	2558	2562	rBV3	15802	21212	0.38%	0.081%
35	18.174	2562	2565	2571	rVV4	19479	34982	0.62%	0.134%
36	18.357	2591	2596	2600	rBV	33972	42192	0.75%	0.161%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023743.D
 Acq On : 21 Jan 2023 01:31
 Operator : CG/JU
 Sample : 01146-10MEDL 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4411MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

37	18.416	2602	2606	2610	rVV2	27106	32462	0.58%	0.124%
38	18.457	2610	2613	2618	rVB3	22889	29906	0.53%	0.114%
39	18.639	2640	2644	2648	rVV2	26651	33852	0.60%	0.129%
40	18.686	2649	2652	2657	rVB6	12111	14669	0.26%	0.056%
41	18.745	2658	2662	2665	rVV3	7060	9075	0.16%	0.035%
42	18.780	2665	2668	2671	rVV2	13822	16501	0.29%	0.063%
43	18.816	2671	2674	2678	rVB3	27080	30999	0.55%	0.118%
44	19.127	2725	2727	2730	rVB3	7932	6744	0.12%	0.026%
45	19.210	2738	2741	2744	rBV4	6212	9292	0.17%	0.036%
46	19.674	2815	2820	2826	rBV	578272	758516	13.54%	2.899%
47	21.180	3072	3076	3081	rBV2	85680	108509	1.94%	0.415%
48	21.386	3107	3111	3118	rBV	5155419	5601827	100.00%	21.411%
49	21.480	3121	3127	3134	rVV	2446568	3089237	55.15%	11.807%
50	23.739	3506	3511	3516	rBV	386277	672127	12.00%	2.569%
51	23.898	3530	3538	3553	rVB2	1464403	3141257	56.08%	12.006%




Sum of corrected areas: 26163610

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023743.D
Acq On : 21 Jan 2023 01:31
Operator : CG/JU
Sample : 01146-10MEDL 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4411MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

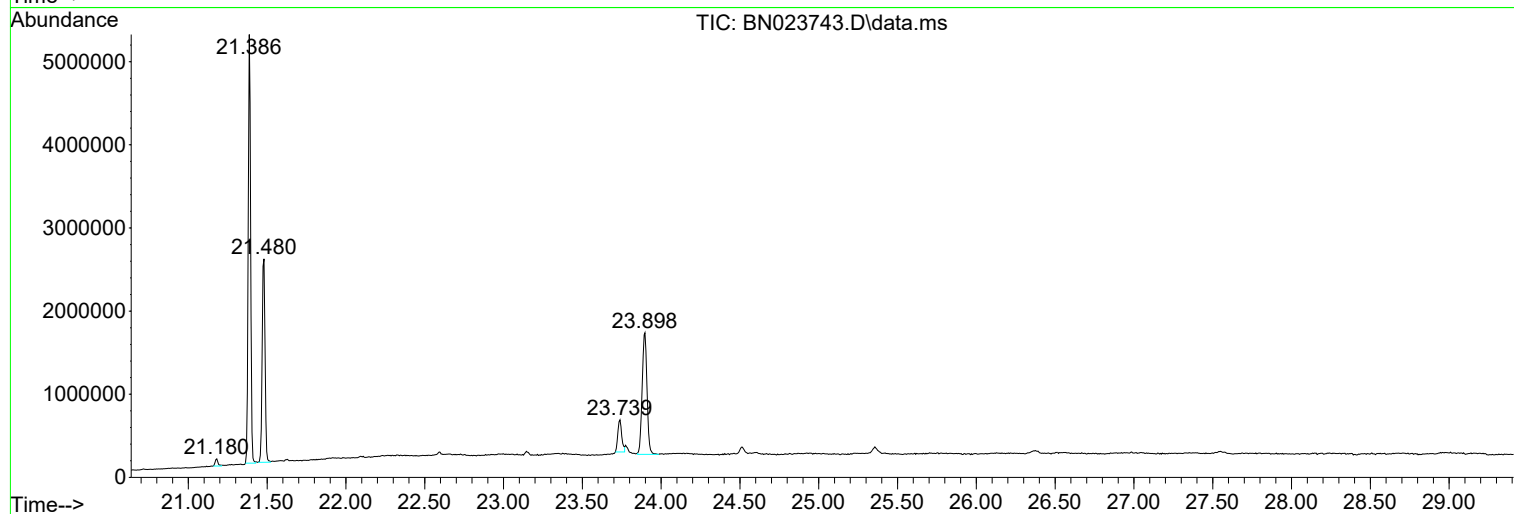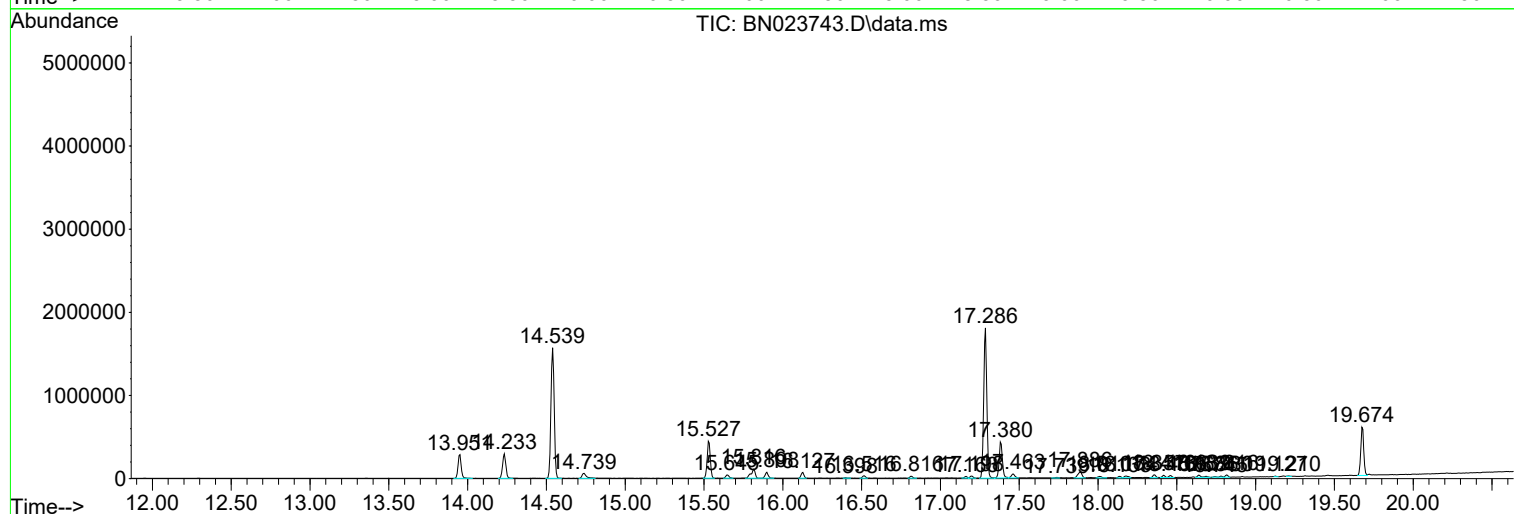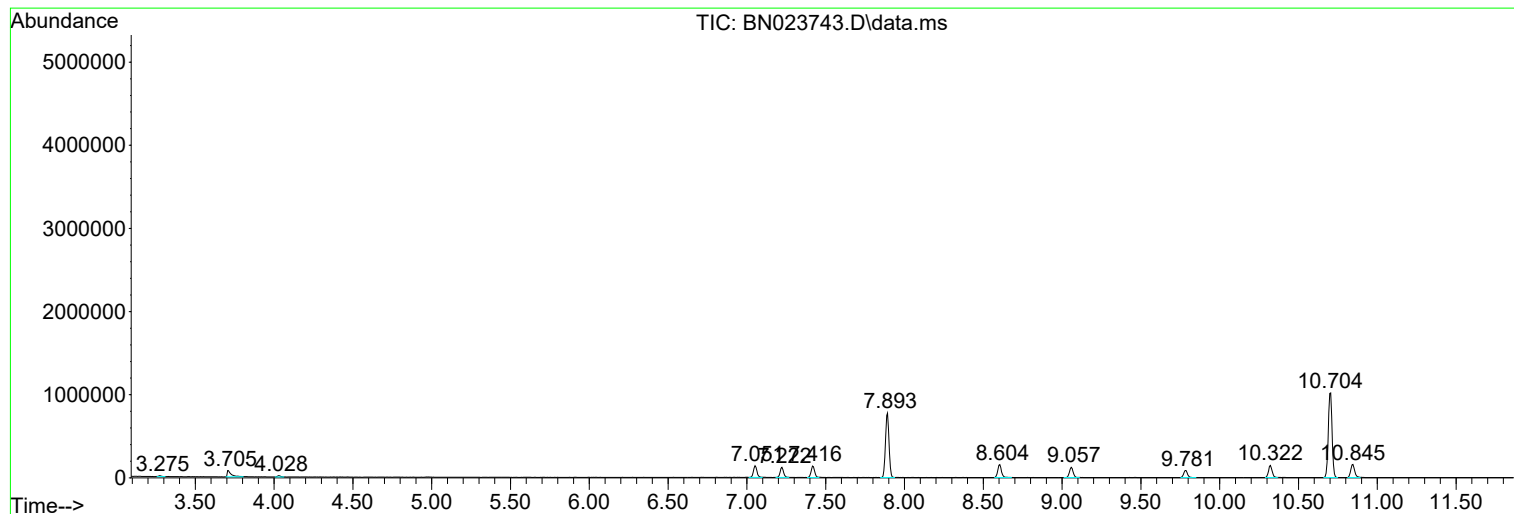

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023743.D
Acq On : 21 Jan 2023 01:31
Operator : CG/JU
Sample : 01146-10MEDL 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4411MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023743.D
Acq On : 21 Jan 2023 01:31
Operator : CG/JU
Sample : 01146-10MEDL 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4411MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------