

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023744.D
 Acq On : 21 Jan 2023 02:08
 Operator : CG/JU
 Sample : 01146-11MEDL 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4412MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023744.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	29	32	37	rVB	10004	13448	0.20%	0.048%
2	3.705	104	105	126	rBV	92156	155312	2.32%	0.560%
3	4.034	156	161	168	rVB	15683	23451	0.35%	0.085%
4	7.052	666	674	686	rBV	146965	222698	3.33%	0.803%
5	7.222	697	703	715	rVB	122742	189968	2.84%	0.685%
6	7.417	730	736	748	rBV	150954	237732	3.56%	0.857%
7	7.893	810	817	826	rVB	819767	1273147	19.04%	4.589%
8	8.605	930	938	947	rBV	158455	254081	3.80%	0.916%
9	9.058	1007	1015	1024	rBV	136844	223621	3.34%	0.806%
10	9.781	1131	1138	1146	rBV	94142	159715	2.39%	0.576%
11	10.322	1221	1230	1243	rBV	159022	269359	4.03%	0.971%
12	10.699	1287	1294	1303	rBV	1172601	1942204	29.05%	7.000%
13	10.846	1312	1319	1329	rBV	166946	292184	4.37%	1.053%
14	13.946	1840	1846	1858	rBV	270645	384367	5.75%	1.385%
15	14.234	1888	1895	1904	rBV	279613	407224	6.09%	1.468%
16	14.540	1940	1947	1954	rBV	1595634	2264543	33.87%	8.162%
17	14.734	1975	1980	1992	rBV2	51751	104499	1.56%	0.377%
18	15.528	2110	2115	2124	rVB	413262	578041	8.65%	2.083%
19	15.651	2129	2136	2144	rBV	36387	55964	0.84%	0.202%
20	15.793	2155	2160	2161	rBV	66743	76811	1.15%	0.277%
21	15.816	2161	2164	2170	rVB	150451	190818	2.85%	0.688%
22	15.898	2172	2178	2183	rBV	65861	89121	1.33%	0.321%
23	16.128	2211	2217	2221	rBV	92551	119602	1.79%	0.431%
24	16.351	2250	2255	2259	rBV7	4799	6699	0.10%	0.024%
25	16.398	2259	2263	2266	rBV3	6023	7056	0.11%	0.025%
26	16.516	2277	2283	2290	rBV	40545	54788	0.82%	0.197%
27	16.816	2329	2334	2339	rBV	35464	42468	0.64%	0.153%
28	17.163	2387	2393	2396	rBV	24264	33510	0.50%	0.121%
29	17.198	2396	2399	2403	rVB	36753	44273	0.66%	0.160%
30	17.287	2407	2414	2425	rVV	2015679	2794441	41.80%	10.072%
31	17.381	2425	2430	2438	rVV2	424496	606991	9.08%	2.188%
32	17.463	2439	2444	2451	rVB2	63132	94304	1.41%	0.340%
33	17.740	2487	2491	2493	rBV4	10816	13106	0.20%	0.047%
34	17.887	2509	2516	2523	rBV	100437	178766	2.67%	0.644%
35	18.016	2532	2538	2542	rBV3	25710	43066	0.64%	0.155%
36	18.134	2555	2558	2562	rBV	25607	32463	0.49%	0.117%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
 Data File : BN023744.D
 Acq On : 21 Jan 2023 02:08
 Operator : CG/JU
 Sample : 01146-11MEDL 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4412MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

37	18.181	2562	2566	2571	rVV5	21464	41228	0.62%	0.149%
38	18.357	2592	2596	2601	rBV	48522	64033	0.96%	0.231%
39	18.416	2602	2606	2610	rVV2	40447	49350	0.74%	0.178%
40	18.457	2610	2613	2619	rVB2	36273	45606	0.68%	0.164%
41	18.639	2640	2644	2649	rBV	36946	50168	0.75%	0.181%
42	18.687	2649	2652	2656	rVB5	17757	21437	0.32%	0.077%
43	18.739	2658	2661	2664	rBV2	11433	13793	0.21%	0.050%
44	18.781	2665	2668	2671	rVV3	20737	24340	0.36%	0.088%
45	18.816	2671	2674	2678	rVB3	37842	43609	0.65%	0.157%
46	19.122	2724	2726	2731	rVB4	8301	9847	0.15%	0.035%
47	19.175	2733	2735	2738	rVV2	9146	8187	0.12%	0.030%
48	19.210	2738	2741	2744	rVB3	8995	11667	0.17%	0.042%
49	19.675	2815	2820	2825	rBV	585540	752880	11.26%	2.714%
50	21.175	3072	3075	3079	rBV4	84448	97407	1.46%	0.351%
51	21.386	3107	3111	3117	rBV	5941126	6685421	100.00%	24.095%
52	21.475	3121	3126	3134	rVV	2436766	2990239	44.73%	10.777%
53	23.733	3505	3510	3516	rBV	314765	616145	9.22%	2.221%
54	23.898	3531	3538	3549	rVB	1260097	2740363	40.99%	9.877%




Sum of corrected areas: 27745561

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023744.D
Acq On : 21 Jan 2023 02:08
Operator : CG/JU
Sample : 01146-11MEDL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4412MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

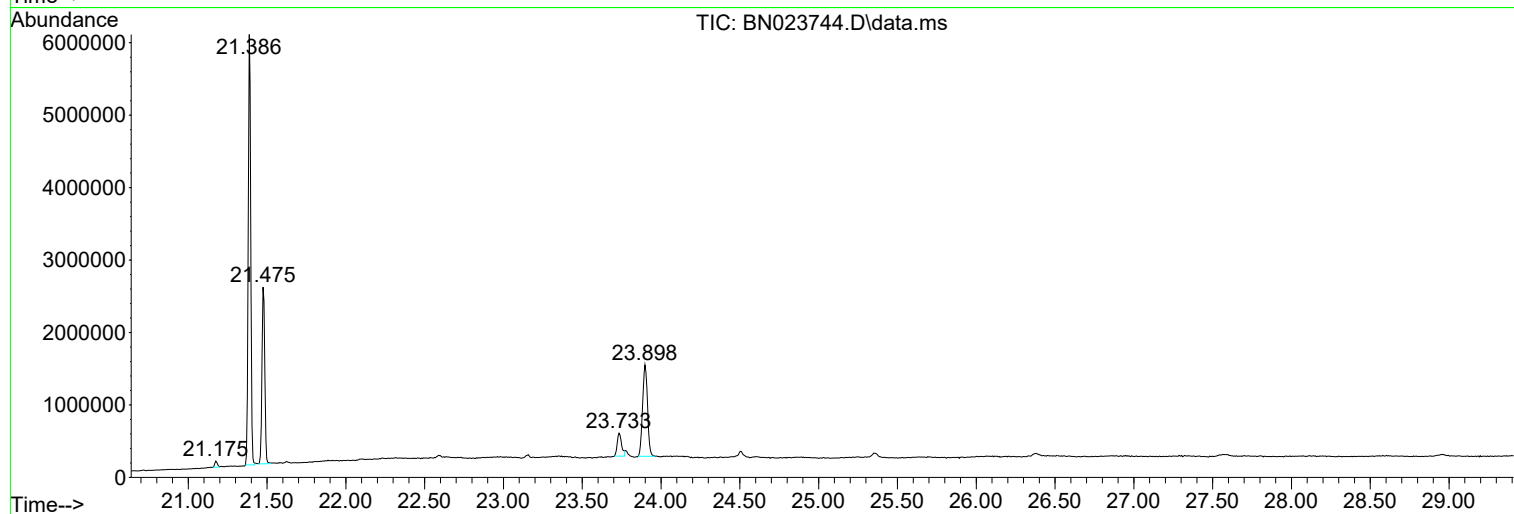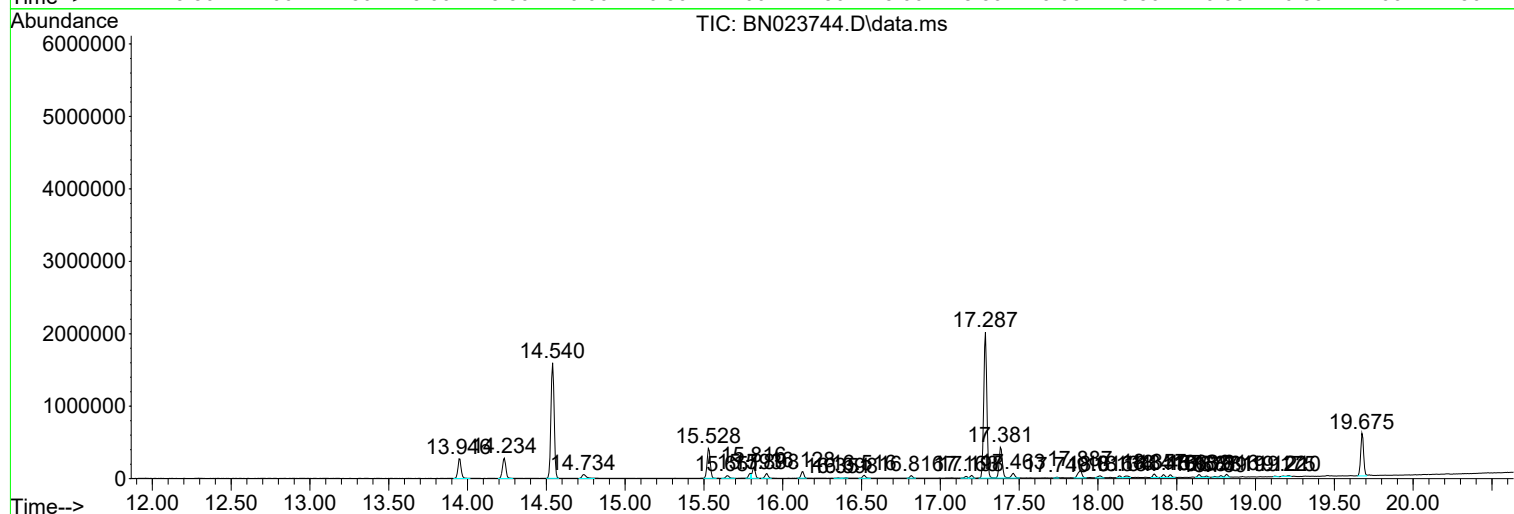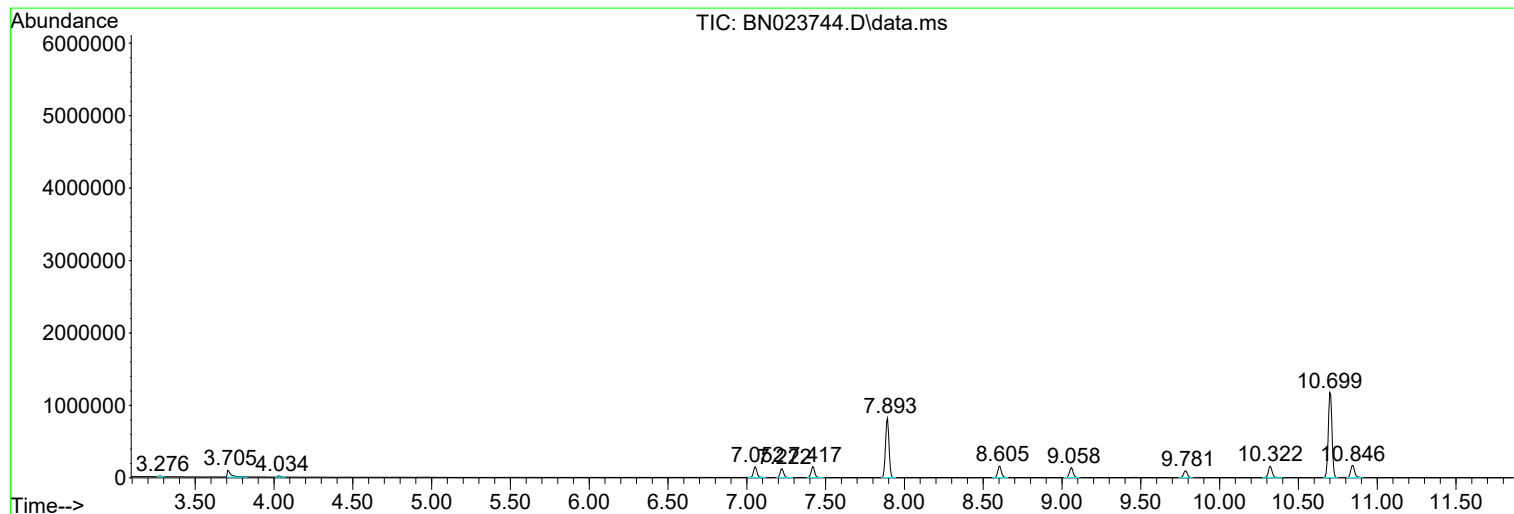

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023744.D
Acq On : 21 Jan 2023 02:08
Operator : CG/JU
Sample : 01146-11MEDL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4412MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012023\
Data File : BN023744.D
Acq On : 21 Jan 2023 02:08
Operator : CG/JU
Sample : 01146-11MEDL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4412MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------