

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012422\
 Data File : BN018450.D
 Acq On : 24 Jan 2022 14:30
 Operator : CG/JU
 Sample : SSTDICCC0.4
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4

Quant Time: Jan 24 17:54:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN012422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 24 17:52:32 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.965	152	32216	0.400	ng	0.00
7) Naphthalene-d8	10.761	136	144234	0.400	ng	# 0.00
13) Acenaphthene-d10	14.573	164	77548	0.400	ng	0.00
19) Phenanthrene-d10	17.310	188	139051	0.400	ng	# 0.00
29) Chrysene-d12	21.493	240	91003	0.400	ng	# 0.00
35) Perylene-d12	23.902	264	66652	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.512	112	31425	0.397	ng	0.00
5) Phenol-d6	7.108	99	33395	0.420	ng	0.00
8) Nitrobenzene-d5	9.114	82	29413	0.320	ng	0.00
11) 2-Methylnaphthalene-d10	12.350	152	96097	0.426	ng	0.00
14) 2,4,6-Tribromophenol	16.056	330	8478	0.277	ng	0.00
15) 2-Fluorobiphenyl	13.216	172	111770	0.399	ng	0.00
27) Fluoranthene-d10	19.341	212	166230	0.419	ng	0.00
31) Terphenyl-d14	19.937	244	121642	0.618	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.392	88	7240	0.399	ng	# 60
3) n-Nitrosodimethylamine	3.724	42	10264	0.353	ng	98
6) bis(2-Chloroethyl)ether	7.375	93	35740	0.416	ng	98
9) Naphthalene	10.812	128	139971	0.382	ng	100
10) Hexachlorobutadiene	11.116	225	27834	0.409	ng	# 100
12) 2-Methylnaphthalene	12.421	142	98705	0.440	ng	99
16) Acenaphthylene	14.294	152	105150	0.341	ng	100
17) Acenaphthene	14.637	154	80970	0.377	ng	97
18) Fluorene	15.626	166	97729	0.404	ng	100
20) 4,6-Dinitro-2-methylph...	15.690	198	1481	0.152	ng	98
21) 4-Bromophenyl-phenylether	16.506	248	29154	0.381	ng	# 93
22) Hexachlorobenzene	16.628	284	33005	0.324	ng	# 93
23) Atrazine	16.774	200	16902	0.332	ng	98
24) Pentachlorophenol	16.969	266	7840	0.317	ng	99
25) Phenanthrene	17.358	178	148378	0.380	ng	100
26) Anthracene	17.443	178	119296	0.369	ng	99
28) Fluoranthene	19.371	202	162796	0.392	ng	# 98
30) Pyrene	19.733	202	164667	0.511	ng	100
32) Benzo(a)anthracene	21.472	228	112823	0.421	ng	99
33) Chrysene	21.525	228	112322	0.369	ng	100
34) Bis(2-ethylhexyl)phtha...	21.419	149	91783	0.571	ng	98
36) Indeno(1,2,3-cd)pyrene	26.408	276	39463	0.186	ng	# 94
37) Benzo(b)fluoranthene	23.169	252	97611	0.452	ng	# 89
38) Benzo(k)fluoranthene	23.217	252	82239	0.389	ng	# 86
39) Benzo(a)pyrene	23.796	252	67874	0.340	ng	# 83
40) Dibenzo(a,h)anthracene	26.432	278	23938	0.151	ng	# 76
41) Benzo(g,h,i)perylene	27.171	276	43578	0.225	ng	# 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012422\
Data File : BN018450.D
Acq On : 24 Jan 2022 14:30
Operator : CG/JU
Sample : SSTDICCC0.4
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4

Quant Time: Jan 24 17:54:14 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN012422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 24 17:52:32 2022
Response via : Initial Calibration




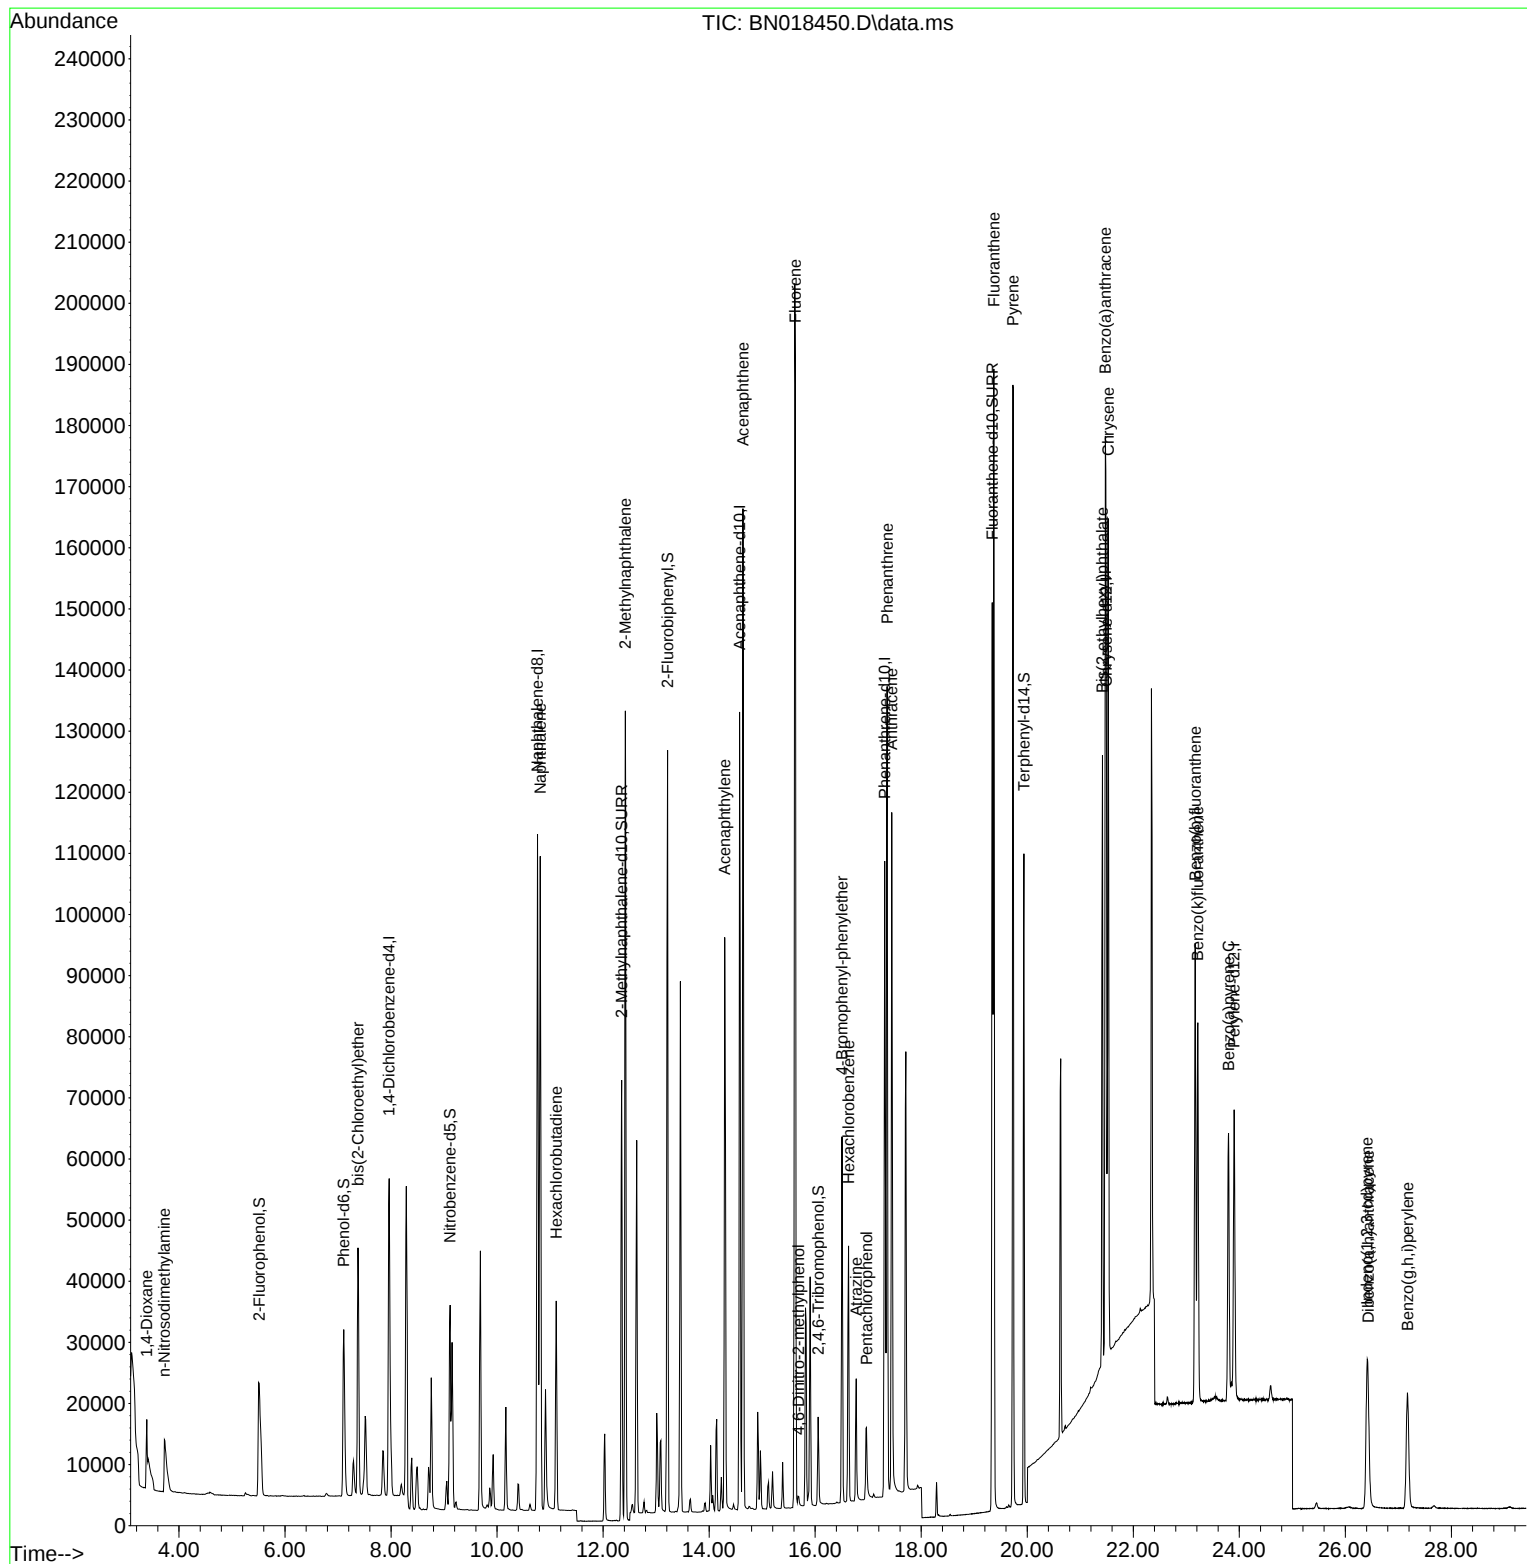




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.965 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: BN018450.D
 Acq: 24 Jan 2022 14:30




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4


Tgt Ion:152 Resp: 32216
 Ion Ratio Lower Upper
 152 100
 150 154.6 121.7 182.5
 115 58.4 43.8 65.8

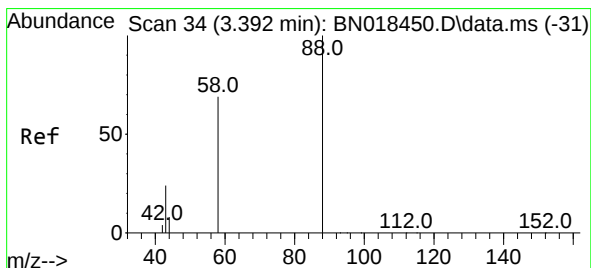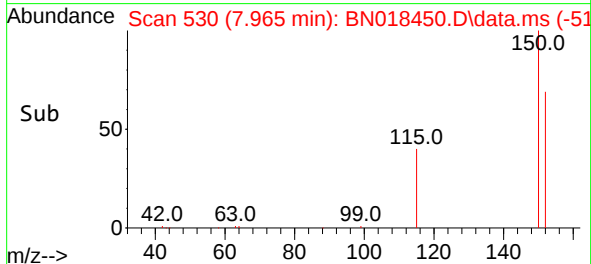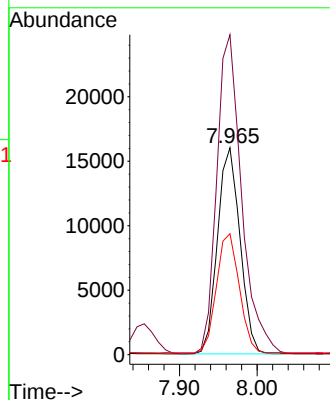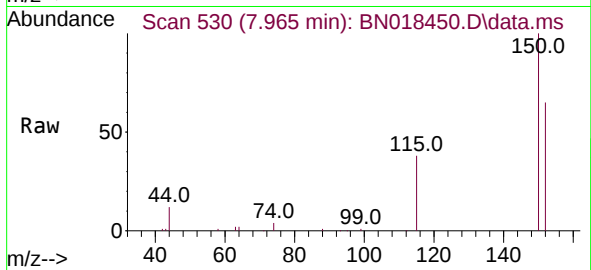

#2
 1,4-Dioxane
 Concen: 0.399 ng
 RT: 3.392 min Scan# 34
 Delta R.T. 0.000 min
 Lab File: BN018450.D
 Acq: 24 Jan 2022 14:30

Tgt Ion: 88 Resp: 7240
 Ion Ratio Lower Upper
 88 100
 43 32.3 69.7 104.5#
 58 80.8 83.8 125.8#

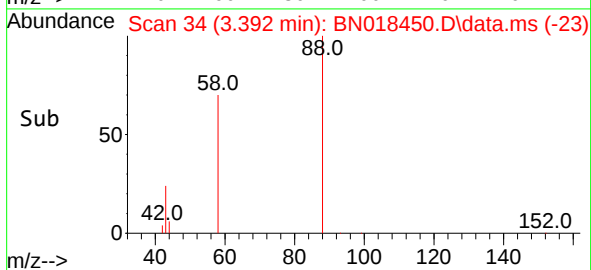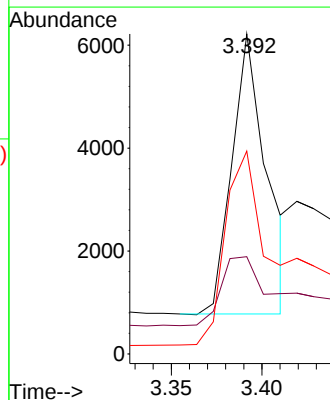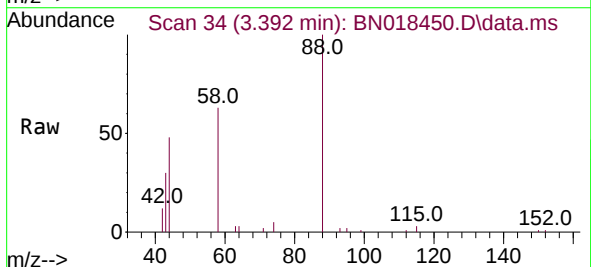







#3
 n-Nitrosodimethylamine
 Concen: 0.353 ng
 RT: 3.724 min Scan# 70
 Delta R.T. 0.000 min
 Lab File: BN018450.D
 Acq: 24 Jan 2022 14:30

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.4

Tgt Ion: 42 Resp: 10264




Ion	Ratio	Lower	Upper
42	100		
74	138.4	108.6	163.0
44	8.1	5.8	8.8

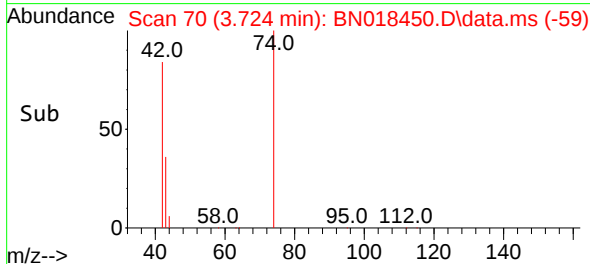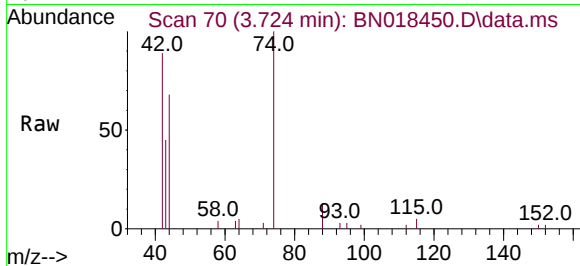


#4
 2-Fluorophenol
 Concen: 0.397 ng
 RT: 5.512 min Scan# 264
 Delta R.T. 0.000 min
 Lab File: BN018450.D
 Acq: 24 Jan 2022 14:30

Tgt Ion: 112 Resp: 31425

Ion	Ratio	Lower	Upper
112	100		
64	56.8	48.0	72.0
63	29.1	25.3	37.9


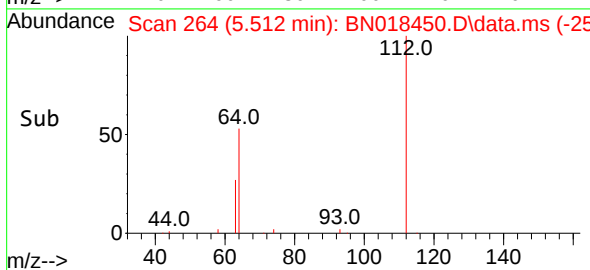

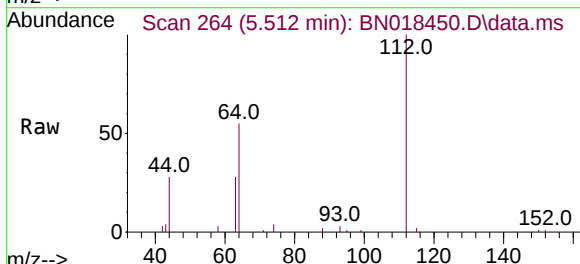




#5
Phenol-d6
Concen: 0.420 ng
RT: 7.108 min Scan# 41
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion: 99 Resp: 33395
Ion Ratio Lower Upper
99 100
42 17.6 16.3 24.5
71 30.5 26.8 40.2

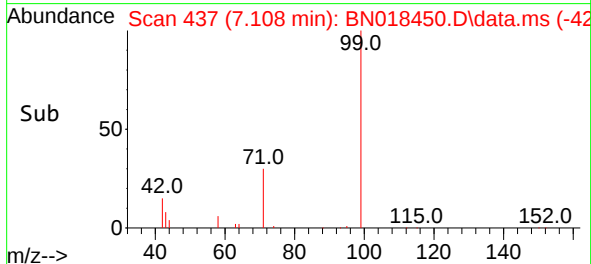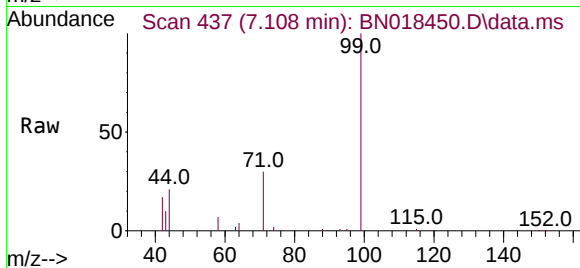

#6
bis(2-Chloroethyl)ether
Concen: 0.416 ng
RT: 7.375 min Scan# 466
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30

Tgt Ion: 93 Resp: 35740
Ion Ratio Lower Upper
93 100
63 75.0 61.7 92.5
95 32.4 26.2 39.4


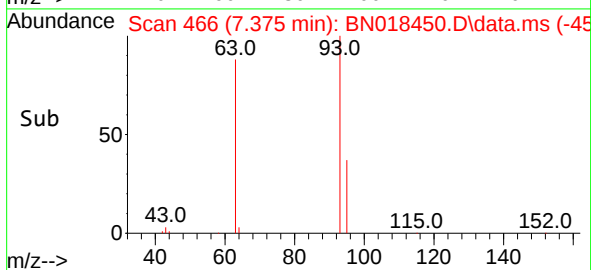

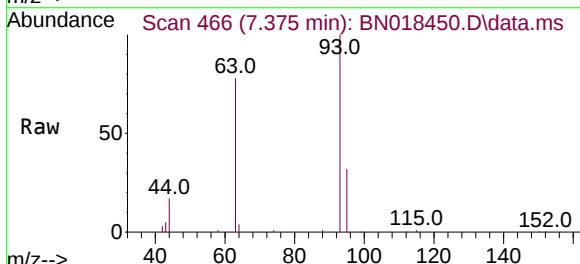




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.761 min Scan# 761
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:136 Resp: 144234
Ion Ratio Lower Upper
136 100
137 11.0 8.8 13.2
54 7.9 5.0 7.6#
68 6.3 4.4 6.6

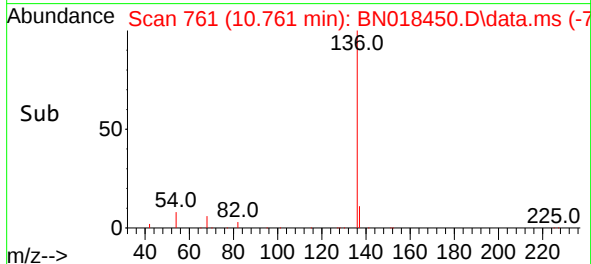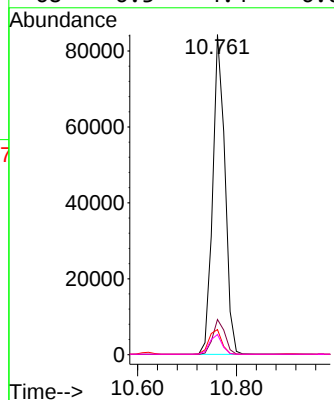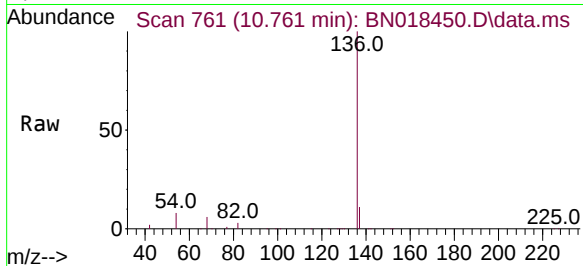

#8
Nitrobenzene-d5
Concen: 0.320 ng
RT: 9.114 min Scan# 631
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30

Tgt Ion: 82 Resp: 29413
Ion Ratio Lower Upper
82 100
128 43.8 33.7 50.5
54 47.5 36.6 55.0

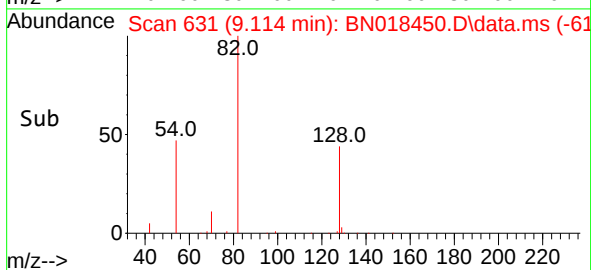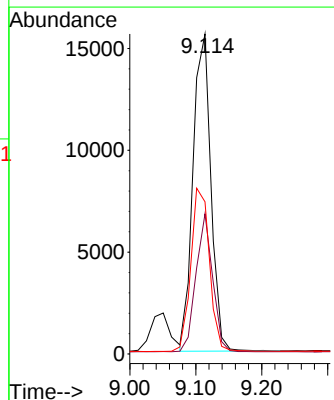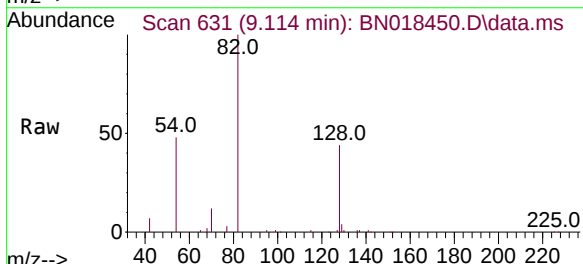







#9
Naphthalene

Concen: 0.382 ng
RT: 10.812 min Scan# 765
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30

Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4




Tgt Ion:128 Resp: 139971
Ion Ratio Lower Upper
128 100
129 11.0 8.7 13.1
127 12.9 10.4 15.6

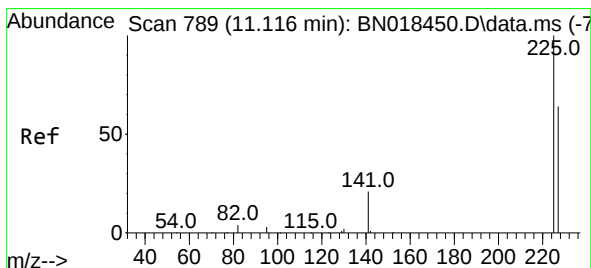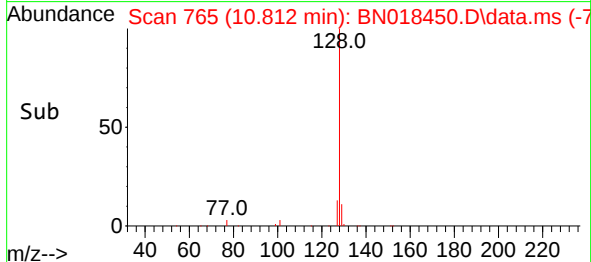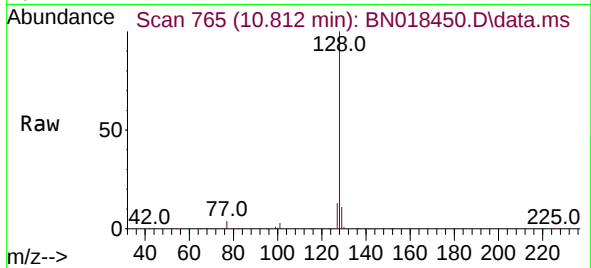


#10

Hexachlorobutadiene
Concen: 0.409 ng
RT: 11.116 min Scan# 789
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30

Tgt Ion:225 Resp: 27834
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.5 51.0 76.6


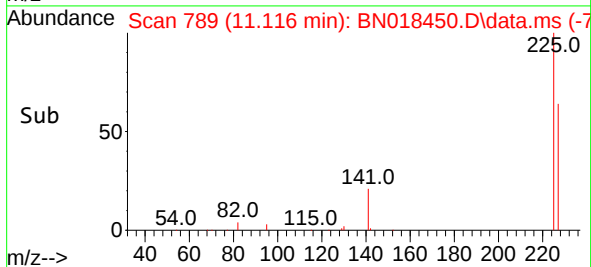

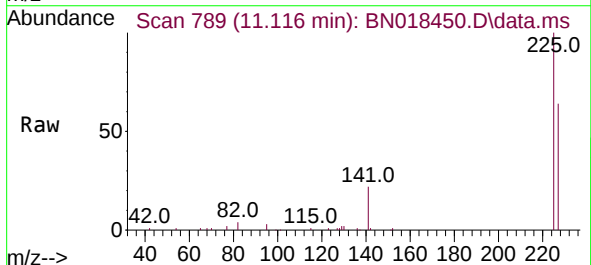




#11
2-Methylnaphthalene-d10
Concen: 0.426 ng
RT: 12.350 min Scan# 1009
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:152 Resp: 96097
Ion Ratio Lower Upper
152 100
151 20.1 16.2 24.2

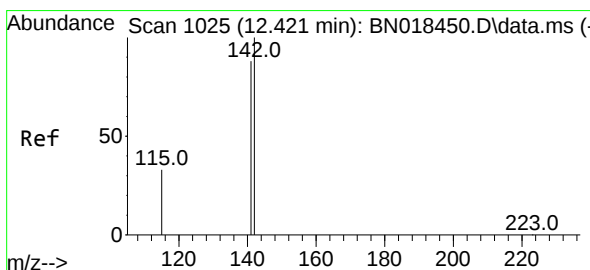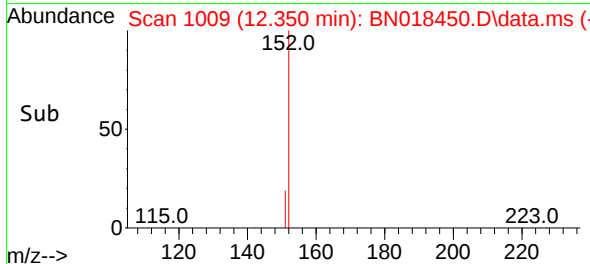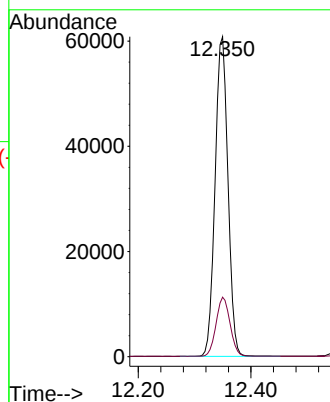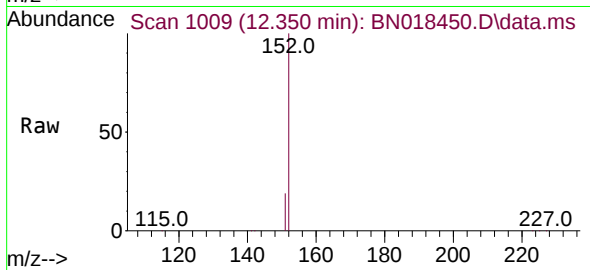

#12
2-Methylnaphthalene
Concen: 0.440 ng
RT: 12.421 min Scan# 1025
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30

Tgt Ion:142 Resp: 98705
Ion Ratio Lower Upper
142 100
141 87.6 70.0 105.0
115 33.1 27.8 41.8


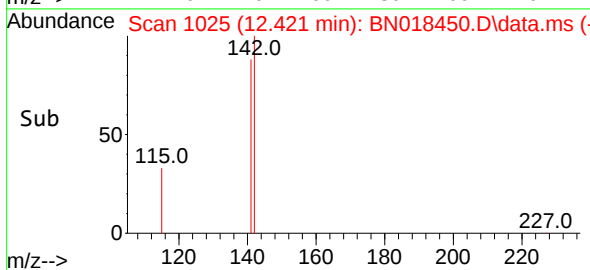
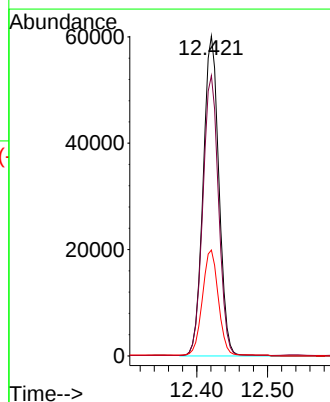
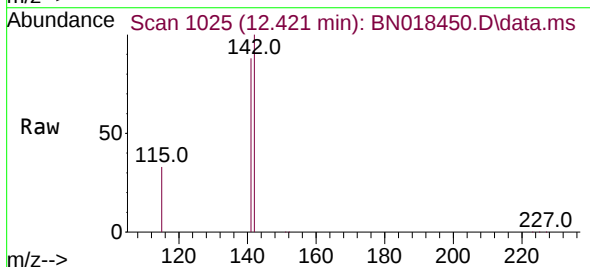




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.573 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:164 Resp: 77548
Ion Ratio Lower Upper
164 100
162 102.6 80.2 120.2
160 46.5 36.9 55.3

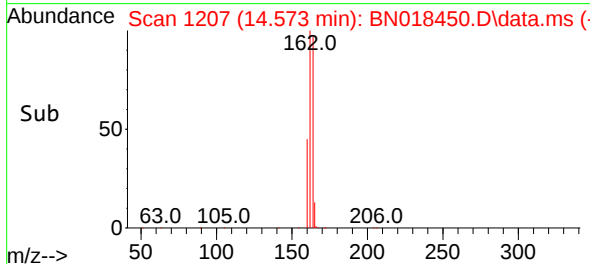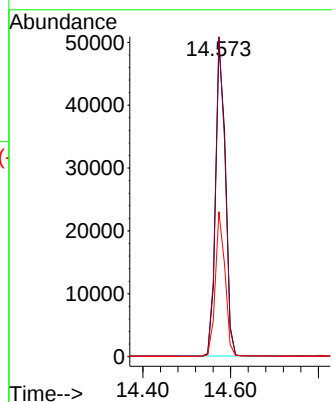

#14
2,4,6-Tribromophenol
Concen: 0.277 ng
RT: 16.056 min Scan# 1324
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30

Tgt Ion:330 Resp: 8478
Ion Ratio Lower Upper
330 100
332 100.9 0.0 0.0#
141 35.0 21.3 31.9#


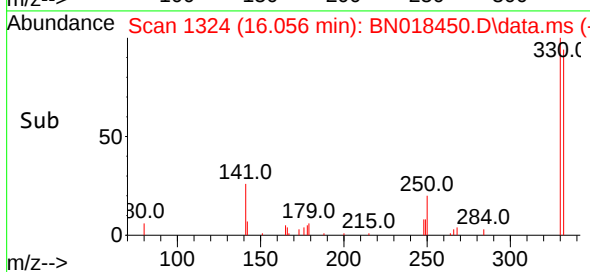
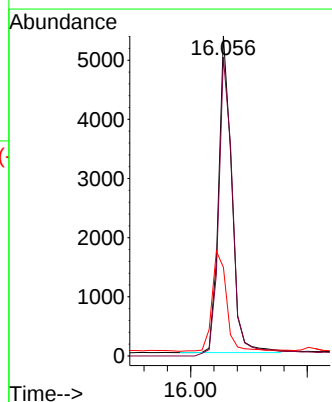





#15
2-Fluorobiphenyl
Concen: 0.399 ng
RT: 13.216 min Scan# 1100
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:172 Resp: 111770
Ion Ratio Lower Upper
172 100
171 33.6 27.4 41.0
170 22.0 18.4 27.6

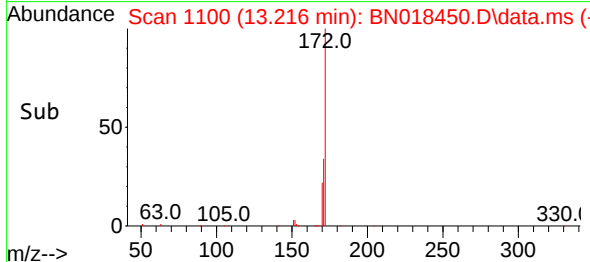

#16
Acenaphthylene
Concen: 0.341 ng
RT: 14.294 min Scan# 1185
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30

Tgt Ion:152 Resp: 105150
Ion Ratio Lower Upper
152 100
151 19.9 15.8 23.6
153 13.2 10.5 15.7


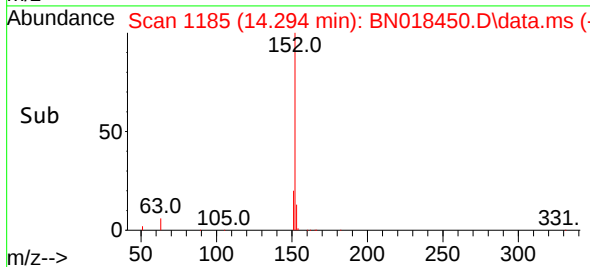

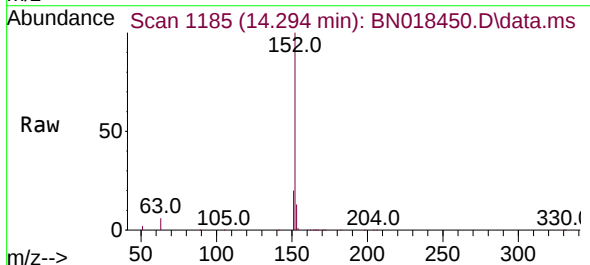




#17
Acenaphthene
Concen: 0.377 ng
RT: 14.637 min Scan# 1212
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:154 Resp: 80970
Ion Ratio Lower Upper
154 100
153 111.7 90.9 136.3
152 53.2 45.0 67.4

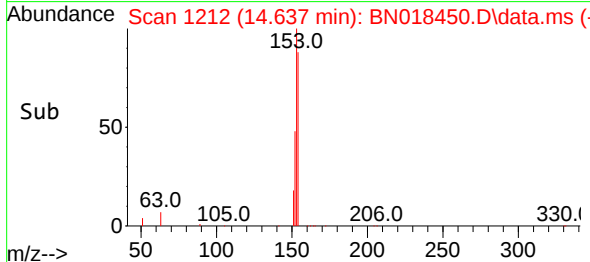

#18
Fluorene
Concen: 0.404 ng
RT: 15.626 min Scan# 1290
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30

Tgt Ion:166 Resp: 97729
Ion Ratio Lower Upper
166 100
165 97.4 77.8 116.6
167 13.5 10.9 16.3


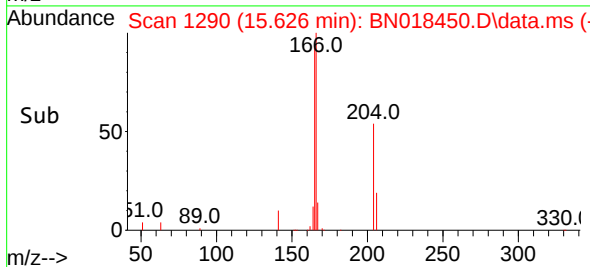

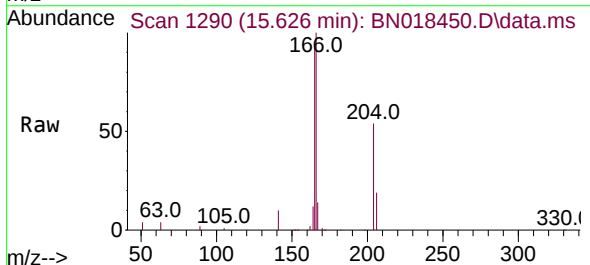


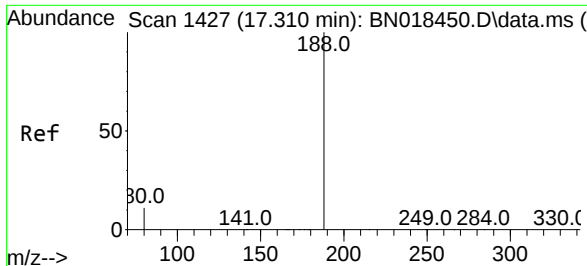

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.310 min Scan# 1427
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:188 Resp: 139051
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.8 7.0 10.4#

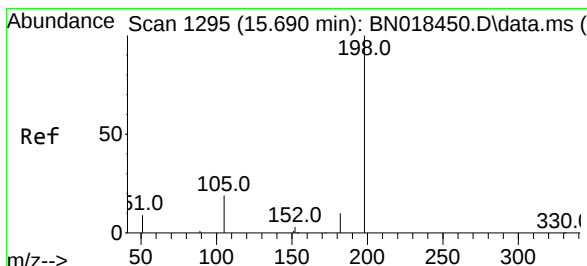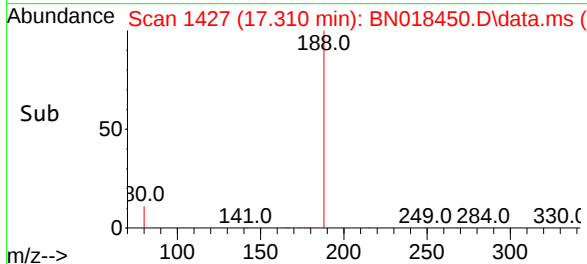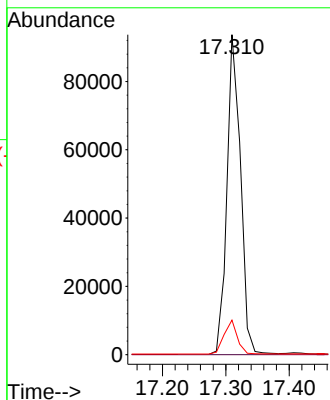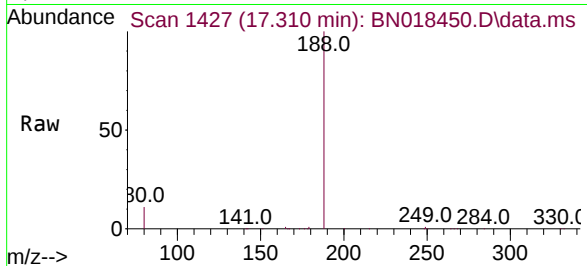

#20
4,6-Dinitro-2-methylphenol
Concen: 0.152 ng
RT: 15.690 min Scan# 1295
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30

Tgt Ion:198 Resp: 1481
Ion Ratio Lower Upper
198 100
182 18.3 15.5 23.3
77 0.0 0.0 0.0


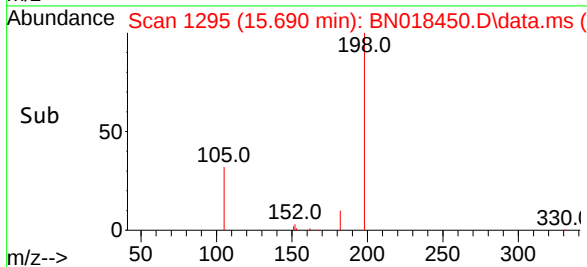
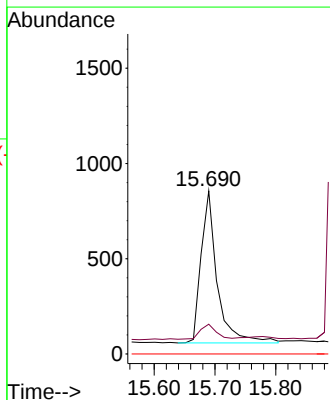
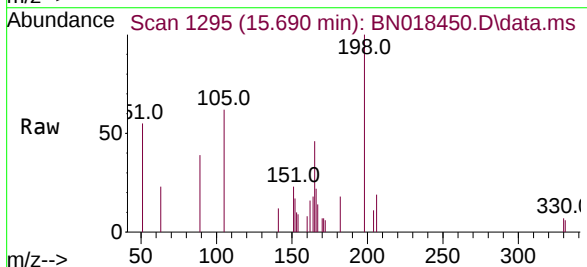




#21
4-Bromophenyl-phenylether
Concen: 0.381 ng
RT: 16.506 min Scan# 1361
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:248 Resp: 29154
Ion Ratio Lower Upper
248 100
250 93.8 74.4 111.6
141 67.3 43.7 65.5#

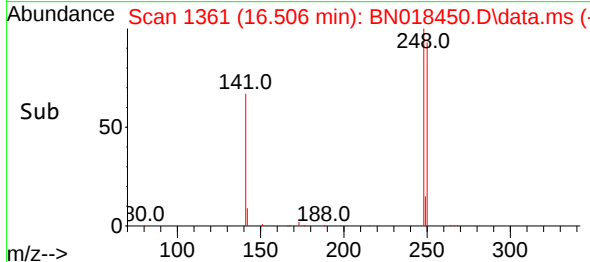

#22
Hexachlorobenzene
Concen: 0.324 ng
RT: 16.628 min Scan# 1371
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30

Tgt Ion:284 Resp: 33005
Ion Ratio Lower Upper
284 100
142 33.6 21.6 32.4#
249 30.7 23.5 35.3


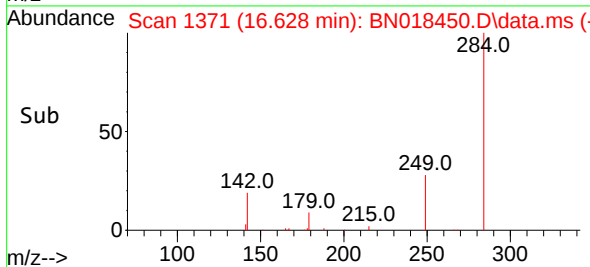

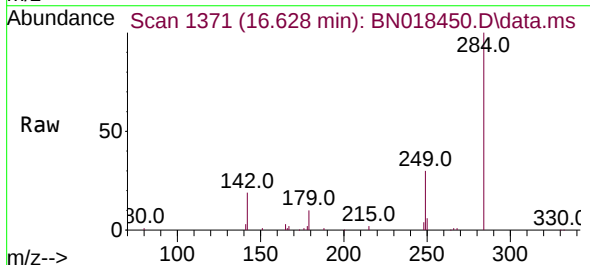




#23
 Atrazine
 Concen: 0.332 ng
 RT: 16.774 min Scan# 1383
 Delta R.T. 0.000 min
 Lab File: BN018450.D
 Acq: 24 Jan 2022 14:30




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4


Tgt Ion:200 Resp: 16902
 Ion Ratio Lower Upper
 200 100
 173 23.6 20.3 30.5
 215 49.4 40.4 60.6

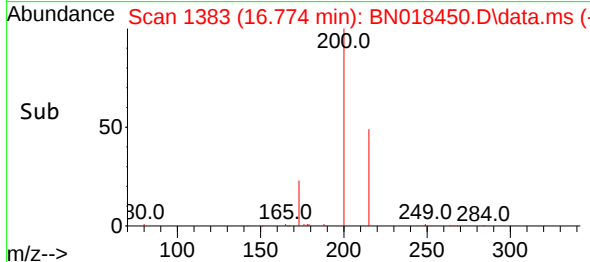

#24
 Pentachlorophenol
 Concen: 0.317 ng
 RT: 16.969 min Scan# 1399
 Delta R.T. 0.000 min
 Lab File: BN018450.D
 Acq: 24 Jan 2022 14:30

Tgt Ion:266 Resp: 7840
 Ion Ratio Lower Upper
 266 100
 264 61.4 49.5 74.3
 268 62.6 50.6 76.0


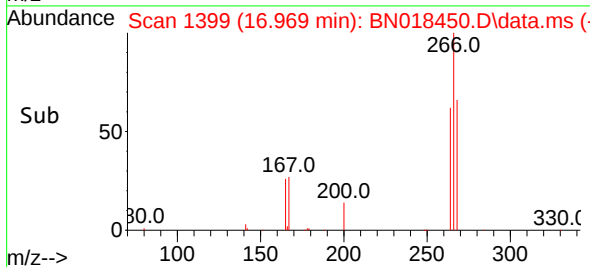

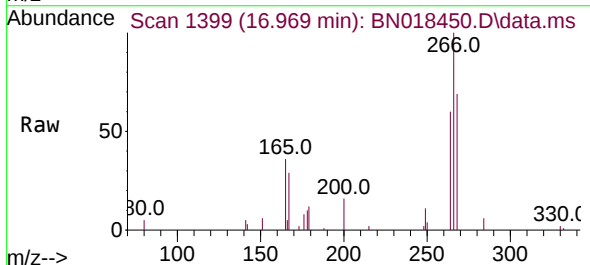


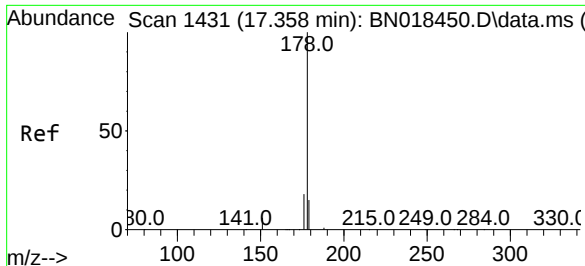

#25
Phenanthrene
Concen: 0.380 ng
RT: 17.358 min Scan# 1431
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:178 Resp: 148378
Ion Ratio Lower Upper
178 100
176 18.8 15.3 22.9
179 15.4 12.3 18.5

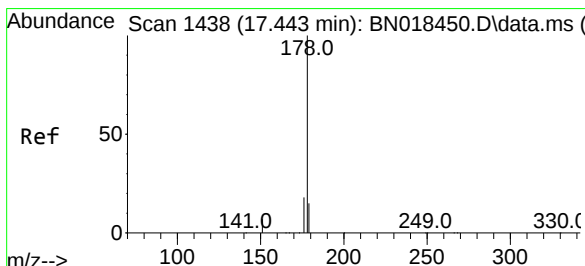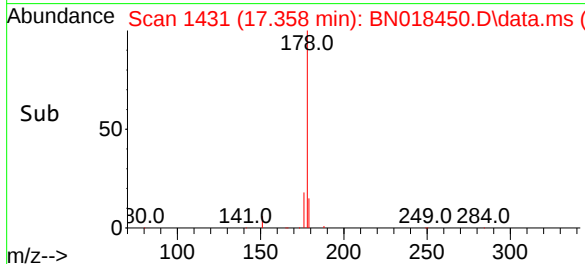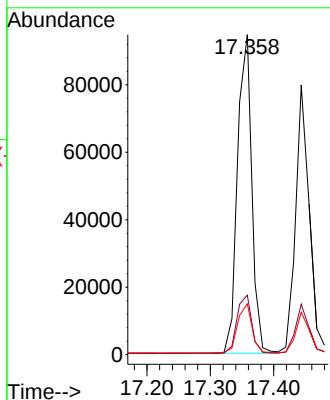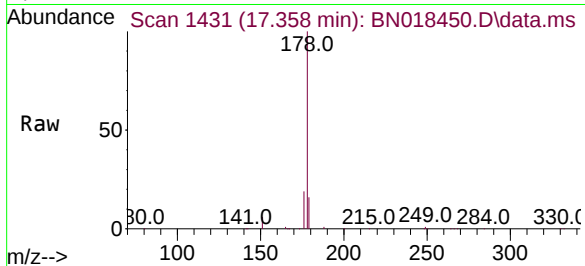

#26
Anthracene
Concen: 0.369 ng
RT: 17.443 min Scan# 1438
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30

Tgt Ion:178 Resp: 119296
Ion Ratio Lower Upper
178 100
176 18.1 14.8 22.2
179 15.2 12.2 18.4


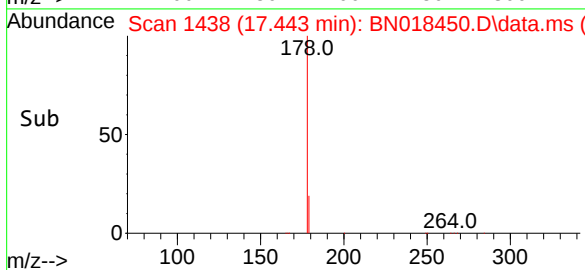
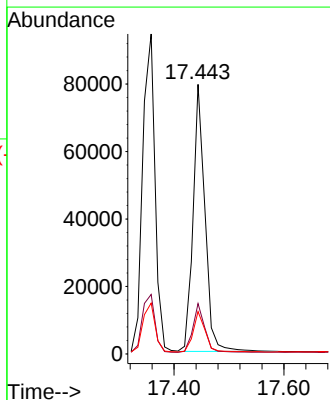
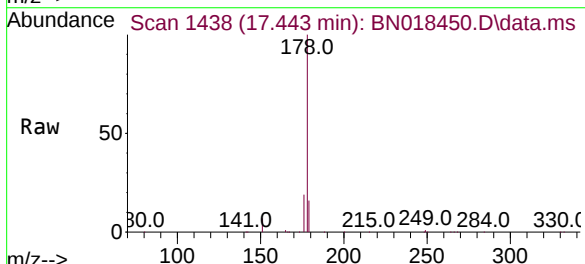




#27
Fluoranthene-d10
Concen: 0.419 ng
RT: 19.341 min Scan# 1752
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:212 Resp: 166230
Ion Ratio Lower Upper
212 100
106 13.0 8.4 12.6#
104 7.2 4.5 6.7#

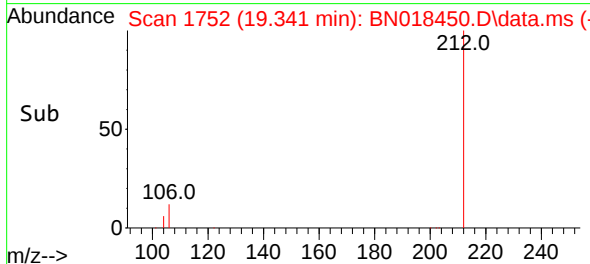

#28
Fluoranthene
Concen: 0.392 ng
RT: 19.371 min Scan# 1758
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30

Tgt Ion:202 Resp: 162796
Ion Ratio Lower Upper
202 100
101 11.3 7.2 10.8#
203 17.3 13.7 20.5



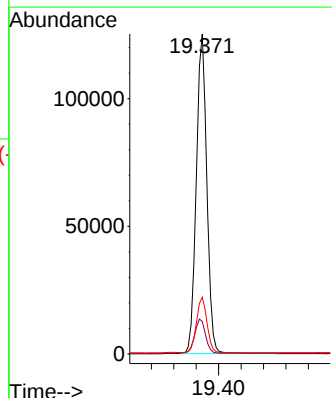
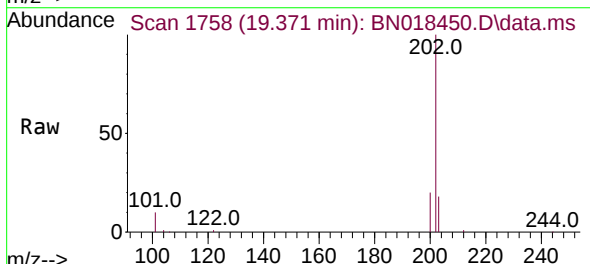




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.493 min Scan# 2026
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:240 Resp: 91003
Ion Ratio Lower Upper
240 100
120 10.5 6.0 9.0#
236 25.8 21.4 32.2

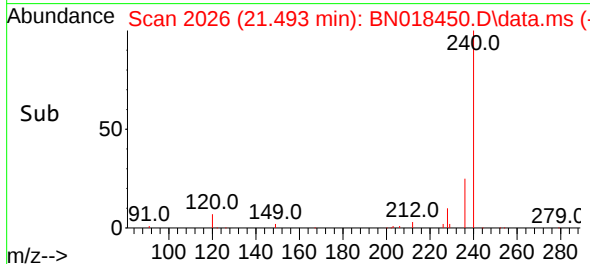

#30
Pyrene
Concen: 0.511 ng
RT: 19.733 min Scan# 1831
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30

Tgt Ion:202 Resp: 164667
Ion Ratio Lower Upper
202 100
200 20.5 16.6 25.0
203 17.7 14.1 21.1


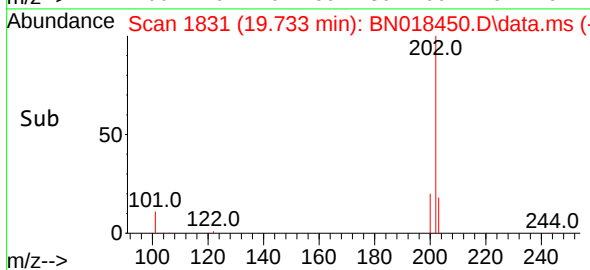

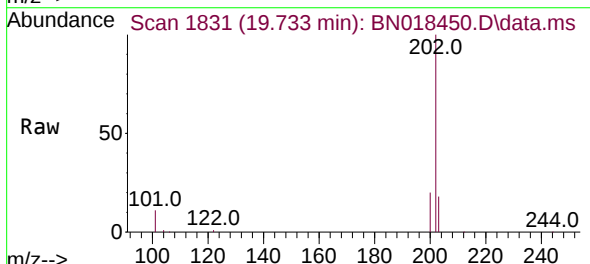




#31
 Terphenyl-d14
 Concen: 0.618 ng
 RT: 19.937 min Scan# 1872
 Delta R.T. 0.000 min
 Lab File: BN018450.D
 Acq: 24 Jan 2022 14:30




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4


Tgt Ion:244 Resp: 121642
 Ion Ratio Lower Upper
 244 100
 212 7.6 6.2 9.2
 122 12.0 7.9 11.9#

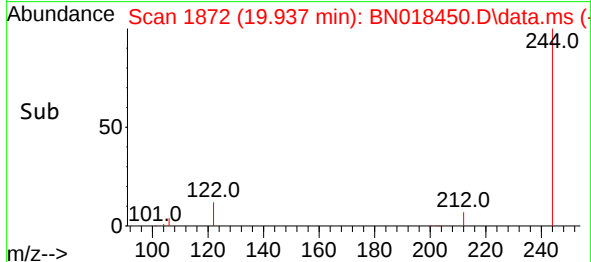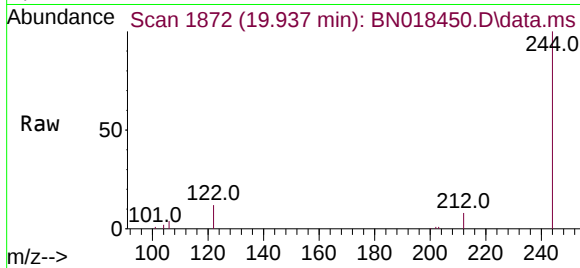

#32
 Benzo(a)anthracene
 Concen: 0.421 ng
 RT: 21.472 min Scan# 2024
 Delta R.T. 0.000 min
 Lab File: BN018450.D
 Acq: 24 Jan 2022 14:30

Tgt Ion:228 Resp: 112823
 Ion Ratio Lower Upper
 228 100
 226 27.1 21.3 31.9
 229 19.5 15.9 23.9

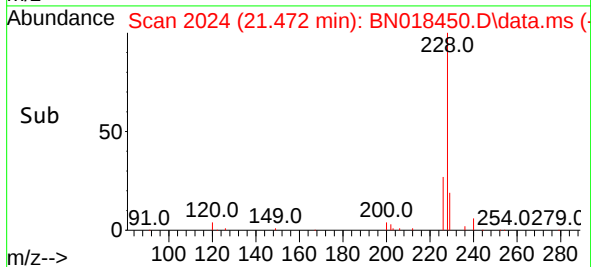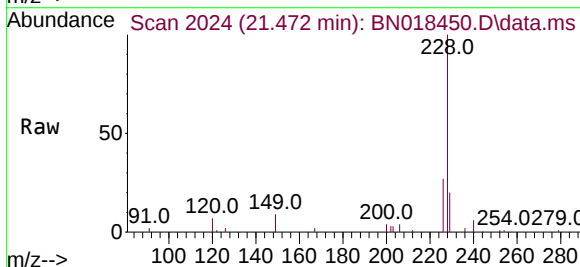

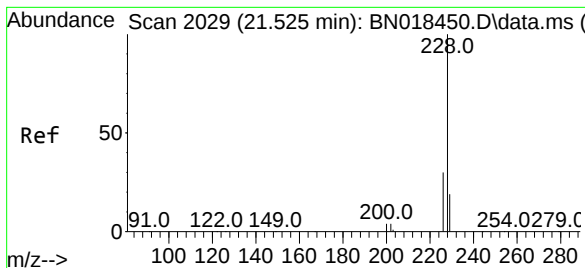

#33

Chrysene

Concen: 0.369 ng

RT: 21.525 min Scan# 2029

Delta R.T. 0.000 min

Lab File: BN018450.D

Acq: 24 Jan 2022 14:30

Instrument :

BNA_N

ClientSampleId :

SSTDICCC0.4





Tgt Ion:228 Resp: 112322

Ion Ratio Lower Upper

228 100

226 30.1 24.2 36.4

229 19.3 15.5 23.3

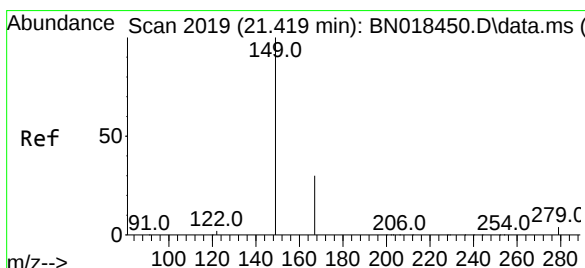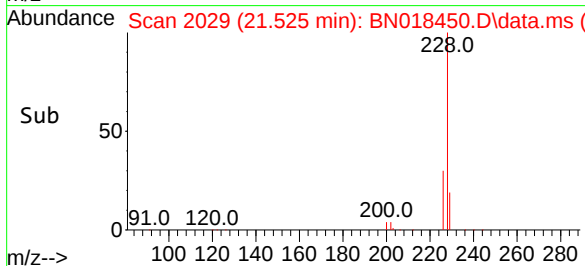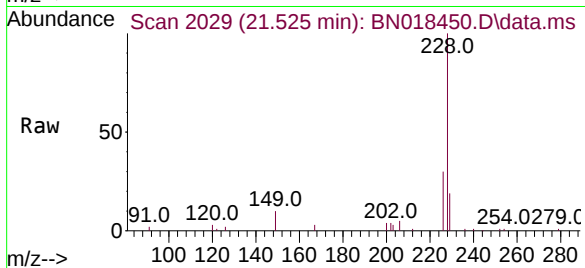

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.571 ng

RT: 21.419 min Scan# 2019

Delta R.T. 0.000 min

Lab File: BN018450.D

Acq: 24 Jan 2022 14:30




Tgt Ion:149 Resp: 91783


Ion Ratio Lower Upper

149 100

167 28.4 23.7 35.5

279 4.1 3.6 5.4


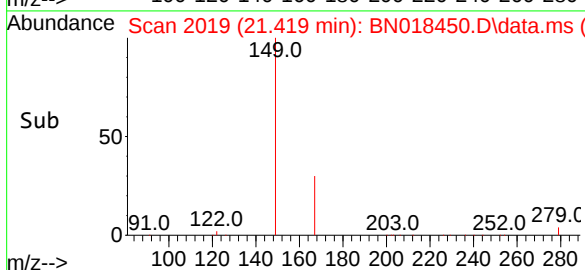

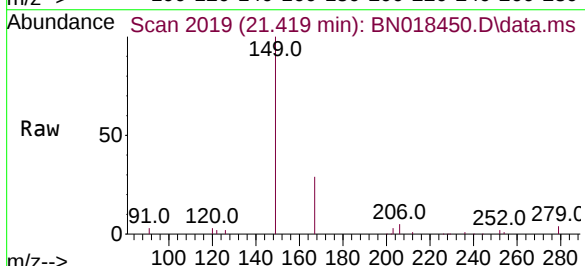




#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.902 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN018450.D
 Acq: 24 Jan 2022 14:30




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4


Tgt Ion:264 Resp: 66652
 Ion Ratio Lower Upper
 264 100
 260 24.9 20.2 30.4
 265 60.0 18.2 27.2#

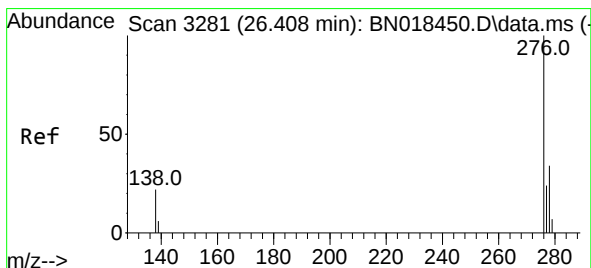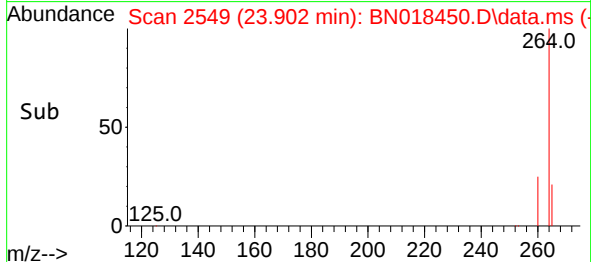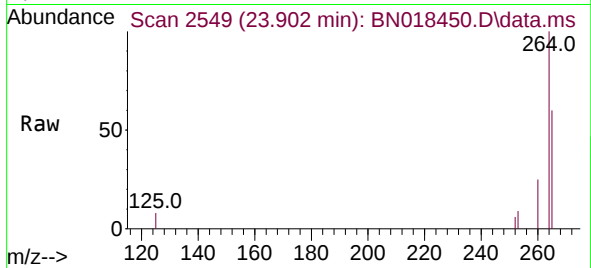

#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.186 ng
 RT: 26.408 min Scan# 3281
 Delta R.T. 0.000 min
 Lab File: BN018450.D
 Acq: 24 Jan 2022 14:30

Tgt Ion:276 Resp: 39463
 Ion Ratio Lower Upper
 276 100
 138 24.7 14.9 22.3#
 277 24.6 19.9 29.9

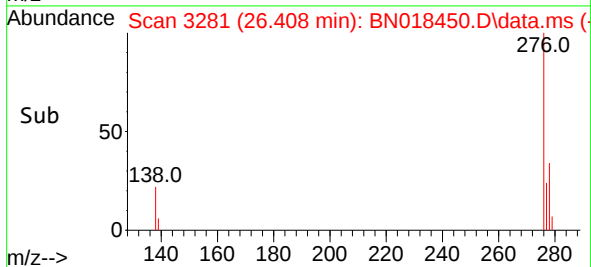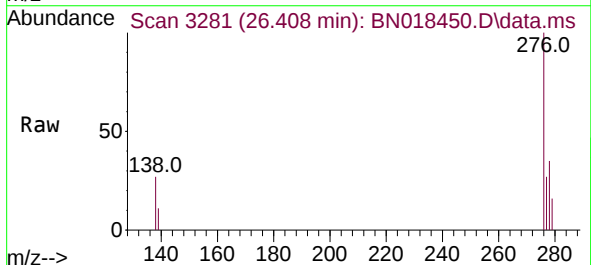



#37

Benzo(b)fluoranthene

Concen: 0.452 ng

RT: 23.169 min Scan# 2335

Delta R.T. 0.000 min

Lab File: BN018450.D

Acq: 24 Jan 2022 14:30

Instrument :

BN018450.D

ClientSampleId :

SSTDICCC0.4





Tgt Ion:252 Resp: 97611

Ion Ratio Lower Upper

252 100

253 26.1 17.8 26.6

125 13.8 6.0 9.0#

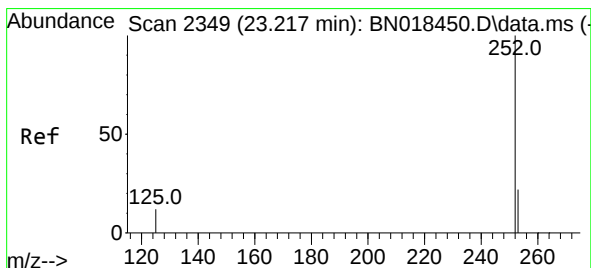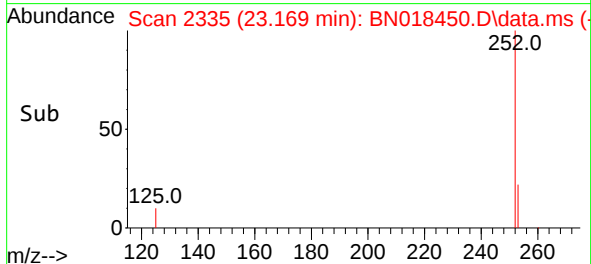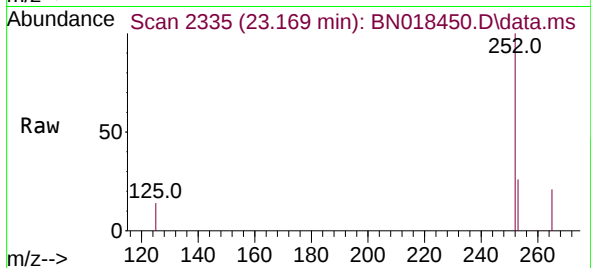

#38

Benzo(k)fluoranthene

Concen: 0.389 ng

RT: 23.217 min Scan# 2349

Delta R.T. 0.000 min

Lab File: BN018450.D

Acq: 24 Jan 2022 14:30




Tgt Ion:252 Resp: 82239


Ion Ratio Lower Upper

252 100

253 27.0 17.7 26.5#

125 16.8 6.2 9.2#


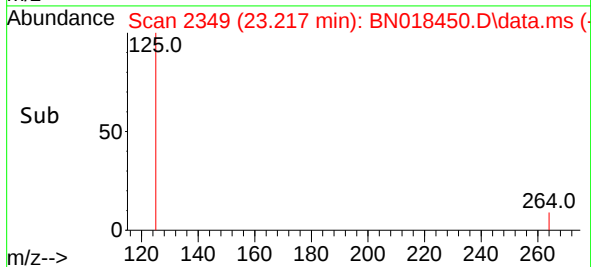

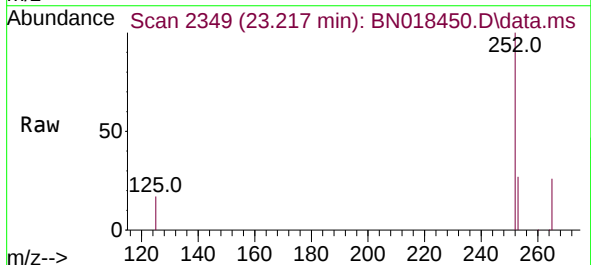




#39
Benzo(a)pyrene
Concen: 0.340 ng
RT: 23.796 min Scan# 2518
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICCC0.4


Tgt Ion:252 Resp: 67874
Ion Ratio Lower Upper
252 100
253 28.9 17.8 26.6#
125 17.7 7.0 10.4#

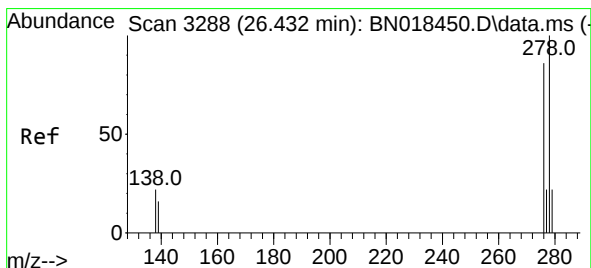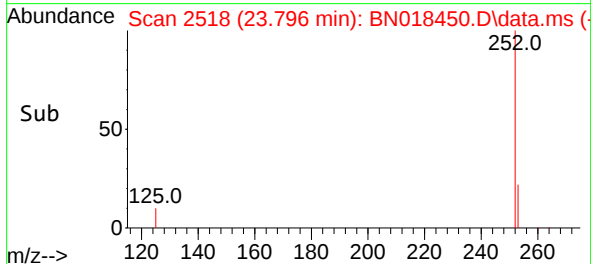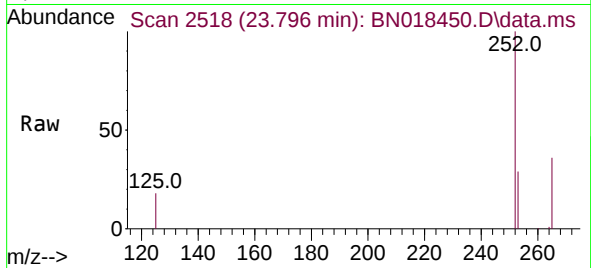

#40
Dibenzo(a,h)anthracene
Concen: 0.151 ng
RT: 26.432 min Scan# 3288
Delta R.T. 0.000 min
Lab File: BN018450.D
Acq: 24 Jan 2022 14:30

Tgt Ion:278 Resp: 23938
Ion Ratio Lower Upper
278 100
139 23.2 10.8 16.2#
279 35.6 19.0 28.4#

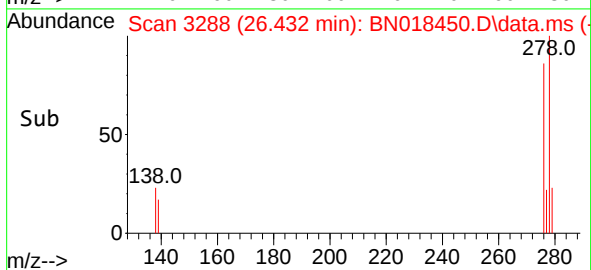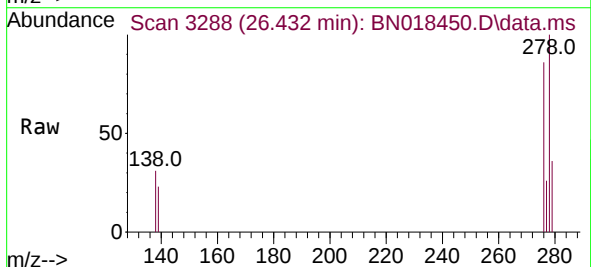

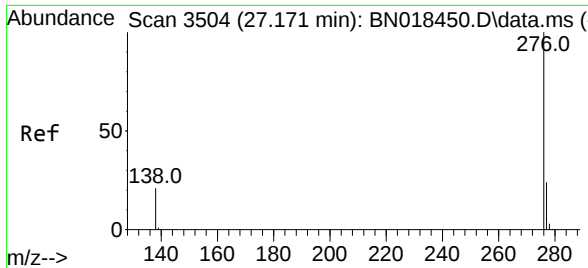

#41
 Benzo(g,h,i)perylene
 Concen: 0.225 ng
 RT: 27.171 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: BN018450.D
 Acq: 24 Jan 2022 14:30

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICCC0.4

Tgt Ion:276 Resp: 43578
 Ion Ratio Lower Upper
 276 100
 277 26.2 19.0 28.6
 138 25.8 12.6 19.0#

