
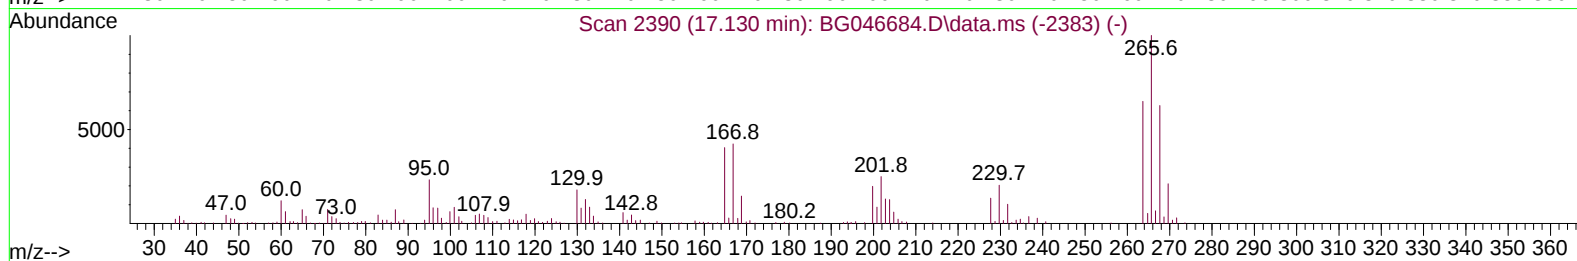
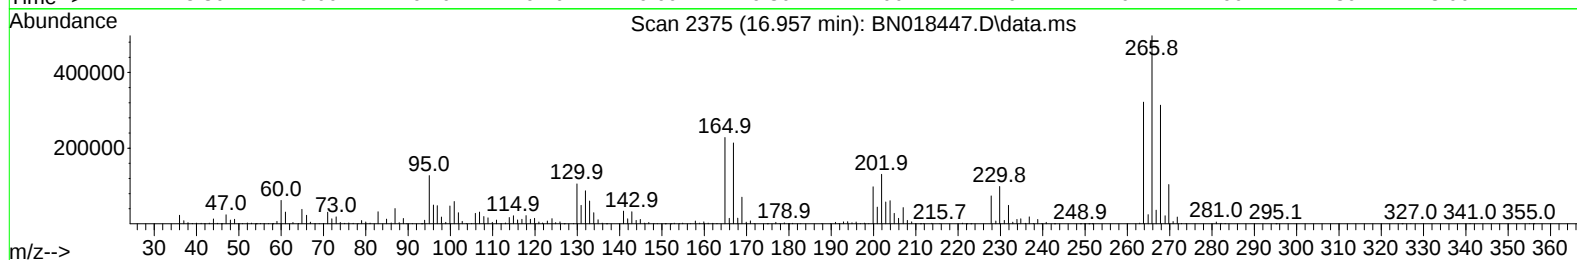


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012422\
Data File : BN018447.D
Acq On : 24 Jan 2022 12:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 17:45:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 24 17:44:56 2022
Response via : Initial Calibration

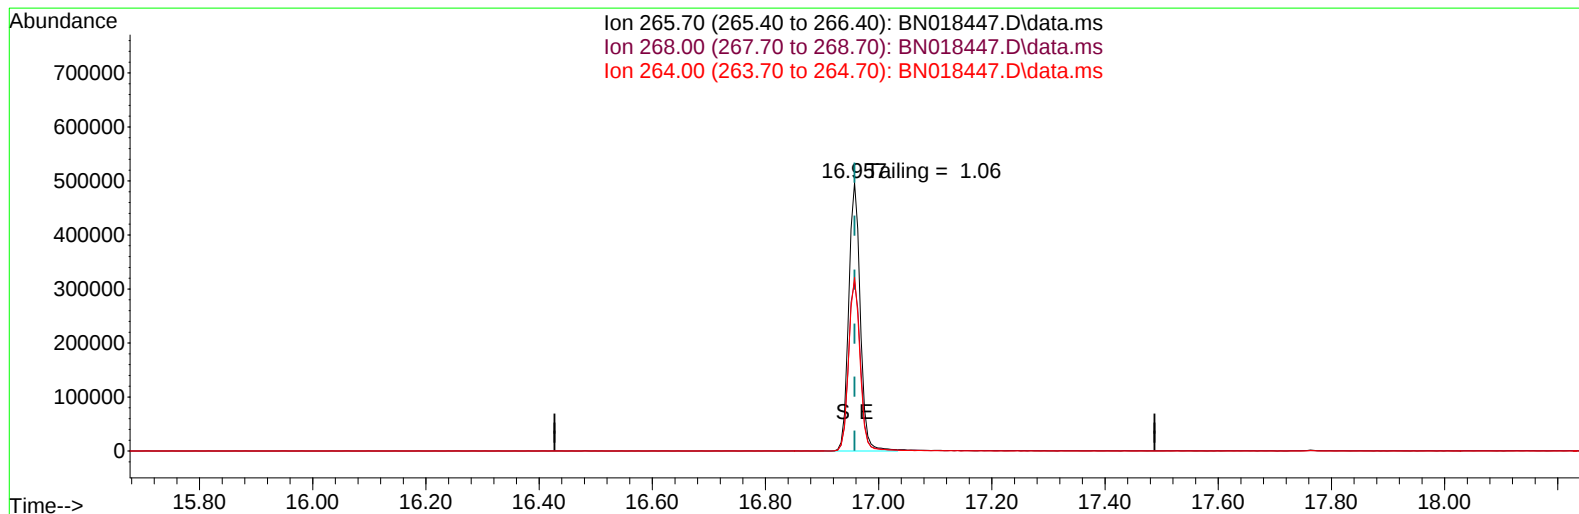

TIC: BN018447.D\data.ms

(70) Pentachlorophenol (C)




16.957min (0.000) 23834.84 ng

response 709293

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.07
264.00	61.60	64.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012422\
Data File : BN018447.D
Acq On : 24 Jan 2022 12:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 17:45:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 24 17:44:56 2022
Response via : Initial Calibration

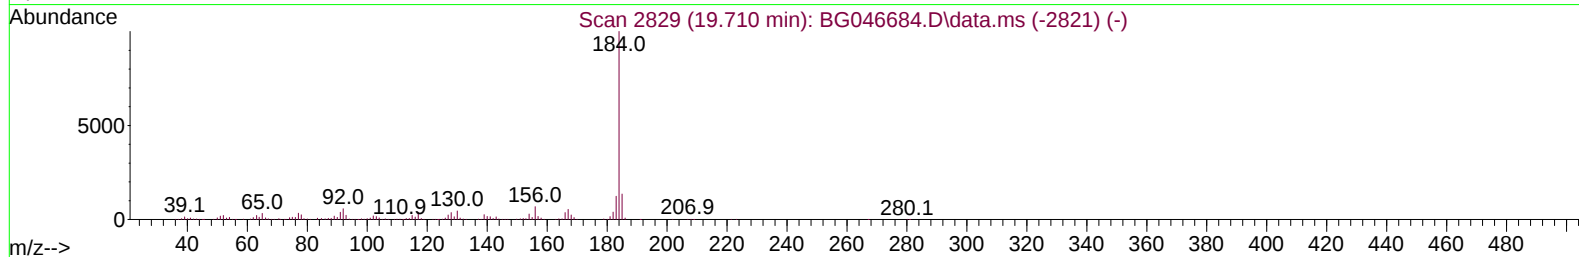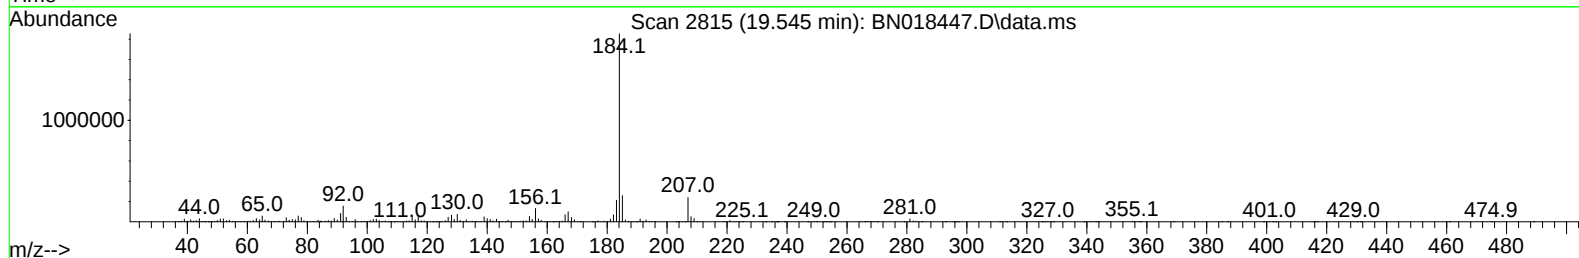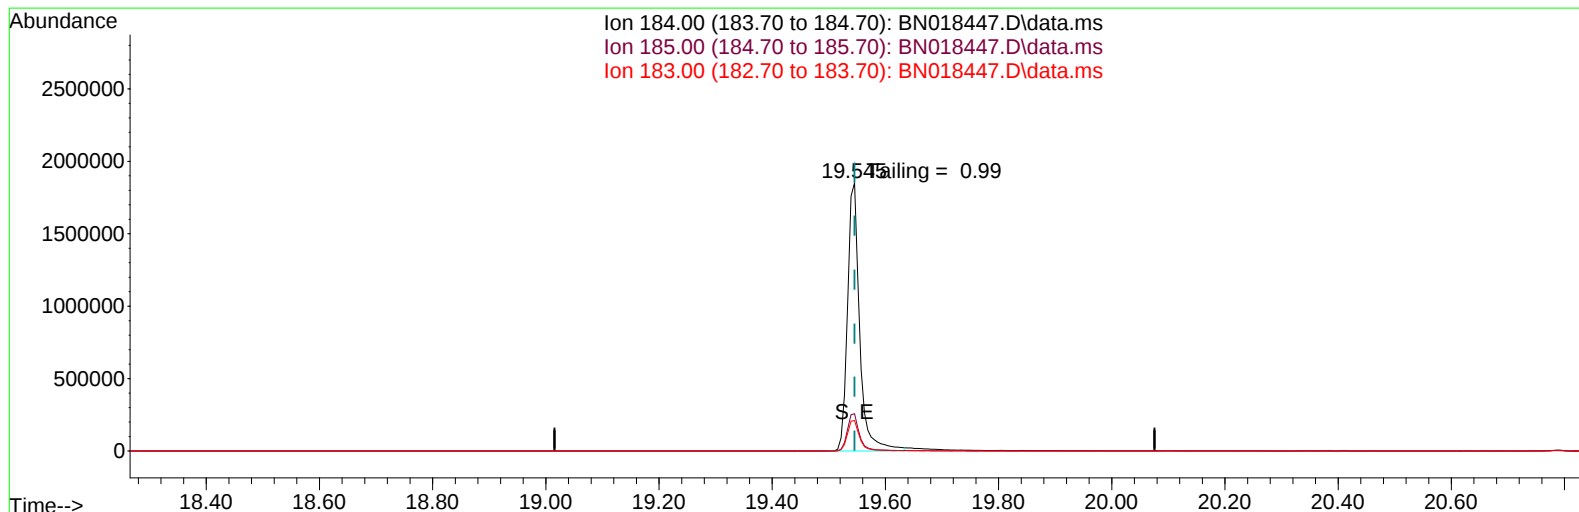

TIC: BN018447.D\data.ms

(77) Benzidine**19.545min (0.000) 210571.82 ng****response 2856020**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.89
183.00	13.20	11.39
0.00	0.00	0.00