

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012523\
 Data File : BN023791.D
 Acq On : 25 Jan 2023 12:39
 Operator : CG/JU
 Sample : PB150438BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK438

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023791.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	27	32	40	rVB	55077	74280	1.97%	0.167%
2	3.693	101	103	126	rBV	518064	806028	21.35%	1.813%
3	4.028	156	160	169	rVB	15360	24820	0.66%	0.056%
4	7.046	667	673	687	rVB	859431	1336283	35.39%	3.006%
5	7.216	696	702	711	rBV	712201	1064469	28.19%	2.395%
6	7.410	728	735	749	rVB	893389	1390225	36.82%	3.127%
7	7.887	809	816	826	rVB	769115	1210637	32.06%	2.723%
8	8.599	930	937	949	rBV	1044507	1614220	42.75%	3.631%
9	9.051	1007	1014	1031	rBV	813733	1294734	34.29%	2.912%
10	9.775	1129	1137	1148	rBV	683913	1080479	28.61%	2.431%
11	10.316	1222	1229	1243	rBV	992672	1633500	43.26%	3.675%
12	10.693	1285	1293	1302	rBV	1027616	1692997	44.84%	3.808%
13	10.834	1311	1317	1329	rBV	755862	1283608	33.99%	2.887%
14	10.934	1333	1334	1343	rVB7	2244	4128	0.11%	0.009%
15	12.287	1558	1564	1572	rVB2	15941	28008	0.74%	0.063%
16	13.945	1837	1846	1861	rBV	1737851	2308899	61.15%	5.194%
17	14.228	1887	1894	1906	rBV2	1901015	2707475	71.70%	6.090%
18	14.534	1939	1946	1957	rVB	1494177	2126819	56.33%	4.784%
19	14.734	1974	1980	1999	rBV	699010	1023286	27.10%	2.302%
20	14.939	2012	2015	2021	rVB8	2627	4229	0.11%	0.010%
21	15.528	2108	2115	2127	rBV	2355320	3340828	88.48%	7.515%
22	15.645	2129	2135	2149	rVV	664512	862916	22.85%	1.941%
23	15.763	2151	2155	2160	rVB2	10796	16426	0.44%	0.037%
24	17.280	2407	2413	2423	rBV	1778612	2410938	63.85%	5.423%
25	17.380	2423	2430	2446	rVV	2544144	3545812	93.90%	7.976%
26	17.939	2522	2525	2529	rBV5	3230	4165	0.11%	0.009%
27	19.239	2741	2746	2750	rBV3	26285	38832	1.03%	0.087%
28	19.310	2754	2758	2763	rVV2	24096	34460	0.91%	0.078%
29	19.674	2814	2820	2832	rBV	2815654	3775959	100.00%	8.494%
30	21.474	3121	3126	3131	rBV	1845815	2242357	59.39%	5.044%
31	23.733	3503	3510	3524	rVB2	1742392	3440235	91.11%	7.739%
32	23.892	3531	3537	3549	rVB2	1047693	2032595	53.83%	4.572%




Sum of corrected areas: 44454647

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012523\
Data File : BN023791.D
Acq On : 25 Jan 2023 12:39
Operator : CG/JU
Sample : PB150438BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK438

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

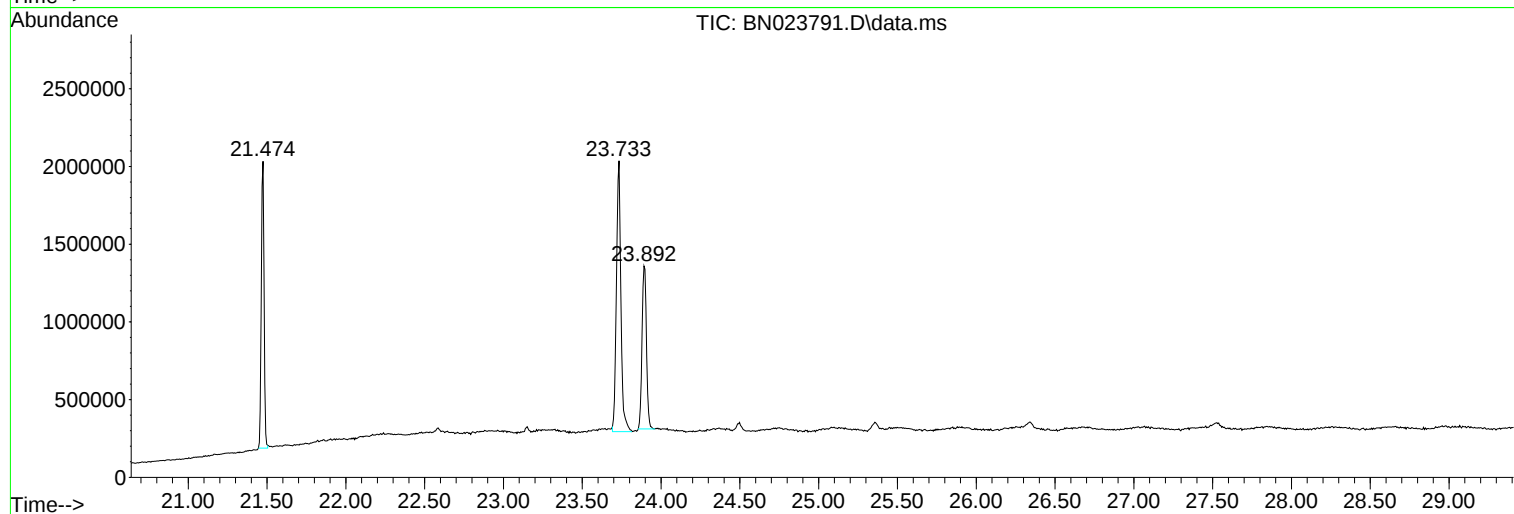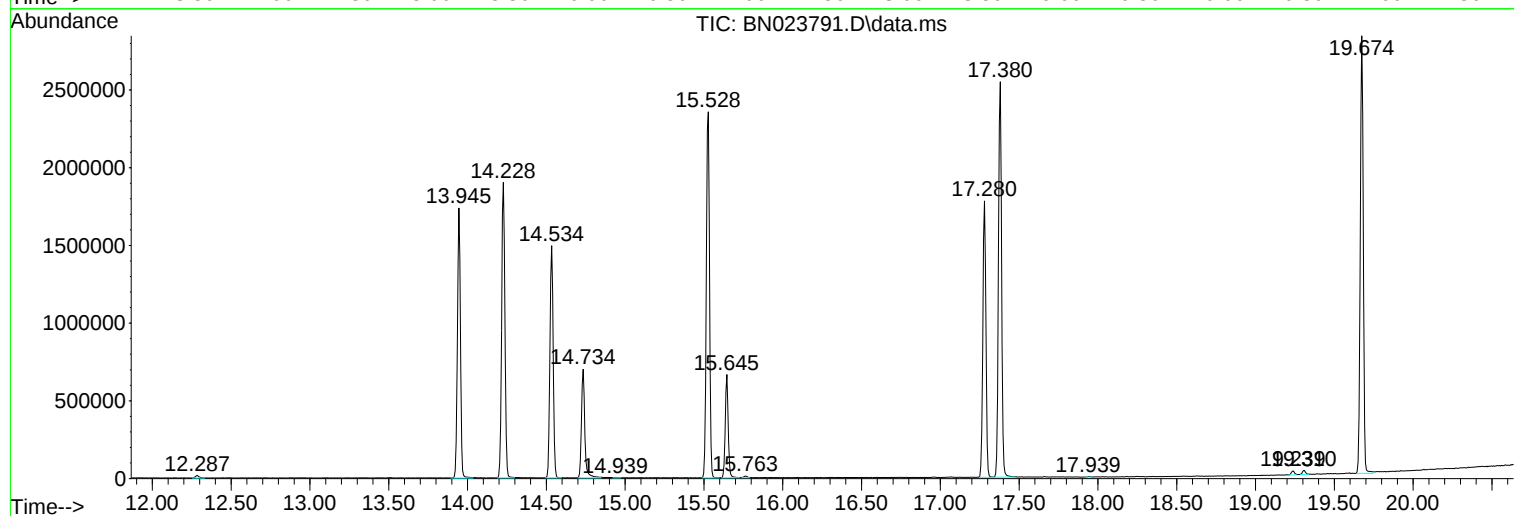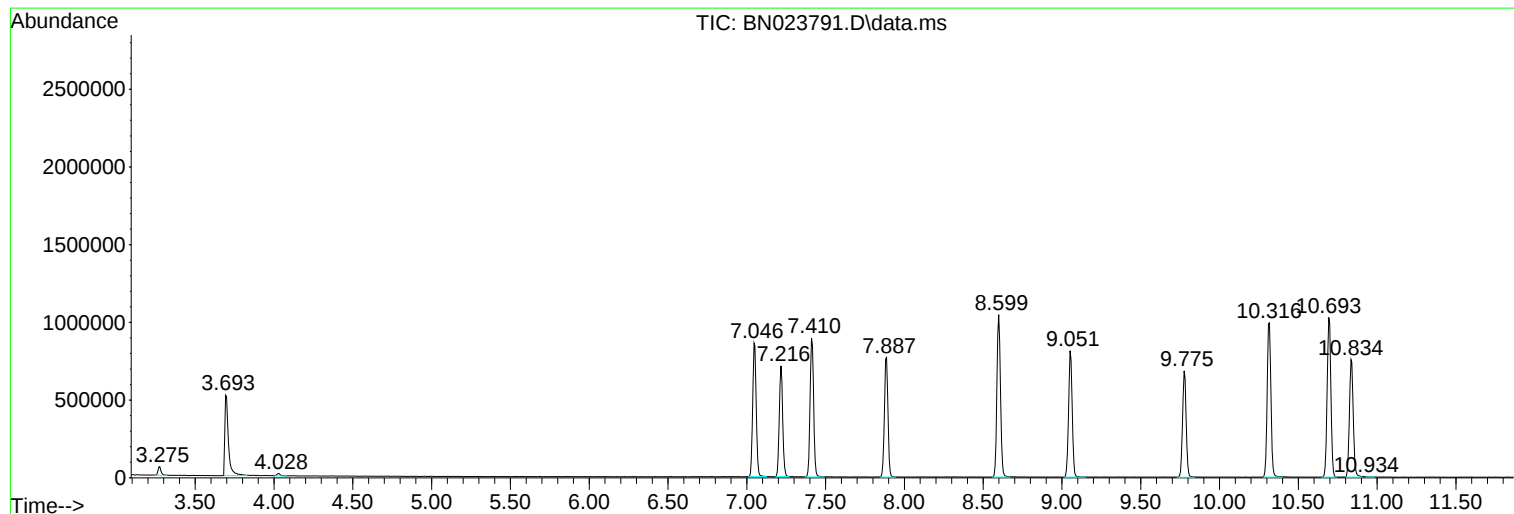

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012523\
Data File : BN023791.D
Acq On : 25 Jan 2023 12:39
Operator : CG/JU
Sample : PB150438BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK438

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012523\
Data File : BN023791.D
Acq On : 25 Jan 2023 12:39
Operator : CG/JU
Sample : PB150438BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK438

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc