
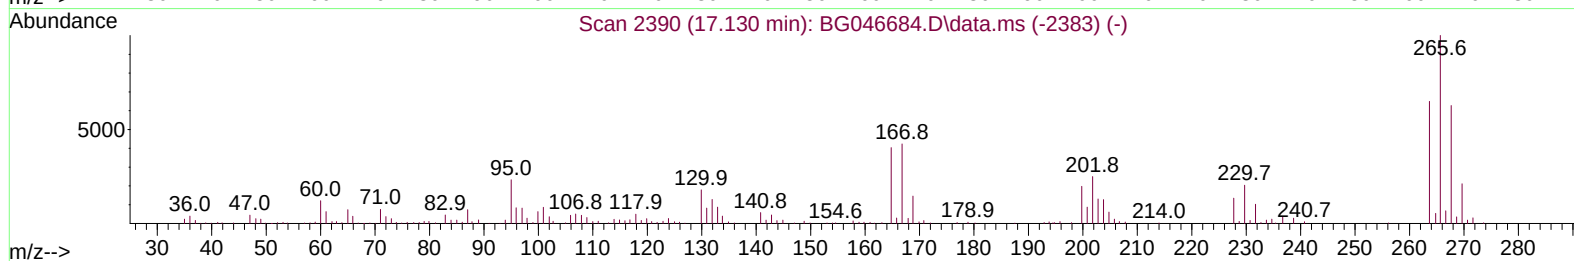
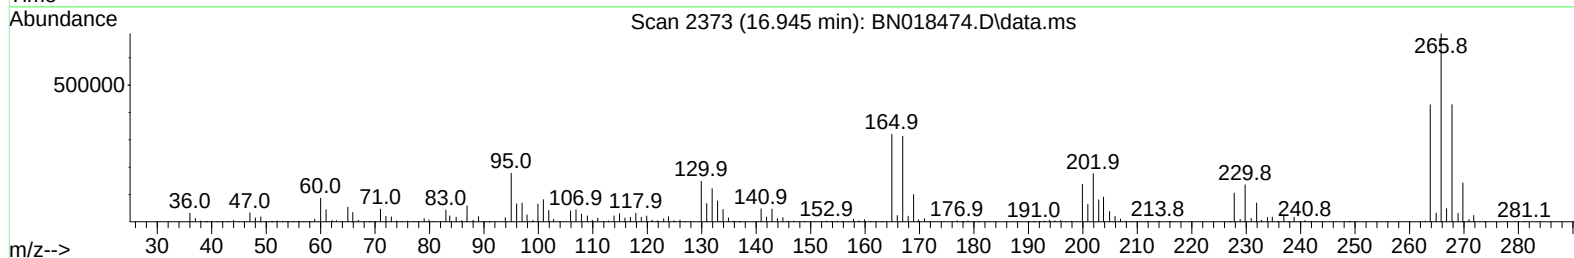


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012622\
 Data File : BN018474.D
 Acq On : 26 Jan 2022 13:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 06:24:17 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 27 06:24:13 2022
 Response via : Initial Calibration

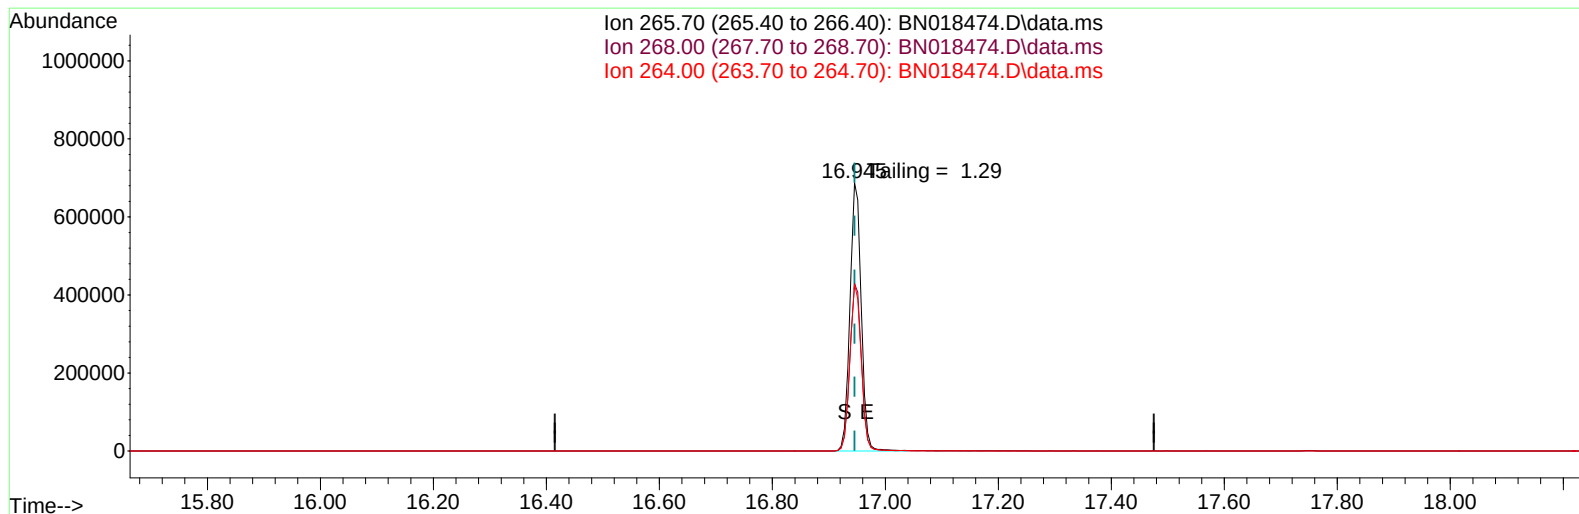

TIC: BN018474.D\data.ms

(70) Pentachlorophenol (C)




16.945min (0.000) 24750.82 ng

response 955652

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.36
264.00	61.60	62.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN012622\
Data File : BN018474.D
Acq On : 26 Jan 2022 13:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 27 06:24:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 27 06:24:13 2022
Response via : Initial Calibration

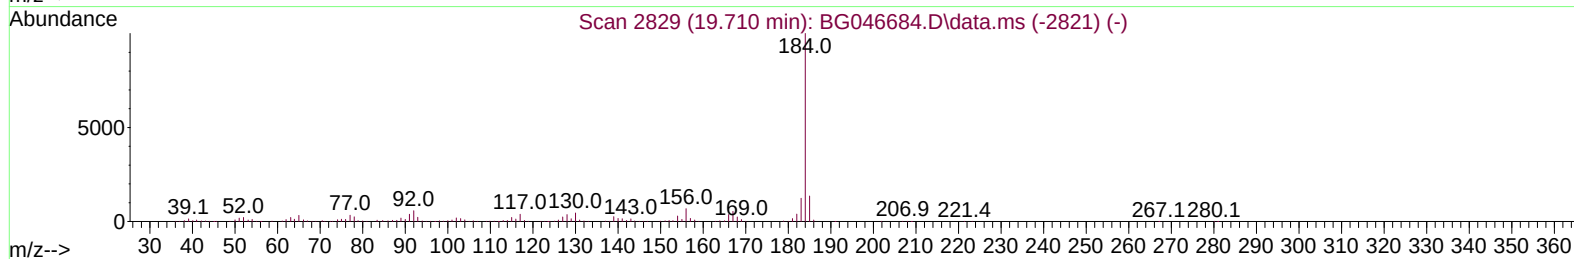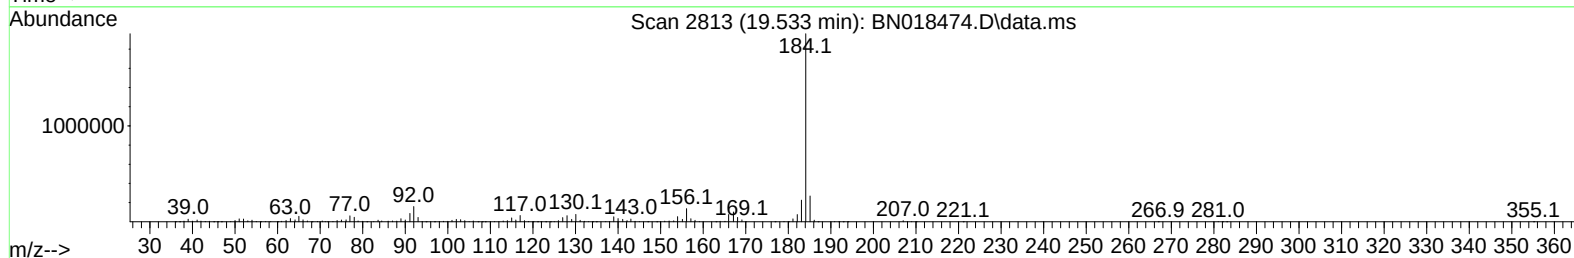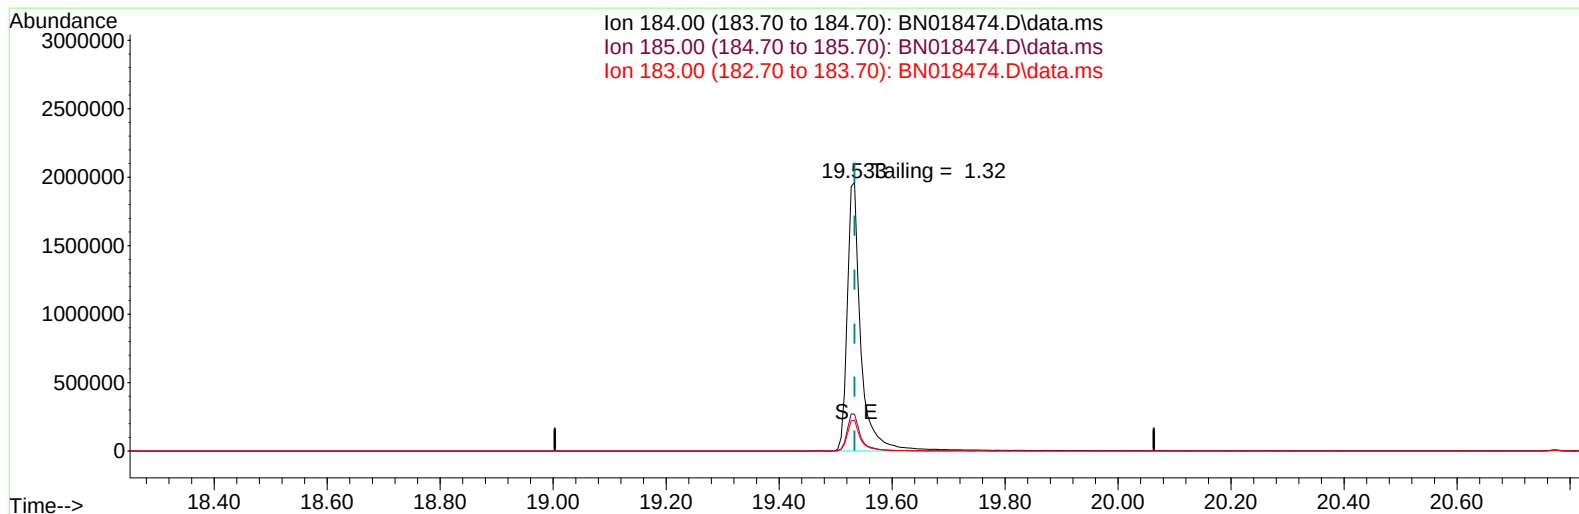

TIC: BN018474.D\data.ms

(77) Benzdine

19.533min (0.000) 0.00 ng

response 3284574

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.75
183.00	13.20	11.53
0.00	0.00	0.00