




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013023\
 Data File : BN023850.D
 Acq On : 30 Jan 2023 18:06
 Operator : CG/JU
 Sample : SSTD3.275
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD3.2235

Manual IntegrationsAPPROVED

Quant Time: Jan 31 01:46:50 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 31 01:40:05 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/31/2023
 Supervised By :Yogesh Patel 01/31/2023

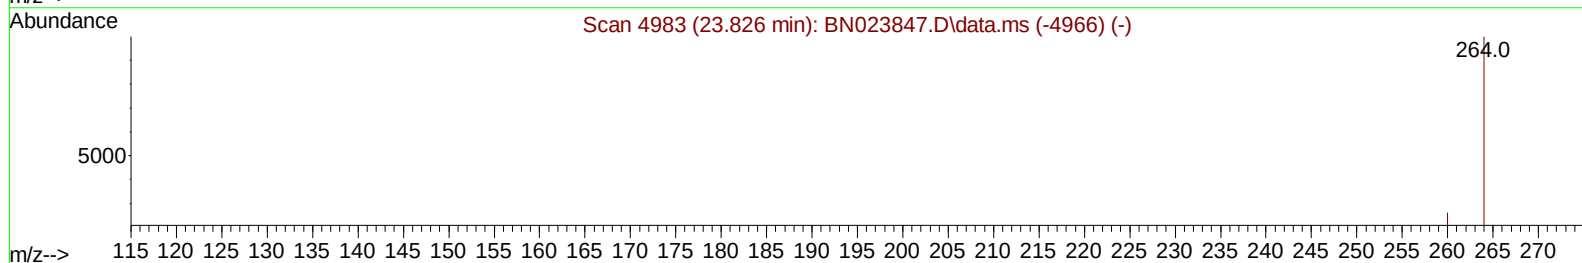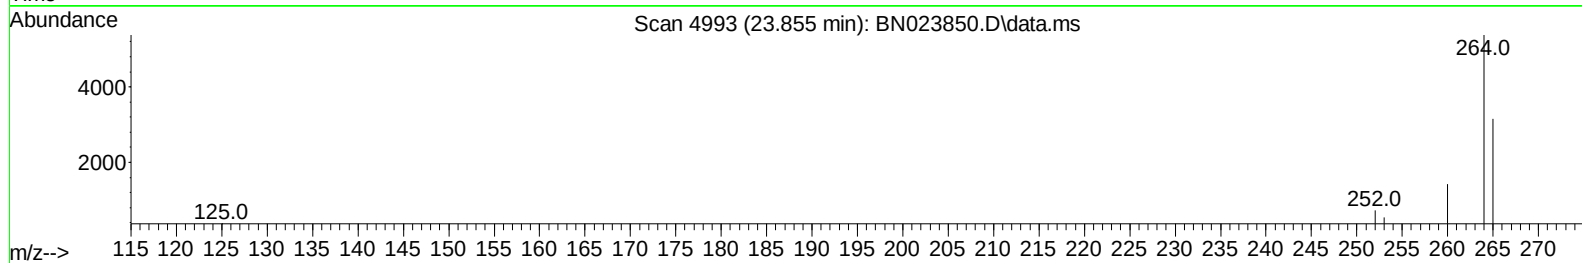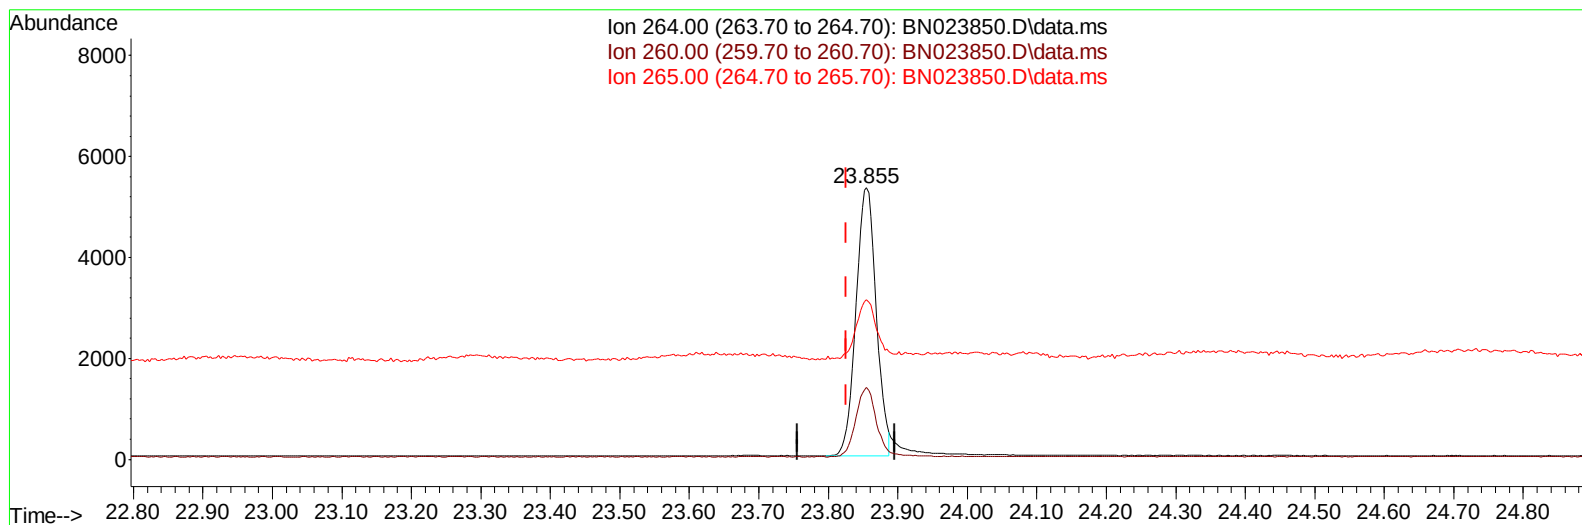

TIC: BN023850.D\data.ms

(23) Perylene-d12 (I)

23.855min (+ 0.029) 0.40 ng/ul

response 10737

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	26.56
265.00	54.60	58.71
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013023\
 Data File : BN023850.D
 Acq On : 30 Jan 2023 18:06
 Operator : CG/JU
 Sample : SST3.275
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SST3.2235

Manual IntegrationsAPPROVED

Quant Time: Jan 31 01:46:50 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 31 01:40:05 2023
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/31/2023
 Supervised By :Yogesh Patel 01/31/2023

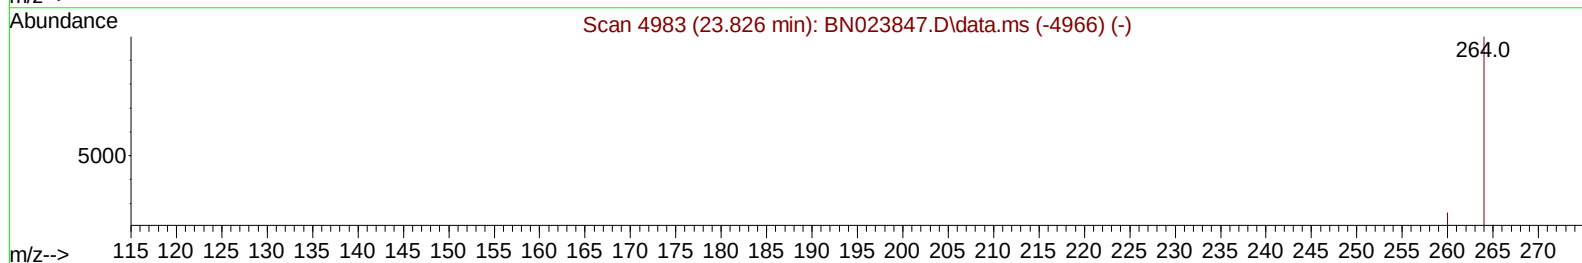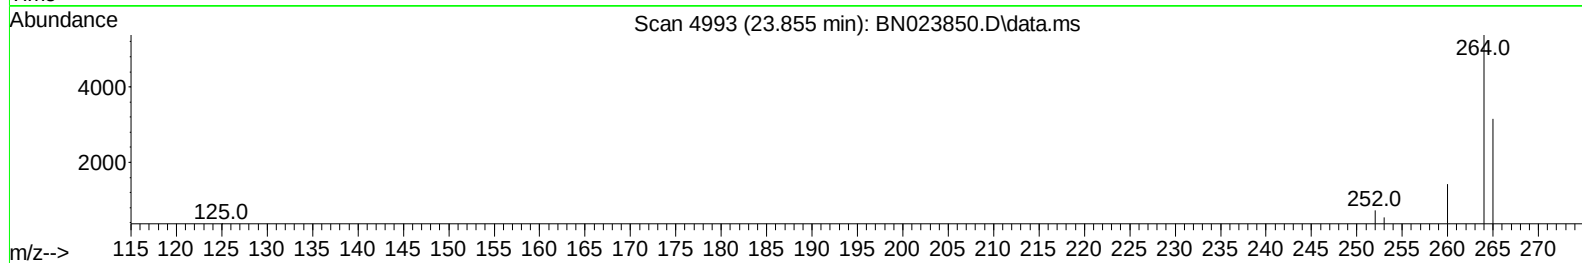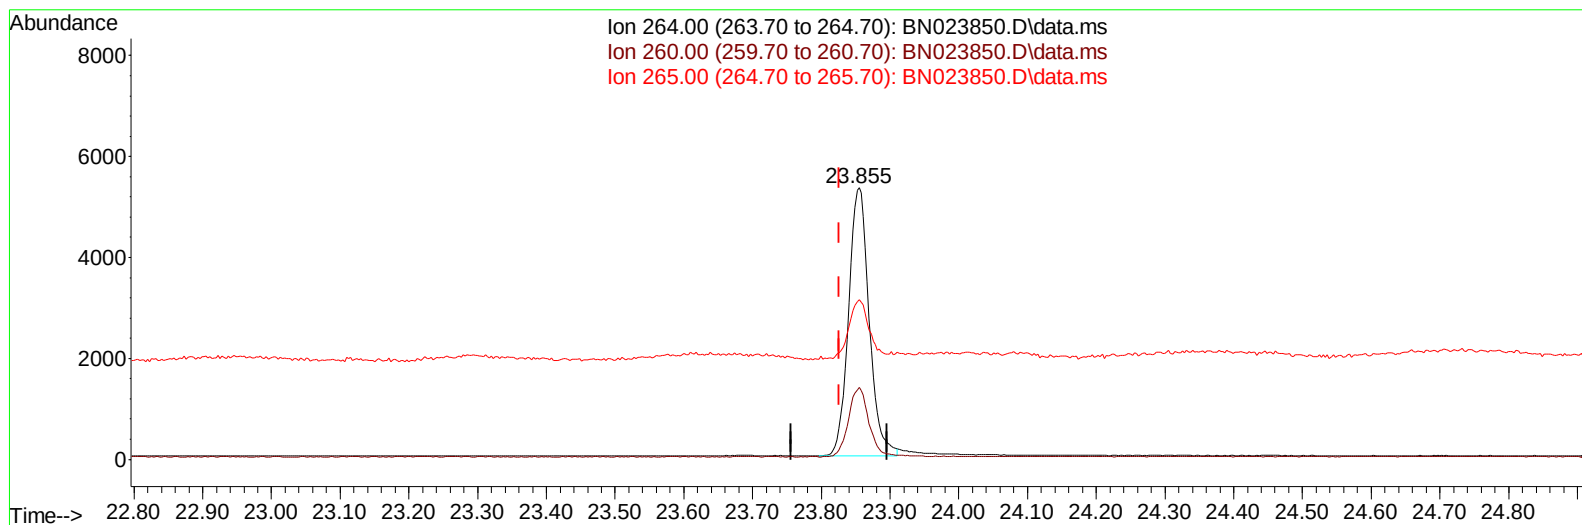

TIC: BN023850.D\data.ms

(23) Perylene-d12 (I)

23.855min (+ 0.029) 0.40 ng/ul m

response 11083

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	26.56
265.00	54.60	58.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013023\
 Data File : BN023850.D
 Acq On : 30 Jan 2023 18:06
 Operator : CG/JU
 Sample : SSTD3.275
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTD3.2235

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 01/31/2023
 Supervised By :Yogesh Patel 01/31/2023

Quant Time: Jan 31 01:46:50 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 31 01:40:05 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.863	152		2747	0.400	ng/ul	0.00
4) Naphthalene-d8	10.667	136		7362	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.511	164		4723	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.255	188		10860	0.400	ng/ul	0.00
17) Chrysene-d12	21.449	240		12738	0.400	ng/ul	0.00
23) Perylene-d12	23.855	264		11083m	0.400	ng/ul	0.03
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.243	96		9890	3.252	ng/ul	0.00
6) 2-Methylnaphthalene-d10	0.000	152		0d	0.000	ng/ul	
18) Fluoranthene-d10	0.000	212		0d	0.000	ng/ul	
Target Compounds							Qvalue
2) 1,4-Dioxane	3.281	88		10516	3.297	ng/ul#	81
14) Pentachlorophenol	16.909	266		13570	3.874	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN013023\
Data File : BN023850.D
Acq On : 30 Jan 2023 18:06
Operator : CG/JU
Sample : SSTD3.275
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTD3.2235

Manual IntegrationsAPPROVED

Quant Time: Jan 31 01:46:50 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 31 01:40:05 2023
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 01/31/2023
Supervised By :Yogesh Patel 01/31/2023

