

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020122\
 Data File : BN018509.D
 Acq On : 01 Feb 2022 12:08
 Operator : CG/JU
 Sample : N1318-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 P031-TW001-A-02

Quant Time: Feb 02 04:43:11 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 01 03:59:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.931	152	461	0.400	ng/ul	0.00
4) Naphthalene-d8	10.733	136	1663	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.558	164	976	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.294	188	1993	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.470	240	1537	0.400	ng/ul	# 0.00
23) Perylene-d12	23.867	264	1595	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	2779	5.234	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.323	152	910	0.406	ng/ul	0.00
18) Fluoranthene-d10	19.319	212	2201	0.513	ng/ul	0.00
Target Compounds						
					Qvalue	
15) Phenanthrene	17.336	178	243	0.038	ng/ul#	58
19) Fluoranthene	19.351	202	125	0.021	ng/ul#	7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020122\
Data File : BN018509.D
Acq On : 01 Feb 2022 12:08
Operator : CG/JU
Sample : N1318-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
P031-TW001-A-02

Quant Time: Feb 02 04:43:11 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 01 03:59:58 2022
Response via : Initial Calibration




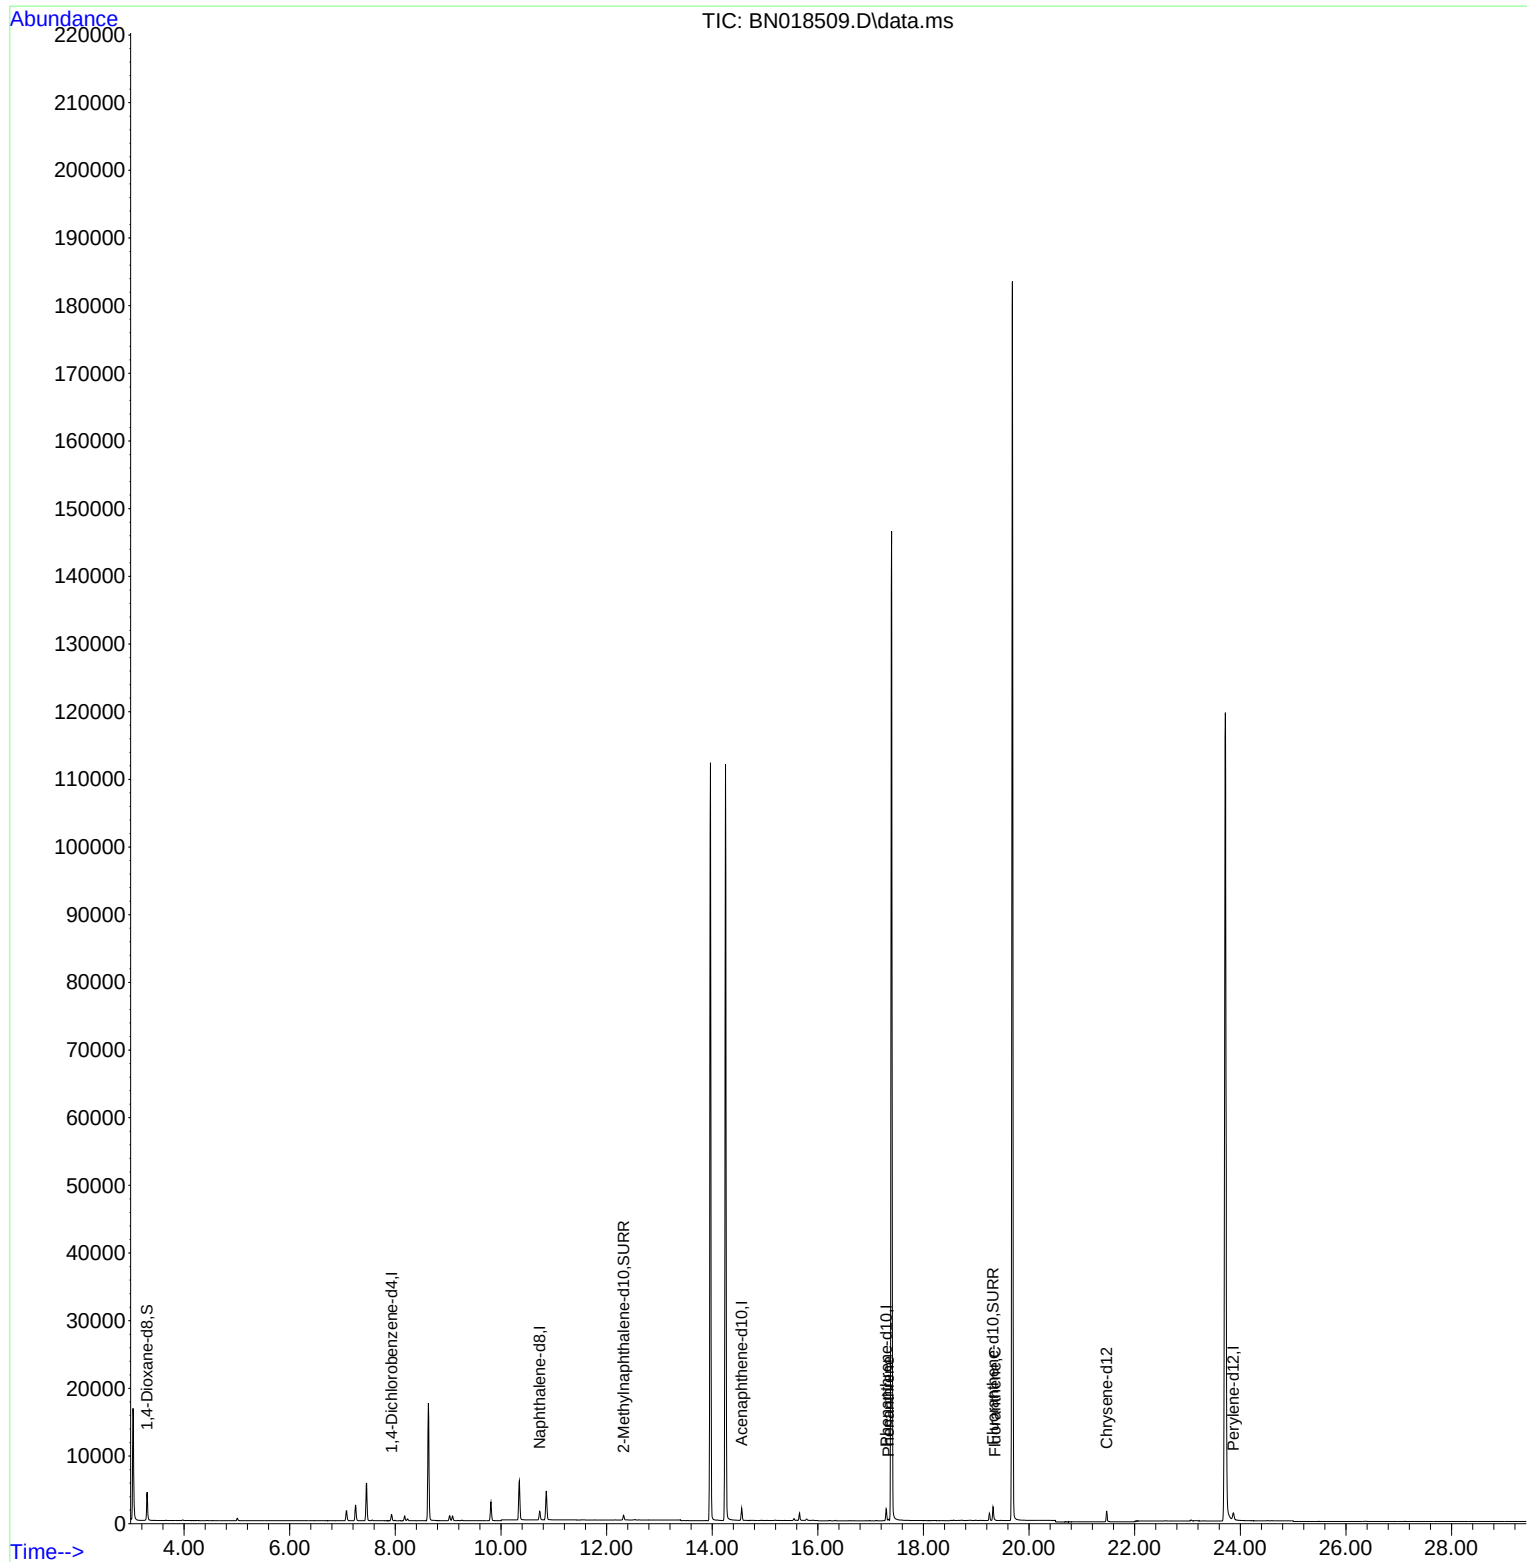


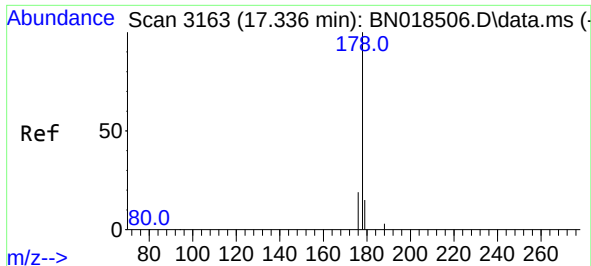

#15
Phenanthrene
Concen: 0.038 ng/ul
RT: 17.336 min Scan# 3163
Delta R.T. -0.005 min
Lab File: BN018509.D
Acq: 01 Feb 2022 12:08

Instrument :
BNA_N
ClientSampleId :
P031-TW001-A-02

Tgt Ion:178 Resp: 243
Ion Ratio Lower Upper
178 100
179 35.1 12.2 18.4#
176 36.4 15.4 23.2#

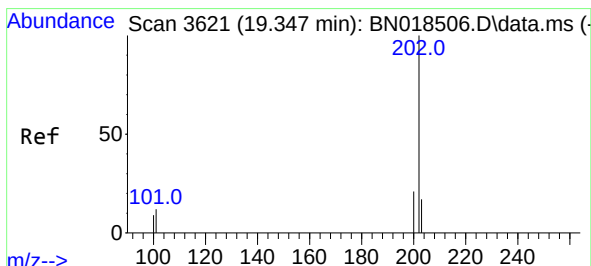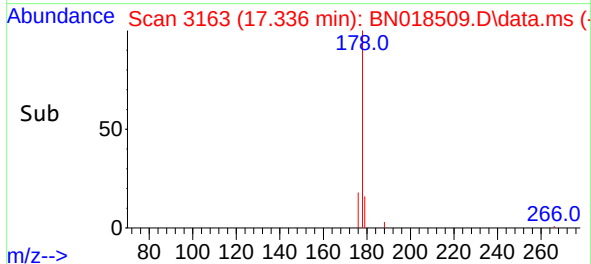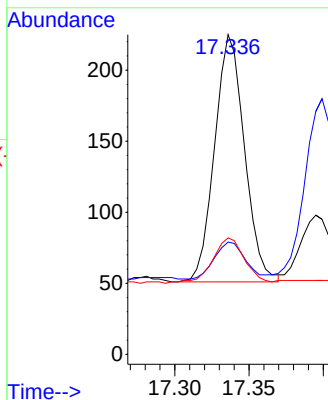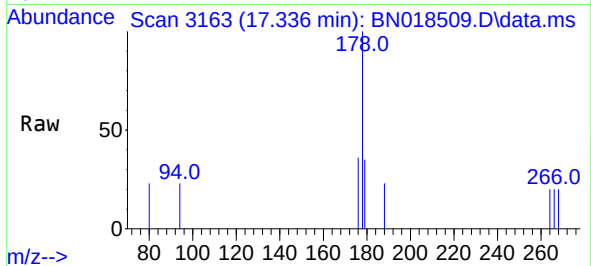

#19
Fluoranthene
Concen: 0.021 ng/ul
RT: 19.351 min Scan# 3622
Delta R.T. -0.001 min
Lab File: BN018509.D
Acq: 01 Feb 2022 12:08

Tgt Ion:202 Resp: 125
Ion Ratio Lower Upper
202 100
101 42.6 7.5 11.3#
100 39.7 5.4 8.2#

