

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020122\
 Data File : BN018510.D
 Acq On : 01 Feb 2022 12:43
 Operator : CG/JU
 Sample : N1318-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 P031-TW001-B-01

Quant Time: Feb 02 04:43:25 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 01 03:59:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.927	152	385	0.400	ng/ul	0.00
4) Naphthalene-d8	10.733	136	1394	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.558	164	801	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.294	188	1625	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.468	240	1287	0.400	ng/ul	# 0.00
23) Perylene-d12	23.867	264	1303	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.295	96	2161	4.873	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.323	152	687	0.365	ng/ul	0.00
18) Fluoranthene-d10	19.319	212	1670	0.465	ng/ul	0.00
Target Compounds						
15) Phenanthrene	17.336	178	161	0.031	ng/ul#	Qvalue 40


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020122\
Data File : BN018510.D
Acq On : 01 Feb 2022 12:43
Operator : CG/JU
Sample : N1318-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
P031-TW001-B-01

Quant Time: Feb 02 04:43:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 01 03:59:58 2022
Response via : Initial Calibration

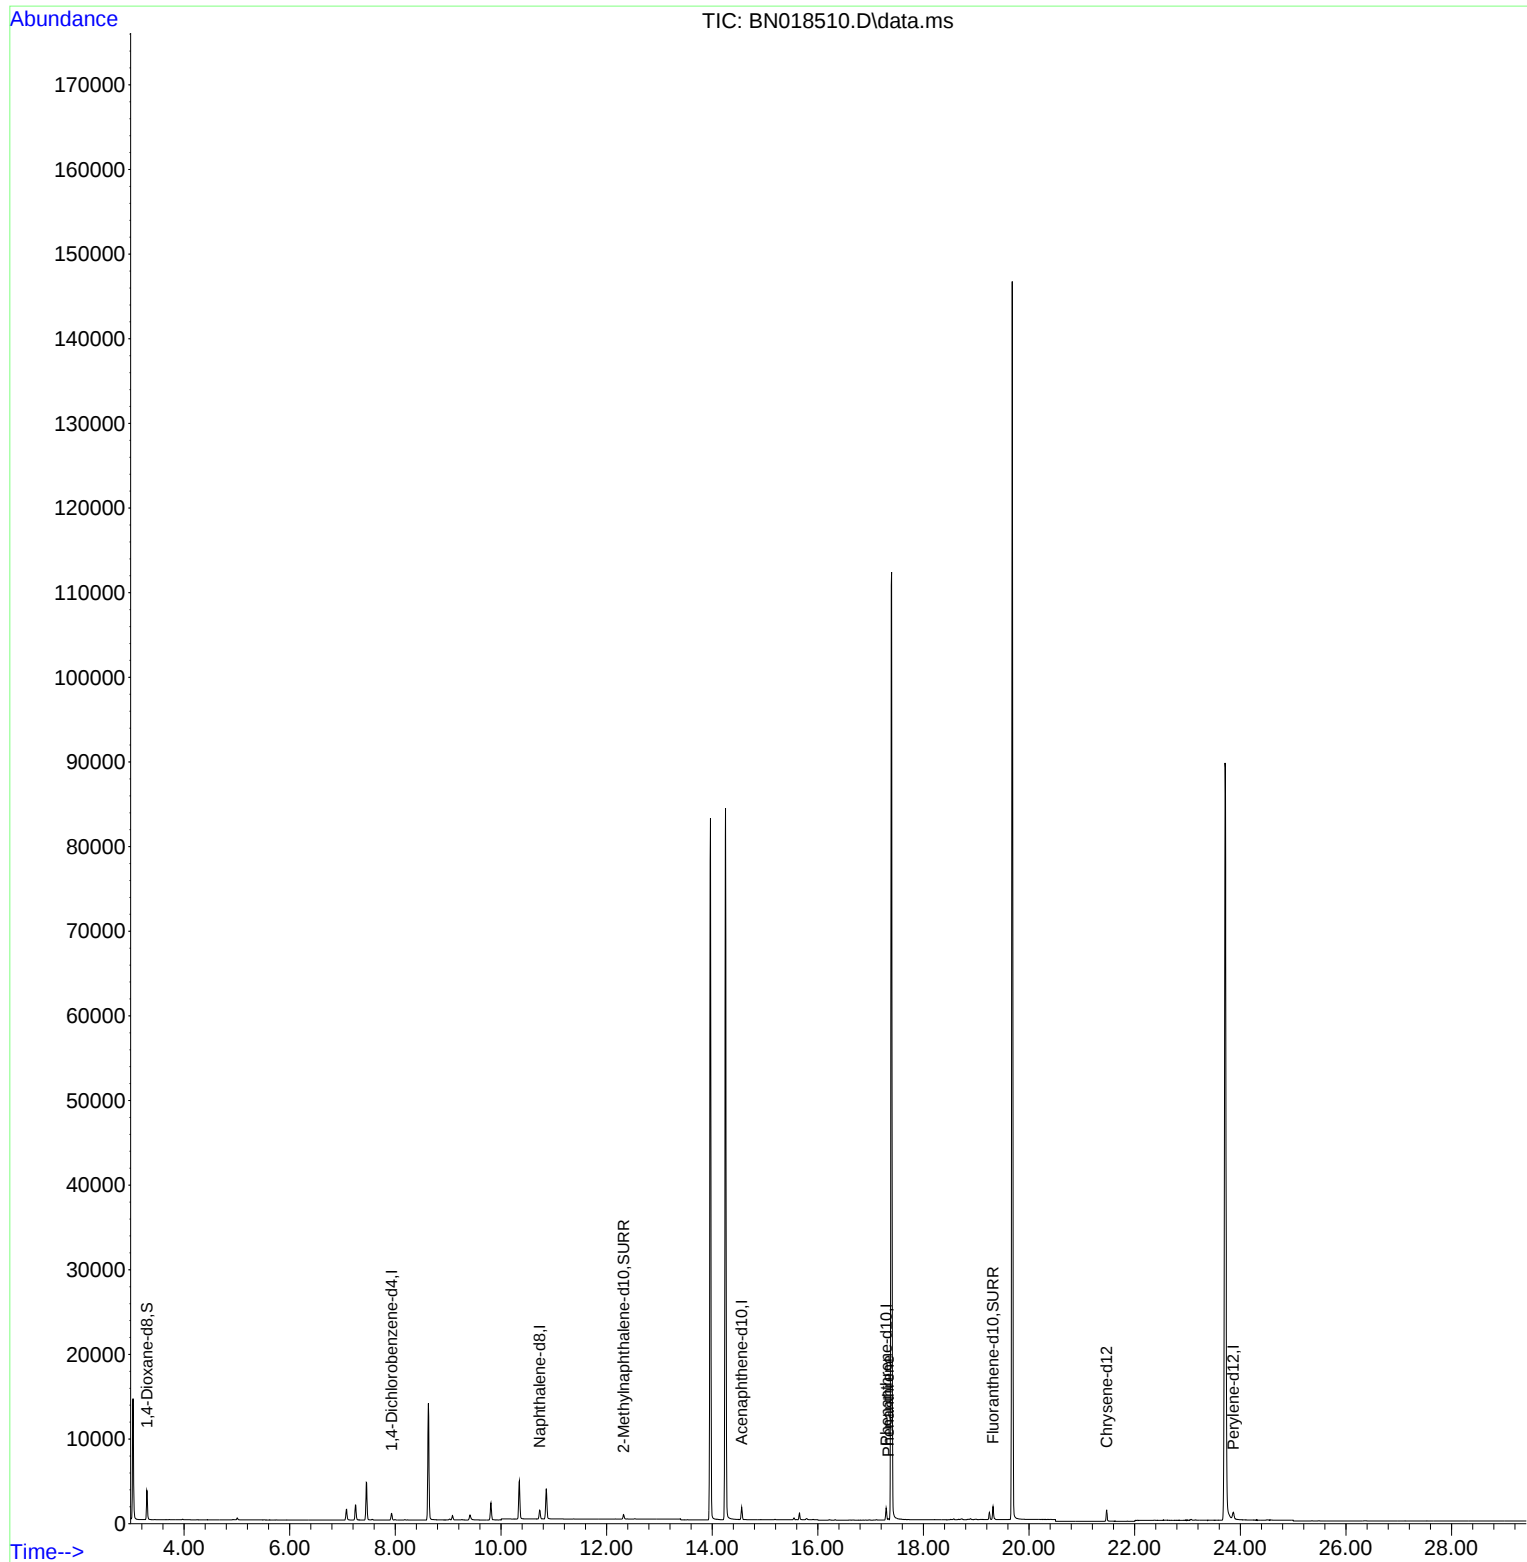

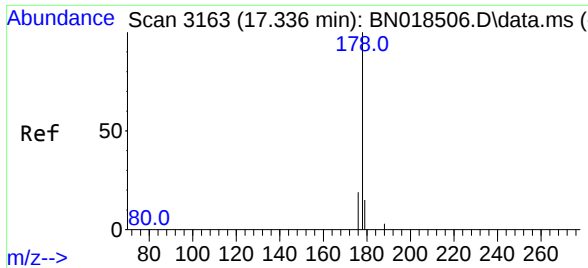

#15
 Phenanthrene
 Concen: 0.031 ng/ul
 RT: 17.336 min Scan# 31
 Delta R.T. -0.005 min
 Lab File: BN018510.D
 Acq: 01 Feb 2022 12:43

Instrument :
 BNA_N
 ClientSampleId :
 P031-TW001-B-01

Tgt Ion:	178	Resp:	161
Ion	Ratio	Lower	Upper
178	100		
179	43.9	12.2	18.4#
176	43.9	15.4	23.2#

