

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020122\
 Data File : BN018515.D
 Acq On : 01 Feb 2022 15:41
 Operator : CG/JU
 Sample : N1307-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0Q04

Quant Time: Feb 02 04:44:36 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 01 03:59:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.927	152	403	0.400	ng/ul	0.00
4) Naphthalene-d8	10.735	136	1390	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.560	164	821	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.295	188	1642	0.400	ng/ul #	0.00
17) Chrysene-d12	21.469	240	1365	0.400	ng/ul #	0.00
23) Perylene-d12	23.866	264	1429	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.295	96	1996	4.300	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.324	152	703	0.375	ng/ul	0.00
18) Fluoranthene-d10	19.320	212	1877	0.492	ng/ul	0.00
Target Compounds						Qvalue
12) Fluorene	15.600	166	62	0.020	ng/ul#	83
14) Pentachlorophenol	16.944	266	12409	85.043	ng/ul	99
15) Phenanthrene	17.337	178	156	0.029	ng/ul#	36
19) Fluoranthene	19.348	202	181	0.034	ng/ul#	22


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020122\
Data File : BN018515.D
Acq On : 01 Feb 2022 15:41
Operator : CG/JU
Sample : N1307-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0Q04

Quant Time: Feb 02 04:44:36 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 01 03:59:58 2022
Response via : Initial Calibration




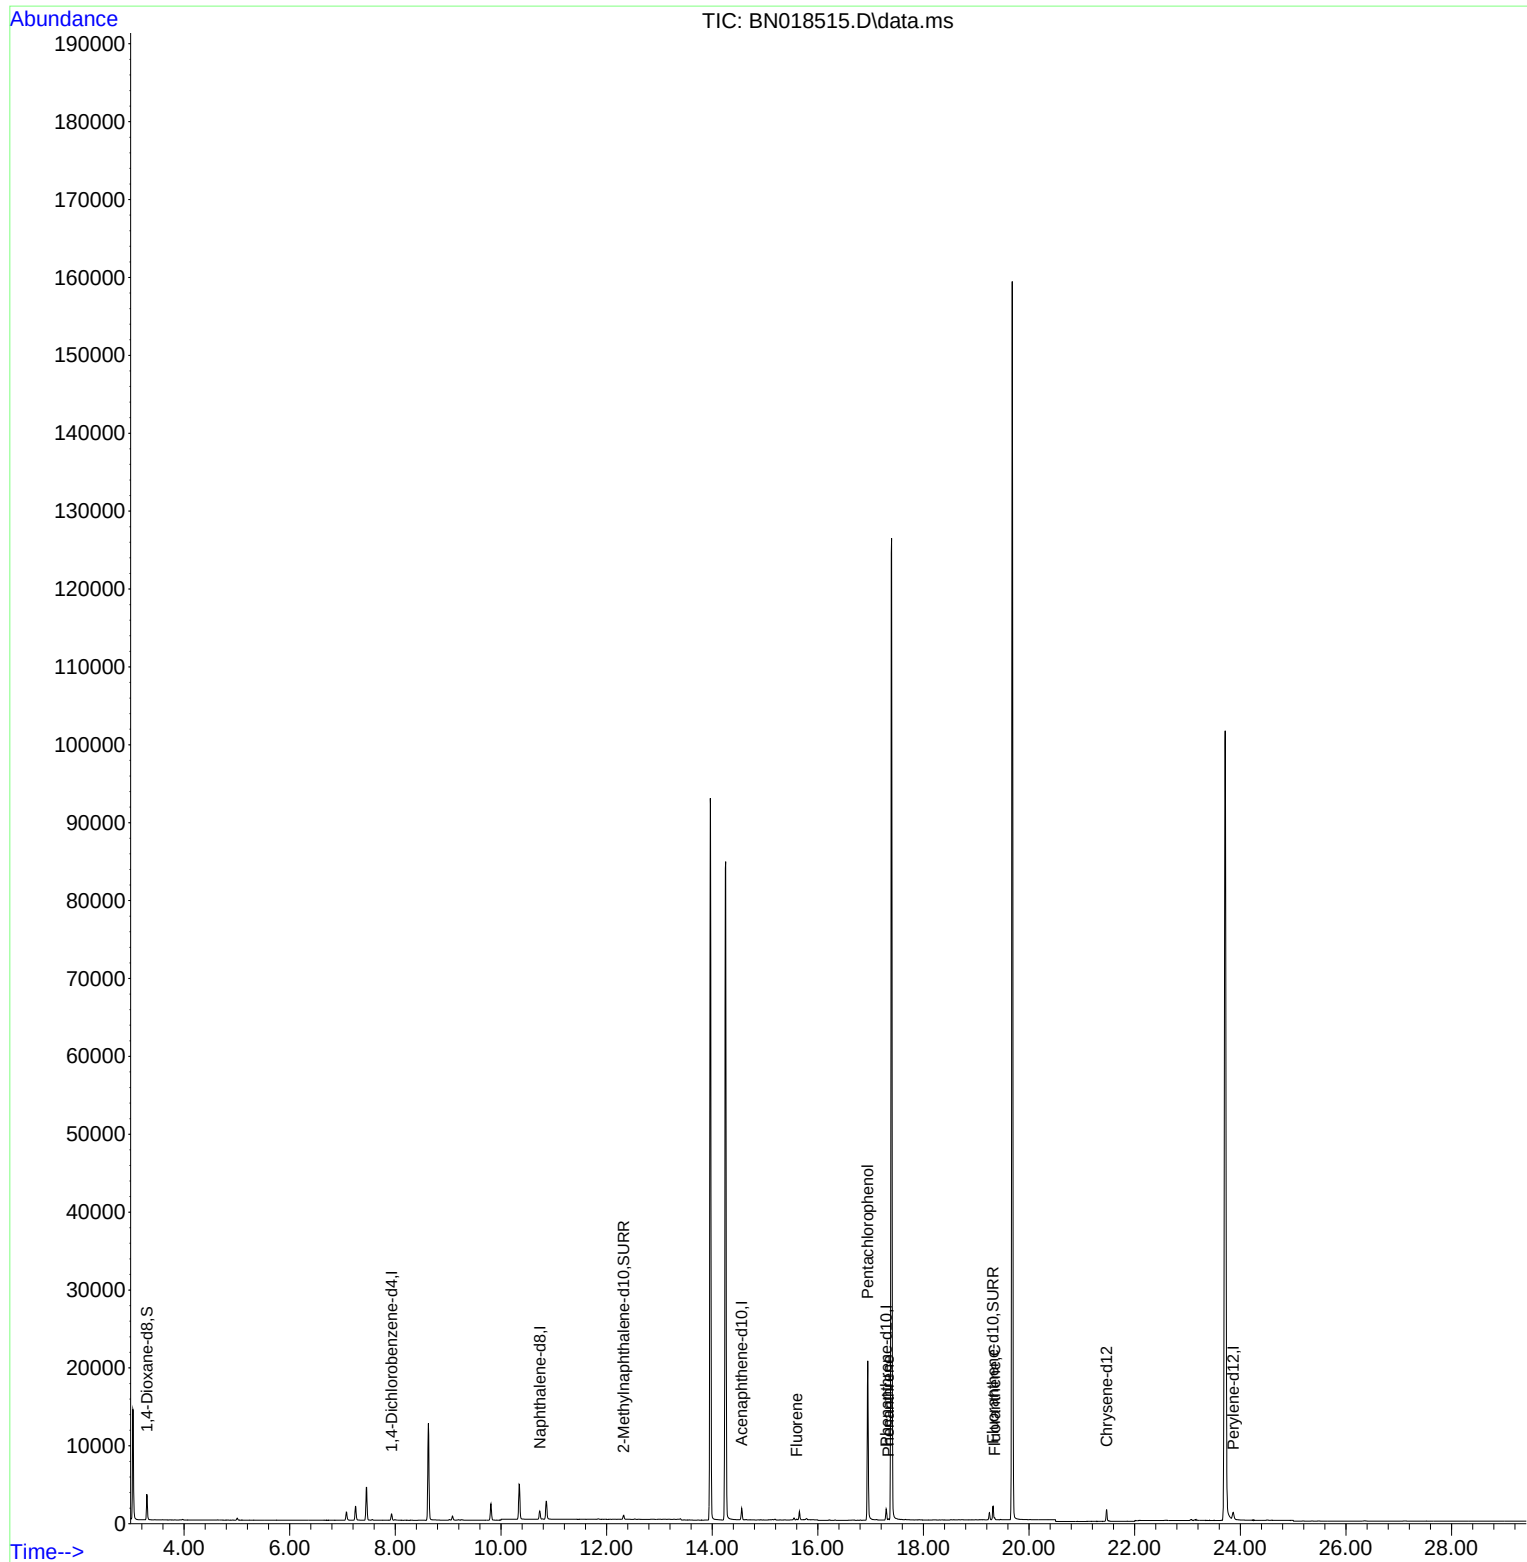


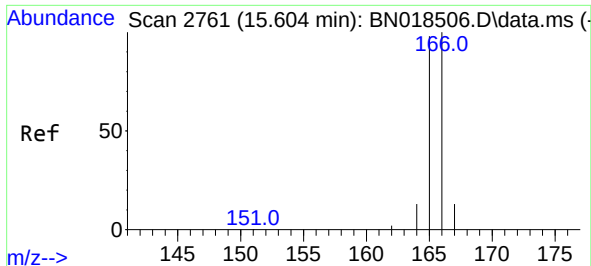

#12
Fluorene
Concen: 0.020 ng/ul
RT: 15.600 min Scan# 21
Delta R.T. -0.005 min
Lab File: BN018515.D
Acq: 01 Feb 2022 15:41




Instrument :
BNA_N
ClientSampleId :
C0Q04


Tgt Ion:166 Resp: 62
Ion Ratio Lower Upper
166 100
165 100.0 77.8 116.6
167 61.7 11.6 17.4#

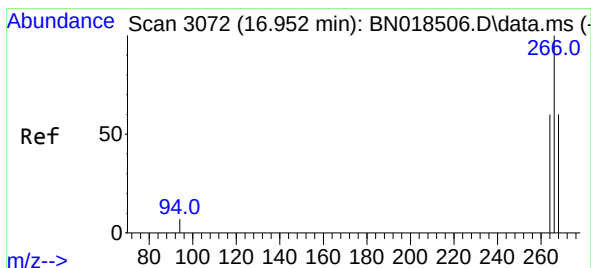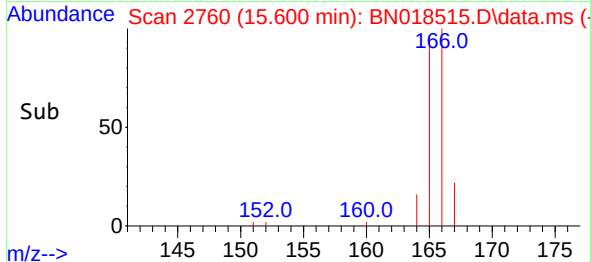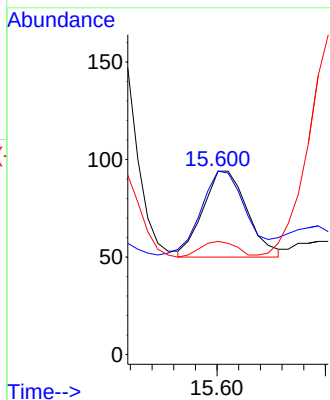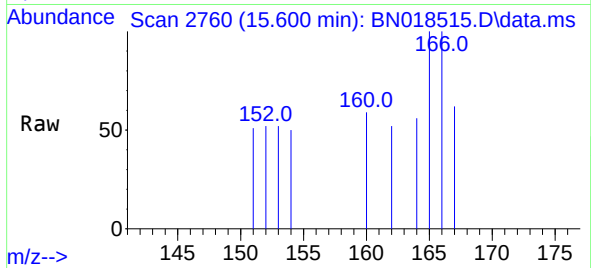

#14
Pentachlorophenol
Concen: 85.043 ng/ul
RT: 16.944 min Scan# 3070
Delta R.T. -0.004 min
Lab File: BN018515.D
Acq: 01 Feb 2022 15:41

Tgt Ion:266 Resp: 12409
Ion Ratio Lower Upper
266 100
264 63.0 49.9 74.9
268 63.9 51.7 77.5


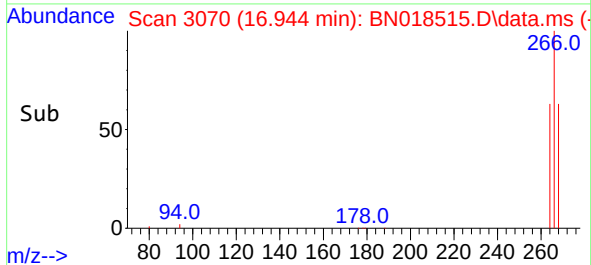
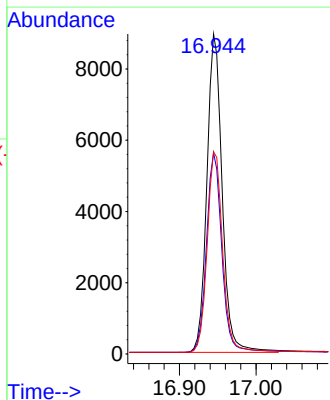
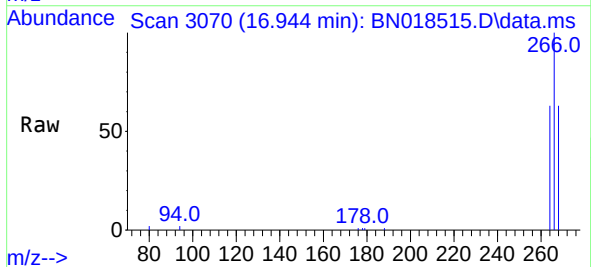


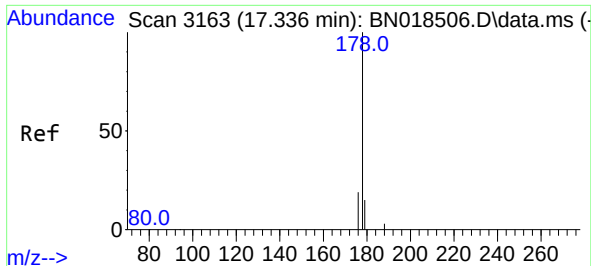

#15
Phenanthrene
Concen: 0.029 ng/ul
RT: 17.337 min Scan# 3163
Delta R.T. -0.004 min
Lab File: BN018515.D
Acq: 01 Feb 2022 15:41

Instrument :
BNA_N
ClientSampleId :
C0Q04

Tgt Ion:	178	Resp:	156
Ion	Ratio	Lower	Upper
178	100		
179	44.4	12.2	18.4#
176	46.3	15.4	23.2#

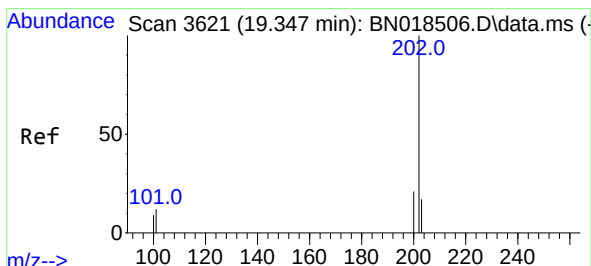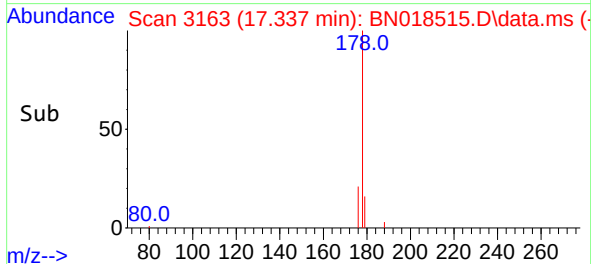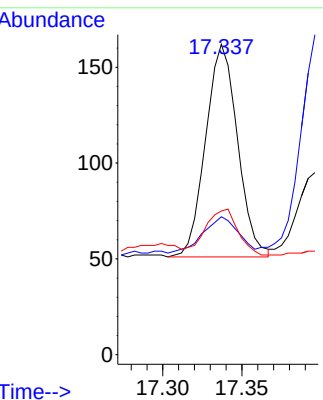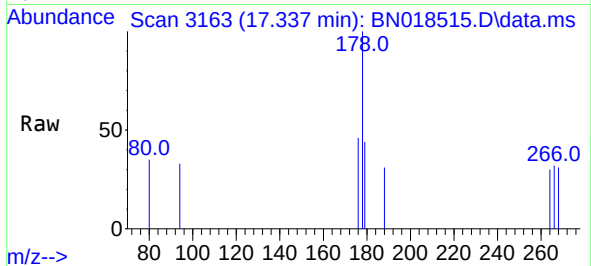

#19
Fluoranthene
Concen: 0.034 ng/ul
RT: 19.348 min Scan# 3621
Delta R.T. -0.005 min
Lab File: BN018515.D
Acq: 01 Feb 2022 15:41

Tgt Ion:	202	Resp:	181
Ion	Ratio	Lower	Upper
202	100		
101	38.3	7.5	11.3#
100	33.0	5.4	8.2#

