

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020122\
 Data File : BN018521.D
 Acq On : 01 Feb 2022 19:14
 Operator : CG/JU
 Sample : N1307-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0Q33

Quant Time: Feb 02 04:45:47 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 01 03:59:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.927	152	480	0.400	ng/ul	0.00
4) Naphthalene-d8	10.733	136	1681	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.558	164	989	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.294	188	2016	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.468	240	1687	0.400	ng/ul	# 0.00
23) Perylene-d12	23.865	264	1706	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	2048	3.704	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.323	152	774	0.341	ng/ul	0.00
18) Fluoranthene-d10	19.319	212	1864	0.396	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	16.943	266	1408	7.859	ng/ul	Qvalue 99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN020122\
Data File : BN018521.D
Acq On : 01 Feb 2022 19:14
Operator : CG/JU
Sample : N1307-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0Q33

Quant Time: Feb 02 04:45:47 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN013122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 01 03:59:58 2022
Response via : Initial Calibration

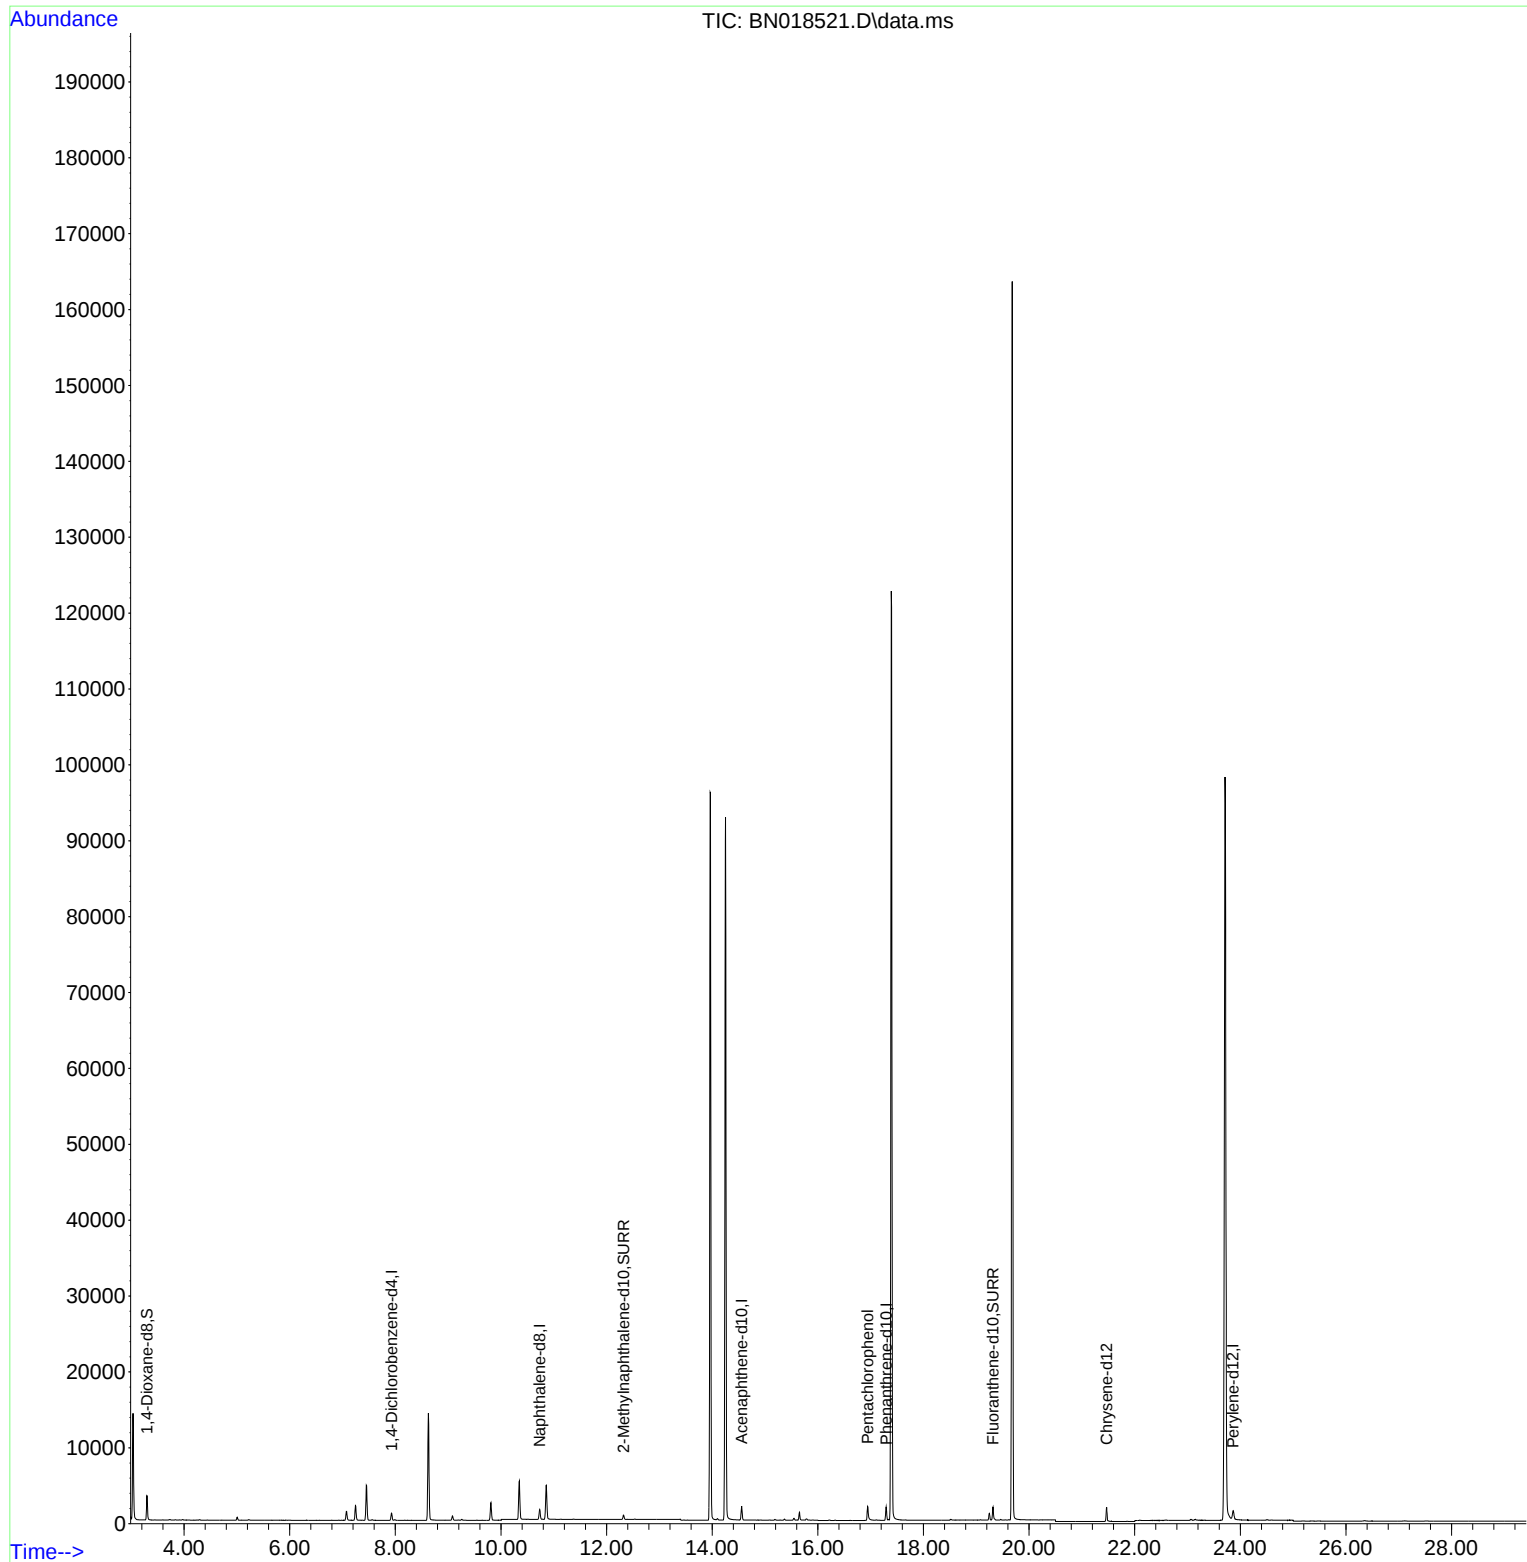

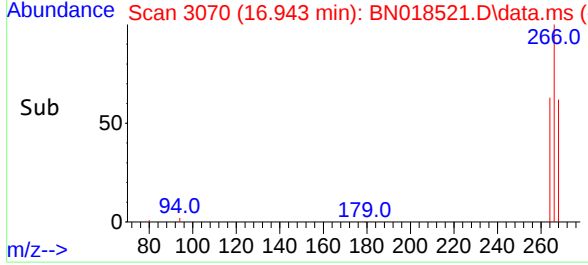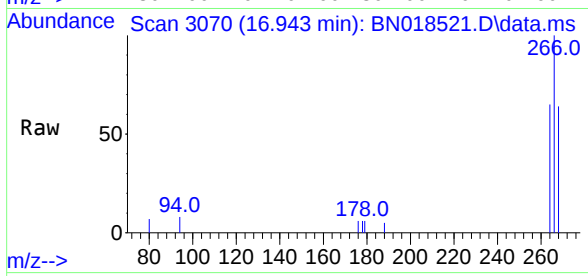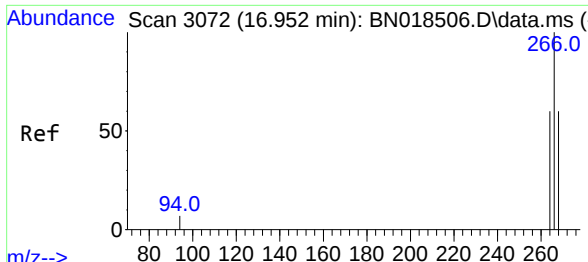

#14
Pentachlorophenol
Concen: 7.859 ng/ul
RT: 16.943 min Scan# 30
Delta R.T. -0.005 min
Lab File: BN018521.D
Acq: 01 Feb 2022 19:14

Instrument :
BNA_N
ClientSampleId :
C0Q33

Tgt Ion:	266	Resp:	1408
Ion	Ratio	Lower	Upper
266	100		
264	62.7	49.9	74.9
268	63.4	51.7	77.5

